

ÄKTA™ pure

User Manual



Table of Contents

1	Introduction	6
1.1	Important user information	7
1.2	ÄKTA pure overview	9
1.3	ÄKTA pure user documentation	11
2	The ÄKTA pure instrument	13
2.1	Overview illustrations	14
2.2	Liquid flow path	25
2.3	Instrument control panel	27
2.4	Instrument modules	32
2.4.1	System pumps	33
2.4.2	Mixer	37
2.4.3	Valves, overview	38
2.4.4	Inlet valves	39
2.4.5	Mixer valve	46
2.4.6	Injection valve	49
2.4.7	Loop valve	52
2.4.8	Column valves	55
2.4.9	Versatile valve	59
2.4.10	pH valve	60
2.4.11	Outlet valves	64
2.4.12	Pressure monitors	67
2.4.13	UV monitors	69
2.4.14	Conductivity monitor	72
2.4.15	Flow restrictor	74
2.5	Installation of internal modules	76
2.6	Accessories	79
3	ÄKTA pure external modules	86
3.1	External air sensors	87
3.2	Fraction collector F9-C	89
3.2.1	Function	90
3.2.2	Fraction collector F9-C illustrations	92
3.2.3	Cassettes, Cassette tray and racks	96
3.2.4	Connect tubing to the ÄKTA pure instrument	102
3.3	Fraction collector F9-R	103
3.4	Sample pump S9 and S9H	107
3.5	I/O-box E9	111
3.5.1	Overview of the I/O-box	112
3.5.2	Analog connector and signals	114
3.5.3	Digital connector and signals	116
3.5.4	Connect the I/O-box	118
3.6	Connection of external modules	119
4	System configuration	121
4.1	Configuration overview	122
4.2	Configure modules	128
4.2.1	Configuration of inlet valves	129
4.2.2	Configuration of Mixer valves	130
4.2.3	Configuration of Loop valves	131
4.2.4	Configuration of column valves	132

4.2.5	Configuration of Versatile valves	134
4.2.6	Configuration of pH valves	135
4.2.7	Configuration of outlet valves	136
4.2.8	Configuration of UV monitors	137
4.2.9	Configuration of Conductivity monitor	138
4.2.10	Configuration of external air sensors	139
4.2.11	Configuration of fraction collectors	140
4.2.12	Configuration of I/O-box	142
4.3	General system settings	143
5	Operation	146
5.1	Before you prepare the system	147
5.2	Prepare the flow path	148
5.3	Start UNICORN and connect to system	155
5.4	Prime inlets and purge pump heads	158
5.4.1	System pumps	159
5.4.2	Sample pump	165
5.5	Connect a column	170
5.6	Pressure alarms	174
5.7	Sample application	177
5.7.1	Sample application using direct injection onto the column	178
5.7.2	Sample application using a Superloop™	180
5.7.3	Sample application using a sample loop	187
5.8	Fractionation	190
5.8.1	Prepare Fraction collector F9-C	191
5.8.2	Prepare Fraction collector F9-R	197
5.8.3	Fractionation overview	204
5.9	Create a method and perform a run	208
5.9.1	Create a method	209
5.9.2	Prepare and perform a run	214
5.9.3	Monitor a run	216
5.9.4	After run procedures	218
6	Performance tests	221
6.1	General performance test actions	222
6.2	Air sensor A and Inlet valve A tests	225
6.3	Air sensor B and Inlet valve B tests	227
6.4	Air sensor S and Sample inlet valve tests	229
6.5	Column valve C tests	231
6.6	Fraction collector F9-C test	233
6.7	Fraction Collector F9-R Test	236
6.8	Sample pump tests	238
6.9	System Test UV U9-L (fixed)	240
6.10	System Test UV U9-M (variable)	244
7	Maintenance	248
7.1	Maintenance Manager	249
7.2	Maintenance program	255
7.3	Weekly maintenance	258
7.3.1	Change pump rinsing solution	259
7.3.2	Replace the inline filter	263
7.3.3	Clean the Fraction collector F9-C sensors	264
7.4	Monthly maintenance	266

7.5	Semiannual maintenance	269
7.5.1	Clean the UV flow cell	270
7.5.2	Replace the pH electrode	272
7.6	Maintenance when required	273
7.6.1	Clean the instrument externally	274
7.6.2	Perform System CIP	275
7.6.3	Perform Column CIP	281
7.6.4	Clean Fraction collector F9-C	285
7.6.5	Clean Fraction collector F9-R	287
7.6.6	Storage of the pH electrode	288
7.6.7	Clean the pH electrode	290
7.6.8	Clean the pump head check valves	293
7.6.9	Wipe off excess oil from the pump head	296
7.6.10	Clean the Conductivity flow cell	297
7.7	Calibration procedures	299
7.7.1	Calibrate the pH monitor	300
7.7.2	Calibrate the pressure monitors	302
7.7.3	Calibrate the Conductivity monitor	305
7.7.4	Calibrate the UV monitors	309
7.8	Replacement procedures	313
7.8.1	Replace tubing and connectors	314
7.8.2	Replace internal tubing in Fraction collector F9-C	316
7.8.3	Replace the Mixer	319
7.8.4	Replace the O-ring inside the Mixer	320
7.8.5	Replace the UV monitor U9-M flow cell	322
7.8.6	Replace the UV monitor U9-L flow cell	325
7.8.7	Replace Flow restrictor	327
7.8.8	Replace the inlet filters	328
7.8.9	Replace the pump head check valves	329
7.8.10	Replace pump piston seals of Pump P9 or P9H	332
7.8.11	Replace pump piston seals of Pump P9-S	341
7.8.12	Replace pump pistons	348
7.8.13	Replace pump rinsing system tubing	349
8	Troubleshooting	352
8.1	Introduction to troubleshooting	353
8.2	Troubleshooting: General Checklist	355
8.3	Troubleshooting: Monitors	357
8.4	Troubleshooting: Valves	372
8.5	Troubleshooting: Fraction collector	374
8.6	Troubleshooting: Pumps	384
8.7	Troubleshooting: Other components	391
8.8	Troubleshooting: Instrument communication	398
8.9	Troubleshooting: Method development	400
8.10	Error codes	401
9	Reference information	407
9.1	System specifications	408
9.2	Module specifications	411
9.3	Tubing and connectors	419
9.4	Recommended tubing kits for prepacked columns	427
9.5	Chemical resistance guide	430
9.6	Wetted materials	434
9.7	Predefined methods and phases	436
9.7.1	Predefined purification methods	437
9.7.2	Predefined maintenance methods	443

9.7.3	Predefined phases	445
9.8	System settings	447
9.8.1	System settings - UV	448
9.8.2	System settings - Conductivity	449
9.8.3	System settings - pH	450
9.8.4	System settings - Pressure alarms	451
9.8.5	System settings - Air sensor	453
9.8.6	System settings - I/O-box	455
9.8.7	System settings - Fraction collection	456
9.8.8	System settings - Tubing and Delay volumes	458
9.8.9	System settings - Wash settings	460
9.8.10	System settings - Watch parameters	461
9.8.11	System settings - Advanced	462
9.8.12	System settings - Data collection	463
9.9	Manual instructions	464
9.9.1	Manual instructions - Pumps	465
9.9.2	Manual instructions - Flow path	469
9.9.3	Manual instructions - Monitors	471
9.9.4	Manual instructions - Fraction collection	472
9.9.5	Manual instructions - I/O-box	476
9.9.6	Manual instructions - Alarms	477
9.9.7	Manual instructions - Wash settings	480
9.9.8	Manual instructions - Watch parameters	481
9.9.9	Manual instructions - Advanced	482
9.9.10	Manual instructions - Other	485
9.10	Available Run data	486
9.11	Available Curves	489
9.12	Injection volumes and peak broadening	491
9.13	Delay volumes	492
9.14	Component volumes	497
9.15	Pressure control	499
9.16	Node IDs	501
10	Ordering information	503
	Index	511

1 Introduction

Purpose of the User Manual

The User Manual provides you with instructions and information to run the ÄKTA pure system. It also includes relevant guidance for practical handling and maintenance of instrument components.

In this chapter

This chapter contains the following sections:

Section	See page
1.1 Important user information	7
1.2 ÄKTA pure overview	9
1.3 ÄKTA pure user documentation	11

1.1 Important user information

Read this before operating ÄKTA pure



All users must read the entire *ÄKTA pure Operating Instructions* before installing, operating, or maintaining the instrument. Always keep the *ÄKTA pure Operating Instructions* at hand when operating ÄKTA pure.

Do not operate ÄKTA pure in any other way than described in the user documentation. If you do, you may be exposed to hazards that can lead to personal injury and you may cause damage to the equipment.

Intended use

ÄKTA pure is intended for purification of bio-molecules, in particular proteins, for research purposes by trained laboratory staff members in research laboratories.

ÄKTA pure shall not be used in any clinical procedures, or for diagnostic purposes.

Prerequisites

In order to operate the system according to the intended purpose, it is important that:

- you have a general understanding of how the computer and the Microsoft® Windows® operating system work.
 - you understand the concepts of liquid chromatography.
 - you have read and understood the Safety instructions chapter in *ÄKTA pure Operating Instructions*.
 - a user account has been created according to UNICORN™ Administration and Technical Manual.
-

Safety notices

This user documentation contains WARNINGS, CAUTIONS and NOTICES concerning the safe use of the product. See definitions below.

Warnings



WARNING

WARNING indicates a hazardous situation which, if not avoided, could result in death or serious injury. It is important not to proceed until all stated conditions are met and clearly understood.

Cautions



CAUTION

CAUTION indicates a hazardous situation which, if not avoided, could result in minor or moderate injury. It is important not to proceed until all stated conditions are met and clearly understood.

Notices



NOTICE

NOTICE indicates instructions that must be followed to avoid damage to the product or other equipment.

Notes and tips

Note: A Note is used to indicate information that is important for trouble-free and optimal use of the product.

Tip: A tip contains useful information that can improve or optimize your procedures.

1.2 ÄKTA pure overview

Introduction

ÄKTA pure is intended for purification of bio-molecules, in particular proteins, for research purposes by trained laboratory staff members in research laboratories.

This section gives an overview of the ÄKTA pure instrument and the UNICORN software. For detailed information about UNICORN, see the UNICORN manuals listed in [UNICORN user documentation, on page 12](#). For detailed information about the instrument, see [Chapter 2 The ÄKTA pure instrument, on page 13](#).

Main features

The main features of ÄKTA pure are listed below.

- ÄKTA pure is a flexible system that allows the user to configure both hardware and software to meet many purification needs.
 - The instrument can be easily extended with additional valves, detectors and fraction collectors.
 - There are a large number of different hardware modules to choose from. The user can adjust, for example, the number of columns, inlets, outlets and detectors and choose between different ways to apply and collect samples.
 - Purification and maintenance methods are easily created using predefined methods and method phases. A method phase refers to a specific step/part in the method, such as column wash or elution. Method phases are described in **Phase Properties** and are displayed graphically in a method outline. This makes methods and phases easy to understand and edit.
 - ÄKTA pure is controlled by the UNICORN software: a complete package for control, supervision and evaluation of chromatography instruments and purification runs.
 - UNICORN has different software licence options, such as Design of Experiments (DoE) and Column logbook, to further add user support.
-

UNICORN modules overview

UNICORN consists of four modules: **Administration**, **Method Editor**, **System Control** and **Evaluation**. The main functions of each module are described in the following table.

Module	Main functions
Administration	Perform user and system setup, system log and database administration.
Method Editor	Create and edit methods using one or a combination of: • Predefined methods with built-in application support • Drag-and-drop function to build methods with relevant steps • Line-by-line text editing The interface provides easy viewing and editing of run properties.
System Control	Start, monitor and control runs. The current flow path is illustrated in the Process Picture , which allows manual interactions with the system and provides feedback on run parameters.
Evaluation	Open results, evaluate runs and create reports. • The default Evaluation module includes a user interface optimized for workflows like quick evaluation, compare results and work with peaks and fractions. • To perform operations like Design of Experiments, users can easily switch to Evaluation Classic.

1.3 ÄKTA pure user documentation

Introduction

This section describes the user documentation that is delivered with ÄKTA pure.

User documentation

The user documentation listed in the table below is delivered with ÄKTA pure. It is also available on the user documentation CD.

Document	Main contents
ÄKTA pure Operating Instructions	Instructions needed to install, operate and maintain ÄKTA pure in a safe way.
Fraction collector F9-C and F9-R Operating Instructions	Instructions needed to install, operate and maintain Fraction collectors F9-C and F9-R in a safe way.
Sample pump S9 and S9H Operating Instructions	Instructions needed to install, operate and maintain Sample pump S9 and S9H in a safe way.
ÄKTA pure User Manual	Detailed instrument and module descriptions and instructions on how to run, maintain and troubleshoot the system.

UNICORN user documentation

The user documentation listed in the following table is available from the **Help** menu in UNICORN or by pressing the **F1** key.

Documentation	Main contents
UNICORN Help	Dialog descriptions for UNICORN (available from the Help menu).
UNICORN Method Manual	• Overview and detailed descriptions of the method creation features in UNICORN. • Workflow descriptions for common operations.
Getting started with Evaluation Note: <i>Available in UNICORN 7.0 and later.</i>	• Video clips showing common workflows in the Evaluation module. • Overview of features of the Evaluation module.
UNICORN Evaluation Manual	• Overview and detailed descriptions of the Evaluation Classic module in UNICORN. • Description of the evaluation algorithms used in UNICORN.
UNICORN Administration and Technical Manual	• Overview and detailed description of network setup and complete software installation. • Administration of UNICORN and the UNICORN database.
UNICORN System Control Manual	• Overview and detailed description of the system control features in UNICORN. • Includes general operation, system settings and instructions on how to perform a run.

Additional literature

For practical tips on chromatography, refer to *ÄKTA Laboratory-scale: Chromatography Systems Instrument Management Handbook (29-0108-31)*.

2 The ÄKTA pure instrument

About this chapter

This chapter provides an overview of the ÄKTA pure instrument. It also describes the internal instrument components and how these are installed in the instrument.

In this chapter

This chapter contains the following sections:

Section	See page
2.1 Overview illustrations	14
2.2 Liquid flow path	25
2.3 Instrument control panel	27
2.4 Instrument modules	32
2.5 Installation of internal modules	76
2.6 Accessories	79

2.1 Overview illustrations

Introduction


This section provides an overview of the system and its available modules.

Instrument configurations

ÄKTA pure is available with two core module configurations, one for flow rates up to 25 ml/min and one for flow rates up to 150 ml/min. In this manual they are referred to as ÄKTA pure 25 (25 ml/min) and ÄKTA pure 150 (150 ml/min).

Illustrations of the main parts of the instrument


The illustrations below show the location of the main parts of the instrument.

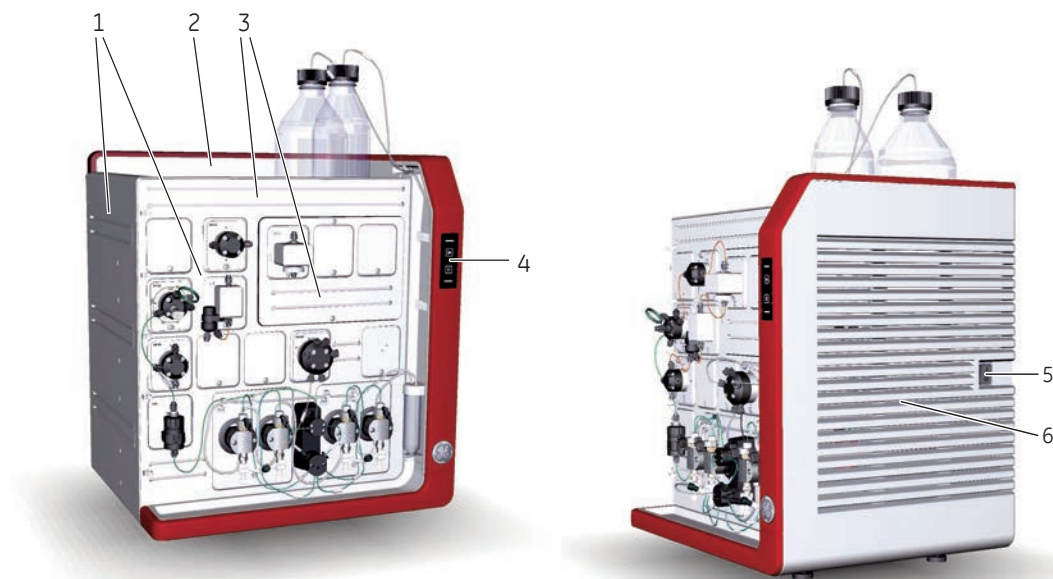

Part	Function
1	Wet sides
2	Buffer tray
3	Holder rails
4	Instrument control panel
5	Power switch
6	Ventilation panel

Example of a typical configuration of the wet side

A typical configuration of ÄKTA pure is illustrated below.

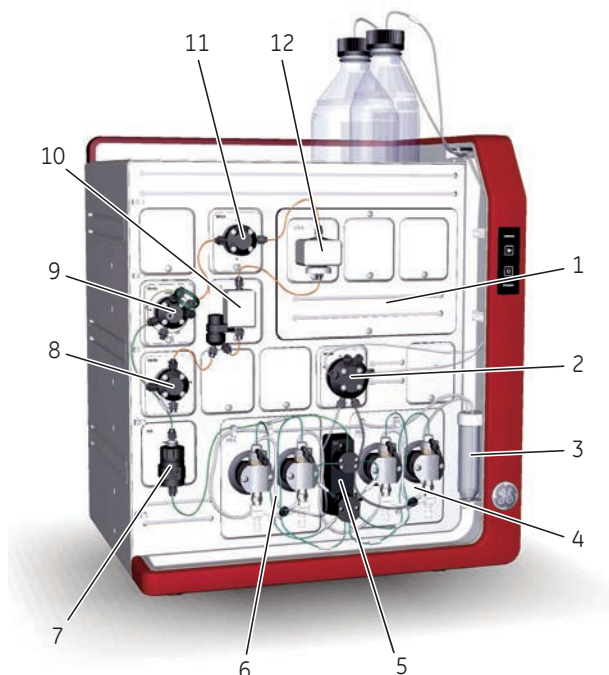

Part	Function
1	Multi-module panel
2	Inlet valve
3	Pump rinsing liquid tube
4	System pump B
5	Pressure monitor
6	System pump A
7	Mixer
8	Outlet valve
9	Injection valve
10	Conductivity monitor
11	Column valve
12	UV monitor

Available modules

The modular design allows the user to customize ÄKTA pure in multiple ways. The system is always delivered with the core modules of the selected configuration, but one or more optional modules may be added to the flow path.

The table below contains information on the core modules and the optional modules of ÄKTA pure 25 and ÄKTA pure 150. The sections that follows contain descriptions of the modules.


Note: The valves for ÄKTA pure 25 and ÄKTA pure 150 are compatible with both systems but for the best performance the specific valve type should be used. The narrow channels in the valves for ÄKTA pure 25 will give too high back pressure if used above 50 ml/min. The larger volumes in the "H" valves for ÄKTA pure 150 may decrease resolution and increase peak broadening if used in ÄKTA pure 25.

Module	Label in	
	ÄKTA pure 25	ÄKTA pure 150
System pump A	P9 A	P9H A
System pump B	P9 B	P9H B
Pressure monitor	R9	R9
Mixer	M9	M9
Injection valve	V9-Inj	V9H-Inj
Inlet valve A	V9-IA	V9H-IA
Inlet valve B	V9-IB	V9H-IB
Inlet valve AB	V9-IAB	V9H-IAB
Inlet valve IX	V9-IX	V9H-IX
Sample inlet valve	V9-IS	V9H-IS
Mixer valve	V9-M	V9H-M
Loop valve	V9-L	V9H-L
Column valves	V9-C	V9H-C
	V9-Cs	V9H-Cs
pH valve	V9-pH	V9H-pH
Outlet valves	V9-O	V9H-O
	V9-Os	V9H-Os
Versatile valve	V9-V	V9H-V

Module	Label in	
	ÄKTA pure 25	ÄKTA pure 150
UV monitors	U9-L	U9-L
	U9-M	U9-M
Conductivity monitor	C9	C9
External air sensor	L9-1.5	L9-1.5
	L9-1.2	L9-1.2
Fraction collectors	F9-C	F9-C
	F9-R	F9-R
I/O-box	E9	E9
Sample pump	S9	S9H


Illustration convention





In the valve illustrations below, the following convention is used to point out the location of the ports on the valve head. Loop valve **V9-L** is used as an example.

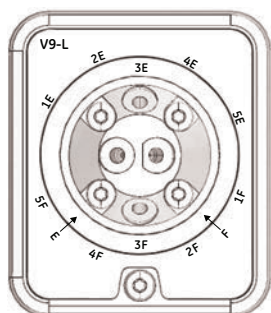





- Ports located on the valve head rim are indicated outside the black ring (e.g., 1E, 2E, etc.).
- Ports located on the pivot part of the valve head are indicated on the inside of the black ring (e.g., 3E and 3F).
- Ports located on the valve head front are indicated by an arrow (e.g., E and F).





Core modules




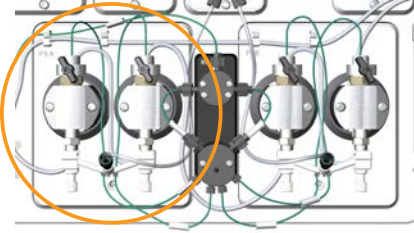
Core module	Description
System pump P9 A or P9H A 	A high precision pump, which delivers buffer or sample in purification runs. For further information, refer to Section 2.4.1 System pumps, on page 33 .

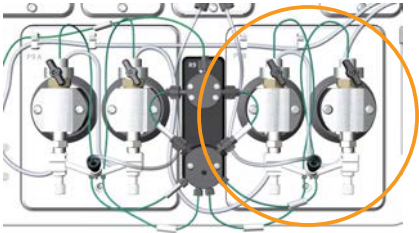
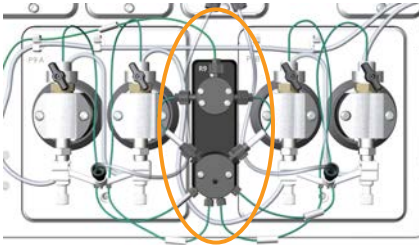
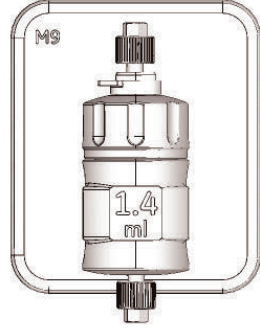

Core module	Description
System pump P9 B or P9H B 	A high precision pump, which delivers buffer in purification runs. For further information, refer to Section 2.4.1 System pumps, on page 33.
Pressure monitor R9 	Reads the system pressure after System pump A and System pump B. For further information, refer to Section 2.4.12 Pressure monitors, on page 67.
Mixer M9 	Mixes the buffers delivered from the system pumps to a homogeneous buffer composition. Three Mixer chambers are available for ÄKTA pure 25, their volumes are: 0.6 ml, 1.4 ml (mounted at delivery) and 5 ml. Three Mixer chambers are available for ÄKTA pure 150. Their volumes are: 1.4 ml (mounted at delivery), 5 ml (included in delivery), and 15 ml.  CAUTION Risk of explosion. Do not use Mixer chamber 15 ml with an ÄKTA pure 25 system configuration. The maximum pressure for Mixer chamber 15 ml is 5 MPa. For further information, refer to Section 2.4.2 Mixer, on page 37.
Injection valve V9-Inj or V9H-Inj 	Directs sample onto the column. For further information, refer to Section 2.4.6 Injection valve, on page 49.



Optional modules

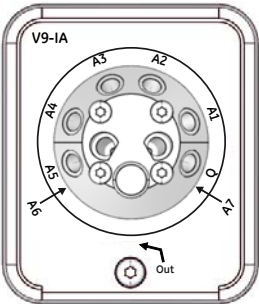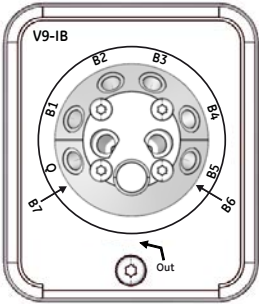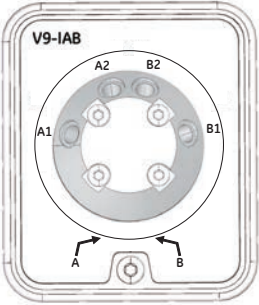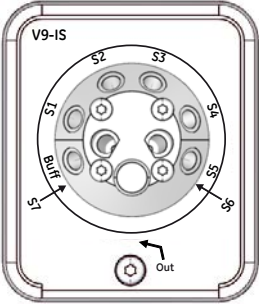Module	Description
Inlet valve V9-IA or V9H-IA 	Inlet valve for System pump A with seven inlet ports and integrated air sensor. For further information, refer to Section 2.4.4 Inlet valves, on page 39.
Inlet valve V9-IB or V9H-IB 	Inlet valve for System pump B with seven inlet ports and integrated air sensor. For further information, refer to Section 2.4.4 Inlet valves, on page 39.
Inlet valve V9-IAB or V9H-IAB 	Inlet valve with two A inlet ports and two B inlet ports. No integrated air sensor. For further information, refer to Section 2.4.4 Inlet valves, on page 39.
Sample inlet valve V9-IS or V9H-IS 	Inlet valve with eight inlet ports (seven sample inlets and one buffer inlet) and integrated air sensor. The Sample inlet valve requires an external Sample pump module. For further information, refer to Section 2.4.4 Inlet valves, on page 39.

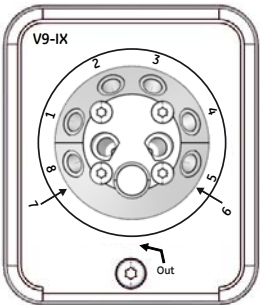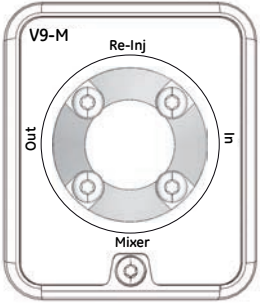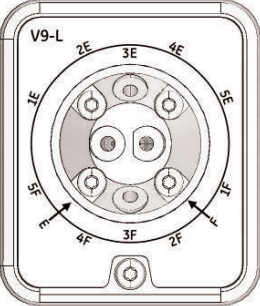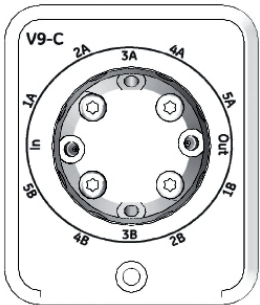Module	Description
Inlet valve V9-IX or V9H-IX 	Inlet valve with eight inlet ports. No integrated air sensor. For further information, refer to Section 2.4.4 Inlet valves, on page 39.
Mixer valve V9-M or V9H-M 	Directs the flow to the Injection valve, bypassing the Mixer, or to the Injection valve via the Mixer. For further information, refer to Section 2.4.5 Mixer valve, on page 46.
Loop valve V9-L or V9H-L 	Enables the use of up to five loops connected to the instrument. For further information, refer to Section 2.4.7 Loop valve, on page 52.
Column valve V9-C or V9H-C 	Connects up to five columns to the instrument, and directs the flow to one column at a time. The Column valve features two integrated pressure sensors. Allows the user to choose flow direction through the column, or to bypass the column. For further information, refer to Section 2.4.8 Column valves, on page 55.

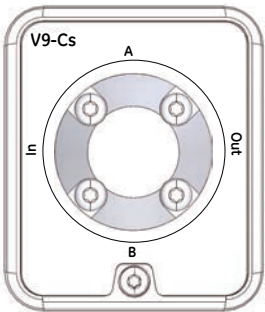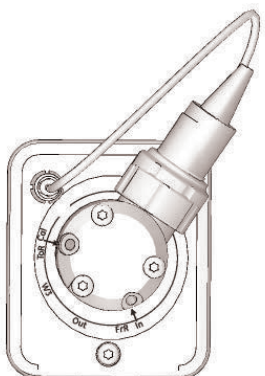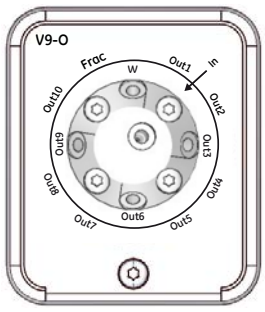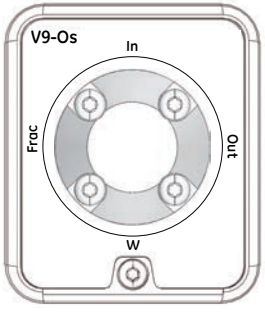
Module	Description
Column valve V9-Cs or V9H-Cs 	Connects a single column to the instrument. Allows the user to chose flow direction through the column, or to bypass the column. For further information, refer to Section 2.4.8 Column valves, on page 55.
pH valve V9-pH or V9H-pH 	Enables the pH electrode to be included in the flow path or bypassed during a run. The pH electrode may be calibrated when installed in the pH valve. For further information, refer to Section 2.4.10 pH valve, on page 60.
Outlet valve V9-O or V9H-O 	Directs the flow to the Fraction collector, Fraction collector 2 (out 10), any of the ten outlet ports, or waste. For further information, refer to Section 2.4.11 Outlet valves, on page 64.
Outlet valve V9-Os or V9H-Os 	Directs the flow to the Fraction collector, Fraction collector 2, the outlet port, or waste. For further information, refer to Section 2.4.11 Outlet valves, on page 64.

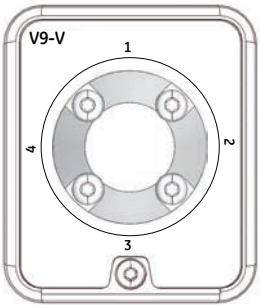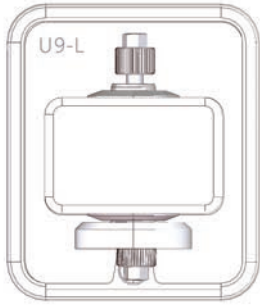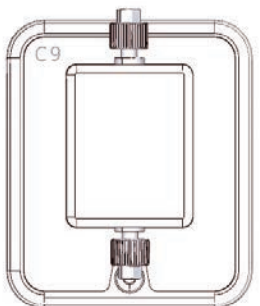Module	Description
Versatile valve V9-V or V9H-V 	A 4-port, 4-position valve, which can be used when adding extra features to the flow path. For further information, refer to Section 2.4.9 Versatile valve, on page 59.
UV monitor U9-L 	Measures the UV absorbance at a fixed wavelength of 280 nm. For further information, refer to Section 2.4.13 UV monitors, on page 69.
UV monitor U9-M 	Measures the UV/Vis absorbance at up to three wavelengths simultaneously in the range 190-700 nm. For further information, refer to Section 2.4.13 UV monitors, on page 69.
Conductivity monitor C9 	Measures the conductivity of buffers and eluted proteins. For further information, refer to Section 2.4.14 Conductivity monitor, on page 72.

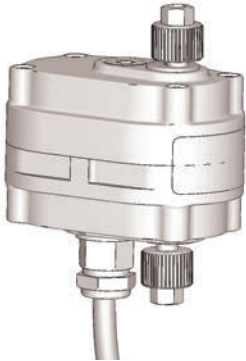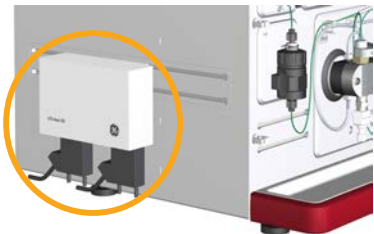Module	Description
External air sensor L9-1.5 or L9-1.2 	Prevents air from being introduced into the flow path. For further information, refer to Section 3.1 External air sensors, on page 87.
Fraction collector F9-C 	Flexible fraction collector that can collect up to 576 fractions. Up to two fraction collectors can be connected at the same time, of which only one (the primary) can be a Fraction collector F9-C. For further information, refer to Section 3.2 Fraction collector F9-C, on page 89.
Fraction collector F9-R 	Round fraction collector that can collect up to 175 fractions. Up to two fraction collectors can be connected at the same time. For further information, refer to Section 3.3 Fraction collector F9-R, on page 103.
I/O-box E9 	Receives analog or digital signals from, or transfers analog or digital signals to, external equipment that has been incorporated in the system. For further information, refer to Section 3.5 I/O-box E9, on page 111.

2 The ÄKTA pure instrument

2.1 Overview illustrations

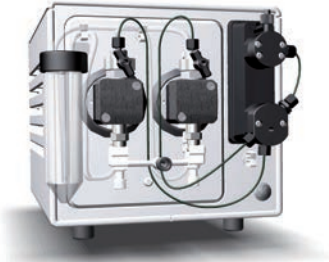Module	Description
Sample pump S9 or S9H 	A high precision pump with an integrated pressure monitor. The sample pump delivers buffer or sample in purification runs. For further information, refer to Section 3.4 Sample pump S9 and S9H, on page 107.


2.2 Liquid flow path

Introduction

ÄKTA pure is a liquid chromatography system with a flexible flow path.
This section provides an overview of the liquid flow path, and its possibilities.

Example of a typical liquid flow path

The illustration below shows the flow path for a typical system configuration. The individual instrument modules are presented in the table below. The configuration of the system is defined by the user.

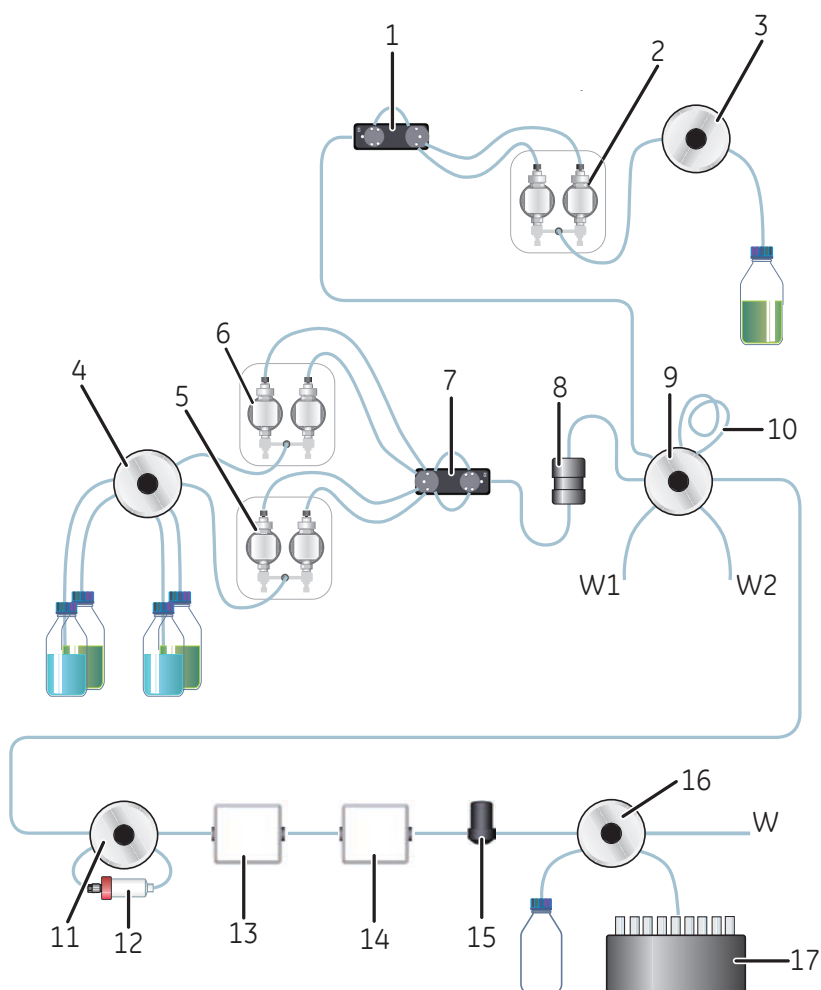

Part	Description
1	Pressure monitor
2	Sample pump
3	Sample inlet valve

2 The ÄKTA pure instrument

2.2 Liquid flow path

Part	Description
4	Inlet valve
5	System pump B
6	System pump A
7	Pressure monitor
8	Mixer
9	Injection valve
10	Sample loop or Superloop
11	Column valve
12	Column
13	UV monitor
14	Conductivity monitor
15	Flow restrictor
16	Outlet valve
17	Fraction collector
W, W1, W2	Waste

2.3 Instrument control panel

Introduction



This section describes the design and main function of the Instrument control panel **B9**.

Function of the Instrument control panel

The Instrument control panel shows the current state of the system. The **Pause** and **Continue** buttons can be used to control an ongoing run. It is possible to lock and unlock the Instrument control buttons from UNICORN.

Location and illustration

The illustration below shows the location and detailed view of the Instrument control panel.

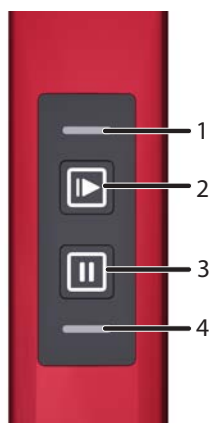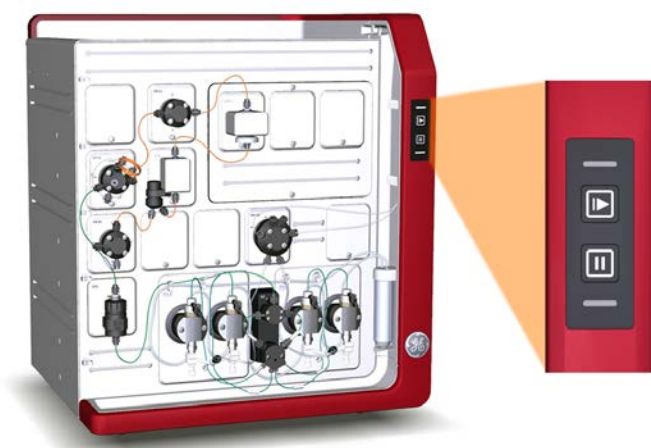


Part	Function
1	Power/Communication indicator (white)
2	Continue button with a green light indicator
3	Pause button with an orange light indicator
4	Alarm and error indicator (red)

Lock/Unlock function

Follow the instruction below to lock or unlock the **Pause** and **Continue** buttons of the Instrument control panel from UNICORN.

Step	Action
1	In System Control , select System:Settings . <i>Result:</i> The System Settings dialog opens.
2	In the System Settings dialog: • Select Advanced:Instrument control panel. • Select Locked or Unlocked. • Click OK.

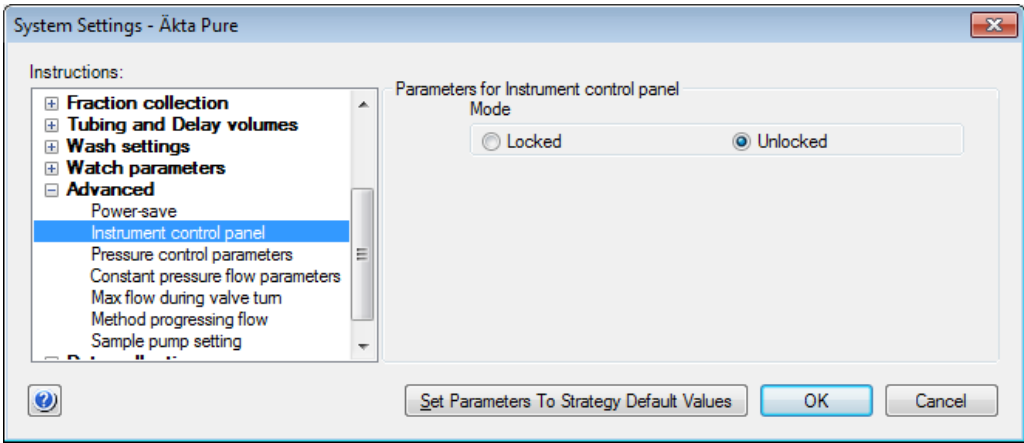

Buttons

The Instrument control panel includes the following buttons:

Part	Function
	Resumes instrument operation from the following states: • Pause • Wash • Hold
	Pauses the run and stops all pumps.

Status indications

The light indicators on the Instrument control panel indicate the current status of ÄKTA pure. The table below describes the different states that can be displayed.

Display	State	Description
All light indicators are off. 	Off	The instrument is turned off.
The Power/Communication indicator flashes slowly. 	Power-on	The instrument has no communication with the Instrument server.
The Power/Communication indicator flashes quickly. 	Connecting	The system is starting up.
The Power/Communication indicator displays a constant light. 	Ready	The instrument is ready to use.

Display	State	Description
Both the Power/Communication indicator and Continue button display a constant light. 	Run	A run is ongoing.
The Power/Communication indicator displays a constant light and the Continue button flashes slowly. 	Wash	A wash instruction or a pump synchronization is ongoing.
	Hold	A run has been put on hold.
Both the Power/Communication indicator and Pause button display a constant light. 	Pause	A run has been paused.
The Power/Communication indicator displays a constant light. and the Alarm and error indicator flashes. 	Alarms and errors	The system has been paused due to an alarm. To resume the run, acknowledge the alarm and continue the run in UNICORN.

Display	State	Description
The Power/Communication indicator displays a pulsating light. 	Power-save	The system is in power-saving mode.
All indicators are lit in a wave pattern. 	Re-programming	A module is being re-programmed to be compatible with the current instrument configuration.

2.4 Instrument modules

Introduction

This section describes the design and main functions of the instrument modules.

In this section

This section contains the following subsections:

Section	See page
2.4.1 System pumps	33
2.4.2 Mixer	37
2.4.3 Valves, overview	38
2.4.4 Inlet valves	39
2.4.5 Mixer valve	46
2.4.6 Injection valve	49
2.4.7 Loop valve	52
2.4.8 Column valves	55
2.4.9 Versatile valve	59
2.4.10 pH valve	60
2.4.11 Outlet valves	64
2.4.12 Pressure monitors	67
2.4.13 UV monitors	69
2.4.14 Conductivity monitor	72
2.4.15 Flow restrictor	74

2.4.1 System pumps

Introduction

This section describes the design and main functions of the system pumps, and also the pump piston rinsing systems. The system can also be equipped with an external, optional sample pump, see [Section 3.4 Sample pump S9 and S9H, on page 107](#).

Function of the system pumps

The ÄKTA pure instrument is fitted with two high precision system pumps, System pump A and System pump B. The system pumps can be used individually, or in combination to generate isocratic or gradient elution in purification methods.


Each pump module consists of two pump heads that work alternately to give a continuous, low pulsation, liquid delivery. To ensure delivery of correct liquid volume, the pumps must be free from air. Each pump head is equipped with a purge valve that is used for this purpose. See [Section 5.4 Prime inlets and purge pump heads, on page 158](#).

The table below contains the operating limits and labels of the system pumps of ÄKTA pure 25 and ÄKTA pure 150, respectively.

Configuration	Label	Pump type	Flow rate	Max. pressure
ÄKTA pure 25	P9 A and P9 B	P9	0.001 – 25 ml/min Note: When running the Column packing flow instruction, the maximum flow rate is 50 ml/min.	20 MPa
ÄKTA pure 150	P9H A and P9H B	P9H	0.01 – 150 ml/min Note: When running the Column packing flow instruction, the maximum flow rate is 300 ml/min.	5 MPa

Location and illustration

The illustration below shows the location of System pump A and System pump B, together with a detailed view of a system pump.

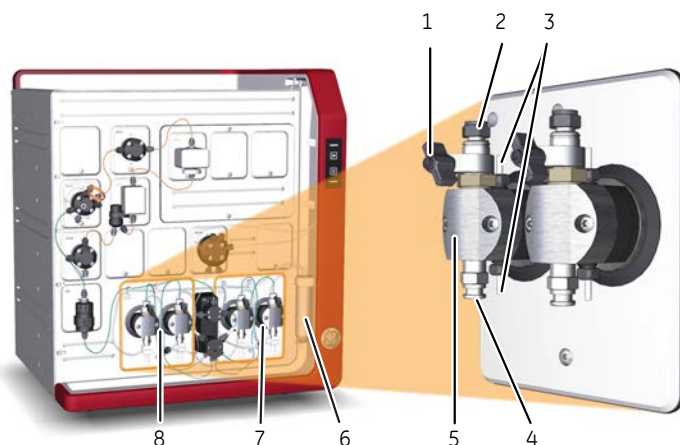

Part	Description
1	Purge valve: Used to remove air from the pump
2	Outlet port with check valve
3	Connections to pump piston rinsing system: Tubing is connected between the pumps and the Pump piston rinsing system tube (6)
4	Inlet port with check valve
5	Pump head: Encapsulates the inner parts of the pump
6	Pump piston rinsing system tube
7	System pump B
8	System pump A


The pump piston rinsing system

A seal prevents leakage between the pump chamber and the drive mechanism. The seal is continuously lubricated by the presence of liquid. The pump piston rinsing system continuously flushes the low pressure chamber behind the piston with a low flow of 20% ethanol. This prevents any deposition of salts from aqueous buffers on the pistons and prolongs the working life of the seals.

The pump piston rinsing system tubing is connected to the rearmost holes on the pump heads.

For instructions on how to fill the rinsing system, see [Prime the system pump piston rinsing system, on page 260](#).


Illustration of the pump piston rinsing system

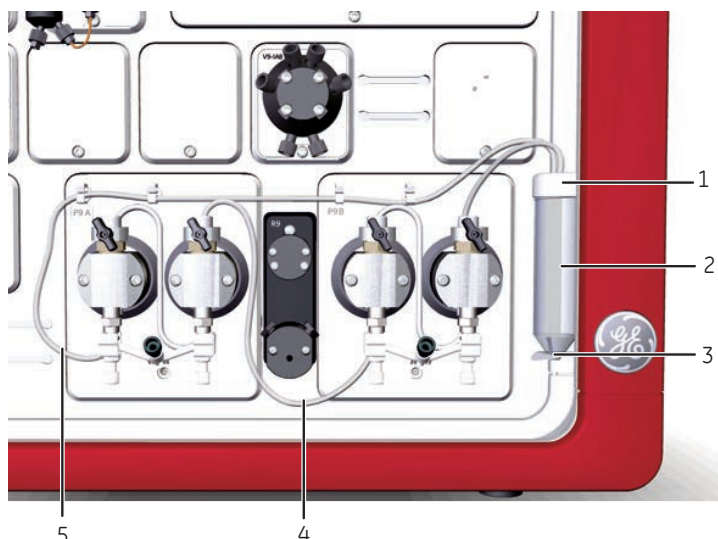

Part	Description
1	Rinsing system tube holder, top
2	Rinsing system tube
3	Rinsing system tube holder, bottom
4	Outlet tubing
5	Inlet tubing

System pump rinsing systems flow path

The illustration below shows the tubing configuration of the pump piston rinsing system of the system pumps.

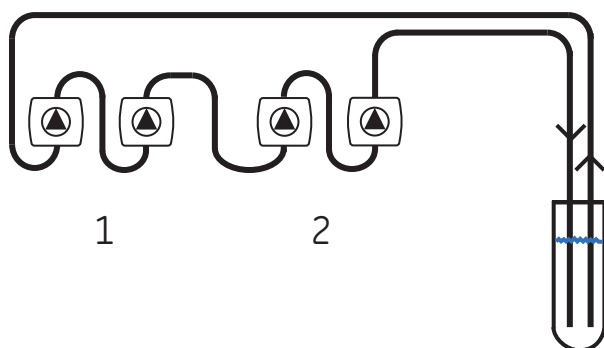

2 The ÄKTA pure instrument

2.4 Instrument modules

2.4.1 System pumps

Part	Description
1	System pump A
2	System pump B

2.4.2 Mixer

Function of the Mixer


Mixer **M9** is located after System pump A and System pump B, and before the Injection valve. The Mixer is a dynamic mixer for high-performance gradients. It is used to make sure that the buffers from the System pumps are mixed to give a homogenous buffer composition.

The Mixer has a built-in filter that prevents particles from reaching the column.

Note: Replace the sealing ring of the mixer with a highly resistant O-ring if the system is going to be exposed to organic solvents or high concentrations of organic acids for longer periods of time. Refer to [Section 7.8.4 Replace the O-ring inside the Mixer, on page 320](#) for how to change the ring.

Location and illustration

The illustration below shows the location, together with a detailed view of Mixer **M9**.

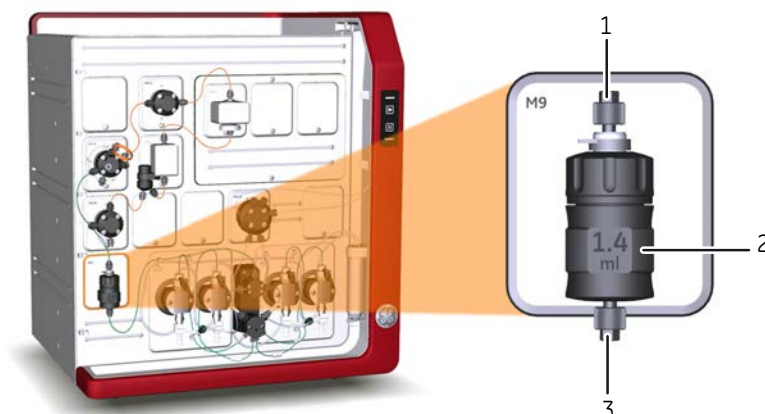

Part	Description
1	Outlet
2	Mixer chamber (0.6, 1.4, 5 or 15 ml)  CAUTION Risk of explosion. Do not use Mixer chamber 15 ml with an ÄKTA pure 25 configuration. The maximum pressure for Mixer chamber 15 ml is 5 MPa.
3	Inlet


2.4.3 Valves, overview

General design and function of rotary valves

The valves of the ÄKTA pure instrument allow flexibility in the liquid flow path. All valves used in the ÄKTA pure instrument are rotary valves. The motorized rotary valve consists of a Valve connection block with a number of defined bores with channels to the inlet and outlet ports of the valve. The Rotary disc, mounted on the motor, has a number of defined channels. The pattern of channels of the Rotary disc together with the pattern and location of the ports of the Valve connection block, define the flow path and function of each type of valve. When the Rotary disc turns, the flow path in the valve changes.

Illustration of inlet valve components

The illustration below shows the components of a disassembled Inlet valve A or a disassembled Inlet valve B. Inlet valve AB is built up by the same parts but have another configuration of defined bores.

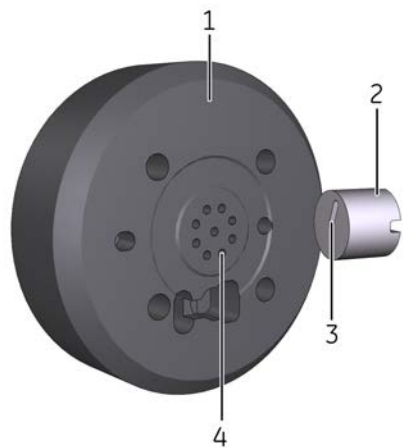

Part	Description
1	Valve connection block (stator)
2	Rotary disc (rotor)
3	Defined channel(s) in the Rotary disc
4	Defined bores in the Valve connection block

Note: Inlet and outlet ports are not visible in the picture. They are located on the opposite side of the Valve connection block.

2.4.4 Inlet valves

Function of the inlet valves

The inlet valves are used to select which buffers or samples to use in a run. The inlet valves available for ÄKTA pure and their functions are described in the table below.

Inlet valve	Label in		Function
	ÄKTA pure 25	ÄKTA pure 150	
Inlet valve A	V9-IA	V9H-IA	Enables automatic change between different buffers and wash solutions (seven inlet ports) . Can be used together with Inlet valve B to generate gradients by mixing buffer from System pump A and buffer from System pump B.
Inlet valve B	V9-IB	V9H-IB	Enables automatic change between different buffers and wash solutions (seven inlet ports). Can be used together with Inlet valve A to generate gradients by mixing buffer from System pump A and buffer from System pump B.
Inlet valve AB	V9-IAB	V9H-IAB	Enables automatic change between different buffers and wash solutions (two A and two B inlet ports). Can be used to generate gradients by mixing buffer from System pump A and buffer from System pump B.
Sample inlet valve	V9-IS	V9H-IS	Enables automatic loading of up to seven samples when used together with a sample pump.
Inlet valve X	V9-IX	V9H-IX	Increases the total number of inlets to the system. Can be used in two different configurations X1 and X2. The configurations are called V9-X1 and V9-X2 for ÄKTA pure 25 and, V9H-X1 and V9H-X2 for ÄKTA pure 150.

The modular design of ÄKTA pure allows the use of several combinations of inlet valves.

The possible combinations of Inlet valve A, Inlet valve B and Inlet valve AB are:

- one Inlet valve A
 - one Inlet valve B
 - Inlet valve A and Inlet valve B,
 - Inlet valve AB together with Inlet valve A or Inlet valve B,
 - one Inlet valve AB,
- or

- no installed inlet valves.

The sample inlet valve can be used together with any of the combinations listed above.

The air sensors integrated in Inlet valve A, Inlet valve B, and Sample inlet valve detect the presence of air and prevent the air from entering the pump.

Inlet valve AB and Inlet valve IX lack built-in air sensors, but can be used together with external air sensors.


Location of inlet valves

The locations of the inlet valves are described in the following table:

Inlet valve	Location
Inlet valve A	Before System pump A
Inlet valve B	Before System pump B
Inlet valve AB	Before both System pump A and System pump B
Sample inlet valve	Before the sample pump
Inlet valve IX	For example, before another inlet valve

Illustration of Inlet valve A and Inlet valve B


The illustration below shows a detailed view of Inlet valve A and Inlet valve B, in this example with labels **V9-IA** and **V9-IB**.

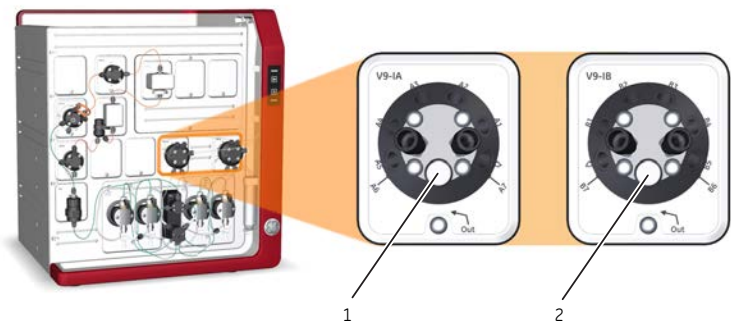

Part	Description
1	Integrated air sensor of Inlet valve A (located under the plug)
2	Integrated air sensor of Inlet valve B (located under the plug)

Ports of Inlet valve A and Inlet valve B


The illustration below shows the ports of Inlet valve A and Inlet valve B, in this example with labels **V9-IA** and **V9-IB**.

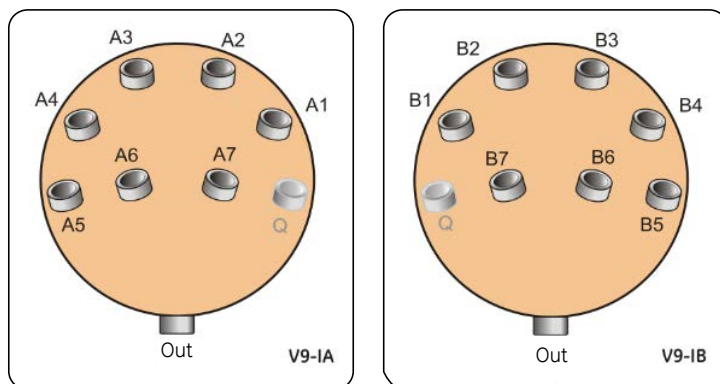

Port	Description
A1-A7	Buffer inlets of Inlet valve A
B1-B7	Buffer inlets of Inlet valve B
Q	Not used for ÄKTA pure
Out	To the respective System pump

Illustration of Inlet valve AB

The illustration below shows a detailed view of Inlet valve AB.

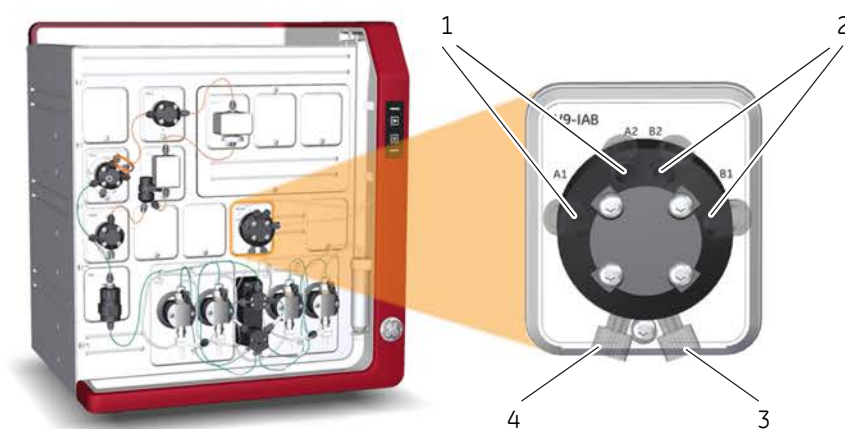


Part	Description
1	A inlet ports
2	B inlet ports
3	Outlet port to System pump B
4	Outlet port to System pump A

Note: Inlet valve AB does not have any integrated air sensor.

Ports of Inlet valve AB


The illustration below shows the ports of Inlet valve AB.

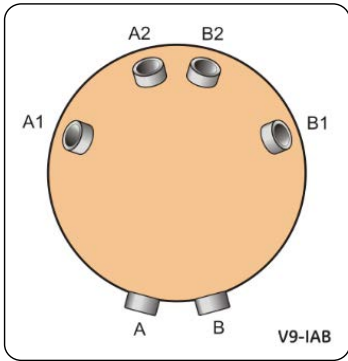

Port	Description
A1-A2	Inlet ports A1 and A2 of Inlet valve AB are used when buffers or samples should be delivered to System pump A
B1-B2	Inlet ports B1 and B2 of Inlet valve AB are used when buffers or samples should be delivered to System pump B
A	Outlet port A of Inlet valve AB leads to System pump A
B	Outlet port B of Inlet valve AB leads to System pump B

Illustration of Sample inlet valve


The illustration below shows a detailed view of the Sample inlet valve.

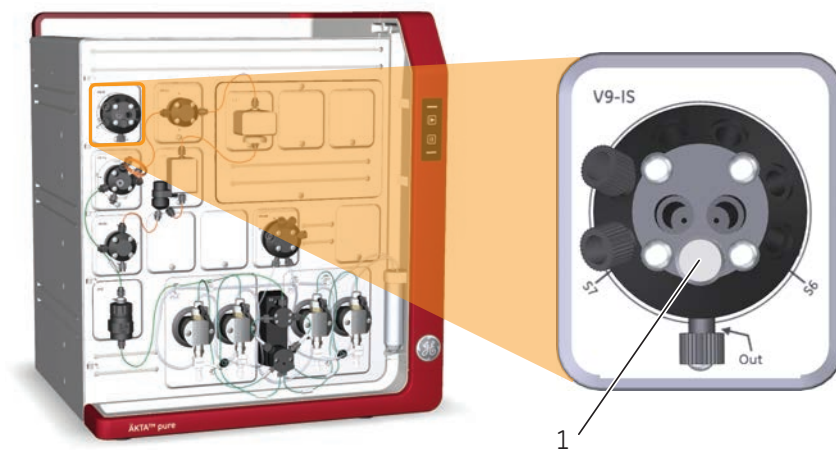

Part	Description
1	Integrated air sensor (located under the plug)

Ports of Sample inlet valve


The illustration below shows the ports of Sample inlet valve, in this example labeled **V9-IS**.

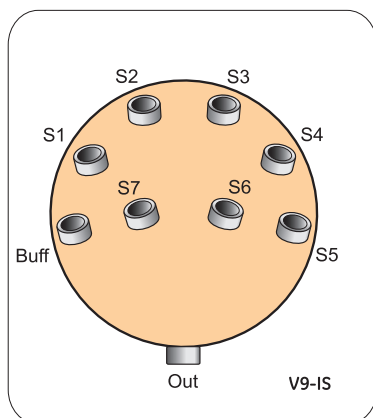

Port	Description
S1-S7	Sample inlets
Buff	Buffer inlet
Out	To Sample pump

Ports of Inlet valve IX

The illustration below shows the ports of Inlet valve IX.

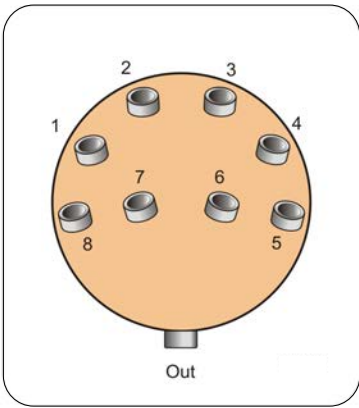

Port	Description
1-8	Inlets
Out	For example, to another inlet valve

Note: Inlet valve IX does not have an integrated air sensor.

Connect tubing

The table below shows the tubing and connectors that is delivered together with the optional inlet valves.

Tubing label	Connection	Tubing		Connector		Tubing length (mm)
		ÄKTA pure 25	ÄKTA pure 150	ÄKTA pure 25	ÄKTA pure 150	
A1-A2 and B1-B2	Inlets to Inlet valve AB	FEP, o.d. 1/8", i.d. 1.6 mm	FEP, o.d. 3/16", i.d. 2.9 mm	Tubing connector, 5/16" with Ferrule (yellow), 1/8"	Tubing connector, 5/16" with Ferrule (blue), 3/16"	1500
A1-A7	Inlets to Inlet valve A	FEP, o.d. 1/8", i.d. 1.6 mm	FEP, o.d. 3/16", i.d. 2.9 mm	Tubing connector, 5/16" with Ferrule (yellow), 1/8"	Tubing connector, 5/16" with Ferrule (blue), 3/16"	1500
B1-B7	Inlets to Inlet valve B	FEP, o.d. 1/8", i.d. 1.6 mm	FEP, o.d. 3/16", i.d. 2.9 mm	Tubing connector, 5/16" with Ferrule (yellow), 1/8"	Tubing connector, 5/16" with Ferrule (blue), 3/16"	1500

Tubing label	Connection	Tubing		Connector		Tubing length (mm)
		ÄKTA pure 25	ÄKTA pure 150	ÄKTA pure 25	ÄKTA pure 150	
InA	From Inlet valve A or Inlet valve AB to System pump A	FEP, o.d. 1/8", i.d. 1.6 mm	FEP, o.d. 3/16", i.d. 2.9 mm	Tubing connector, 5/16" with Ferrule (yellow), 1/8"	Tubing connector, 5/16" with Ferrule (blue), 3/16"	300
InB	From Inlet valve B or Inlet valve AB to System pump B	FEP, o.d. 1/8", i.d. 1.6 mm	FEP, o.d. 3/16", i.d. 2.9 mm	Tubing connector, 5/16" with Ferrule (yellow), 1/8"	Tubing connector, 5/16" with Ferrule (blue), 3/16"	300
S1-S7	Sample inlets to Sample inlet valve	FEP o.d. 1/8", i.d. 1.6 mm	FEP, o.d. 3/16", i.d. 2.9 mm	Tubing connector, 5/16" with Ferrule (yellow), 1/8"	Tubing connector, 5/16" with Ferrule (blue), 3/16"	1000
Buff	Buffer inlet to Sample inlet valve	FEP o.d. 1/8", i.d. 1.6 mm	FEP, o.d. 3/16", i.d. 2.9 mm	Tubing connector, 5/16" with Ferrule (yellow), 1/8"	Tubing connector, 5/16" with Ferrule (blue), 3/16"	1000
InS	Sample inlet valve to Sample Pump	FEP o.d. 1/8", i.d. 1.6 mm	FEP, o.d. 3/16", i.d. 2.9 mm	Tubing connector, 5/16" with Ferrule (yellow), 1/8"	Tubing connector, 5/16" with Ferrule (blue), 3/16"	580

Note: Narrow inlet tubing is available for **S1-S7**. Refer to [Section 9.3 Tubing and connectors](#), on [page 419](#) for more information.

2.4.5 Mixer valve

Function of Mixer valve

Mixer valve (**V9-M** or **V9H-M**) allows the user to bypass the mixer. It is intended to be used when the System pump is used for sample application or when a sample is re-injected.

Note: Mixer valve (**V9-M** or **V9H-M**) cannot be used together with Sample pump **S9** or Sample pump **S9H**.


Location and illustration of Mixer valve

The illustration below shows the recommended location, together with a detailed view of the Mixer valve.



Ports and flow paths of the mixer valve

The illustration and tables below describe the ports of and different flow paths through the Mixer valve. The Mixer valve has two available flow paths; **By-pass**, and **Mixer** (default). If the Mixer valve is installed in the recommended location before the Mixer, **By-pass** allows the flow to bypass the Mixer, and **Mixer** directs the flow to the Mixer.

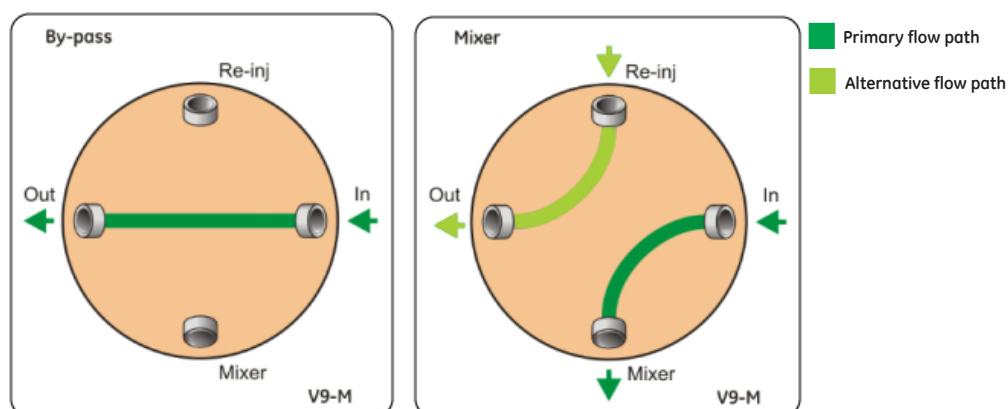

Port	Description
In	Port in which the flow enters the valve. Should be connected to the System pressure monitor outlet.
Out	Port from which the flow leaves the Mixer valve and bypasses the Mixer. Connect to the injection valve SaP port.
Re-inj	Port for advanced configurations including re-injection.
Mixer	Port from which the flow leaves the valve and is directed to the Mixer.

Connect tubing


The table below shows recommended tubing and connectors.

Tubing label	Connection	Tubing		Connector	Tubing length (mm)
		ÄKTA pure 25	ÄKTA pure 150		
3-1	Pressure monitor R9 to Mixer valve V9-M port In	PEEK, o.d. 1/16", i.d. 0.75 mm	PEEK, o.d. 1/16", i.d. 1.00 mm	Fingertight connector, 1/16"	160
3-2	Mixer valve V9-M port Mixer to Mixer M9	PEEK, o.d. 1/16", i.d. 0.75 mm	PEEK, o.d. 1/16", i.d. 1.00 mm	Fingertight connector, 1/16"	330
3-3	Mixer valve V9-M port Out to Injection valve V9-Inj port SaP	PEEK, o.d. 1/16", i.d. 0.75 mm	PEEK, o.d. 1/16", i.d. 1.00 mm	Fingertight connector, 1/16"	260

Flow paths through Mixer valve

The Mixer valve (V9-M, V9H-M) has two available flow paths; **By-pass**, and **Mixer**. If the Mixer valve is installed in the recommended location before the Mixer, **By-pass** allows the flow to bypass the Mixer, and **Mixer** directs the flow to the Mixer.

The illustration below shows the different flow paths through the Mixer valve **V9-M**.

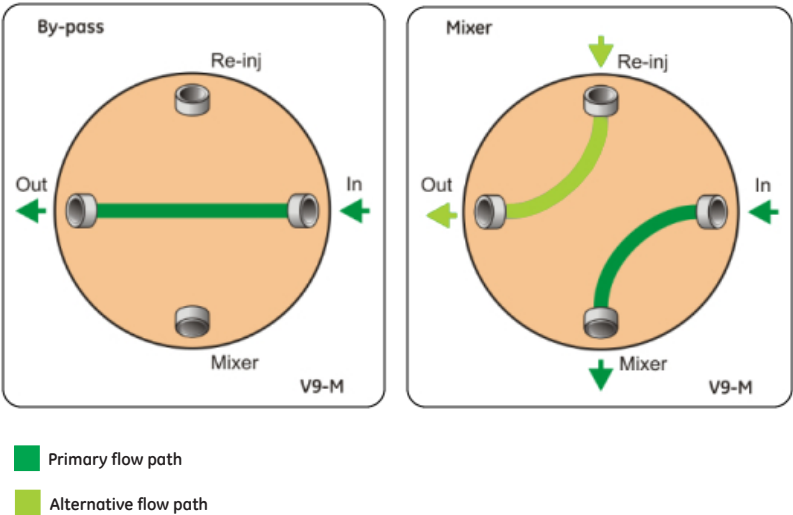

Flow path	Description
By-pass	The flow from the system pumps bypasses the mixer.
Mixer	The flow from the system pumps is directed to the Mixer. Mixer is the default flow path.

2.4.6 Injection valve

Function of the Injection valve

The Injection valve is used to direct sample onto the column. The valve enables usage of a number of different sample application techniques.


The injection valve is labeled **V9-Inj** for ÄKTA pure 25 and **V9H-Inj** for ÄKTA pure 150.

A sample loop or a Superloop can be connected to the injection valve and filled either automatically, using a Sample Pump or System pump A, or manually, using a syringe. The sample can also be injected directly onto the column using a Sample pump, or System pump A together with the mixer valve.

For instructions on how to connect and use loops, see [Section 5.7 Sample application, on page 177](#).

Location and illustration of the Injection valve

The illustration below shows the location, together with a detailed view of the Injection valve, in this example labeled **V9-Inj**.

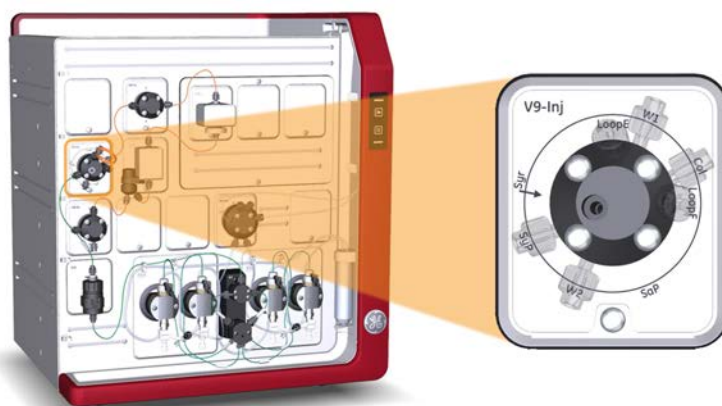

Ports and flow paths of the Injection valve


The illustration and tables below describe the ports of and different flow paths through the Injection valve.

The Injection valve can be set to different positions that give different flow paths through the valve.

2 The ÄKTA pure instrument

2.4 Instrument modules

2.4.6 Injection valve

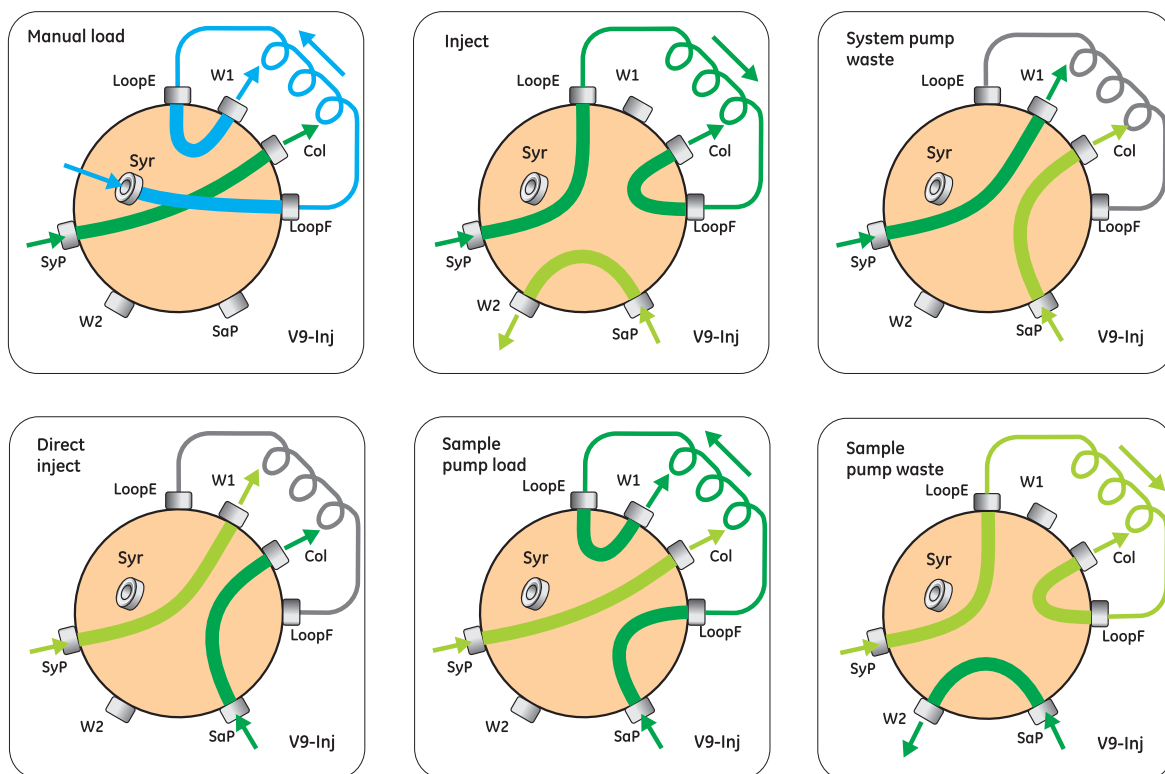

- Primary flow path
- Alternative flow path
- Flow path for manual load
- Closed flow path

Port	Description
SaP	Inlet from - sample pump, or - system pump via the Mixer valve Out port.
SyP	Inlet from the System pumps via the Mixer
Syr	Syringe connection
Col	Outlet to one of the Column valves or to the column.
LoopF	Port for connection of a loop. Used to fill the loop.
LoopE	Port for connection of a loop. Used to empty the loop into the flow path.
W1	Loop and System pump waste
W2	Sample flow waste

Flow path	Description
Manual load - Default position of the valve	The system flow is directed onto the column or column valve. Sample can be manually injected into the loop. Excess sample leaves the valve through waste port W1 .
Inject	The system flow is directed through the loop and onto the column or column valve. If a mixer valve or the sample pump is used, the flow entering the SaP port is directed to waste port W2 .
System pump waste	The system flow is directed to waste port W1 . If a mixer valve or the sample pump is used, the flow entering the SaP port is directed to the column or the column valve.
Direct inject	The flow entering the SaP port is directed to the column or the column valve. This position is used with: - the sample pump, or - a mixer valve and System pump A, bypassing the mixer. Flow entering the SyP port is directed to waste port W1 .
Sample pump load	The flow entering the SaP port is directed to the loop. This position is used with: - the sample pump, or - a mixer valve and System pump A, bypassing the mixer. Excess sample leaves the valve through waste port W1 . The flow entering the SyP port is directed to the column or the column valve.
Sample pump waste	The flow entering the SaP port is directed to waste port W2 . This position is used with: - the sample pump, or - a mixer valve and System pump A. The flow entering the SyP port is directed to the column via the loop.

- Note:**
- In order to avoid sample carry-over when switching techniques for loading samples, wash the injection valve with buffer between the loading of two different samples. For example, when switching from loading sample onto the loop to loading sample directly onto the column with the valve in **Direct inject** position.*
 - Make sure that the **SaP** port is plugged with a stop plug if neither the sample pump nor the mixer is used.*


2.4.7 Loop valve

Function of the Loop valve

The Loop valve allows the user to connect several loops simultaneously to the instrument. It can for example be used for storing intermediate fractions in multi-step purifications, for storing samples to be used in scouting runs, or for storing eluents needed in low volumes. The valve also has a built-in bypass function that enables bypassing all loops. The Loop valve is labeled **V9-L** or **V9H-L**.


Location and illustration of Loop valve

The illustration below shows the recommended location, together with a detailed view of Loop valve **V9-L**.

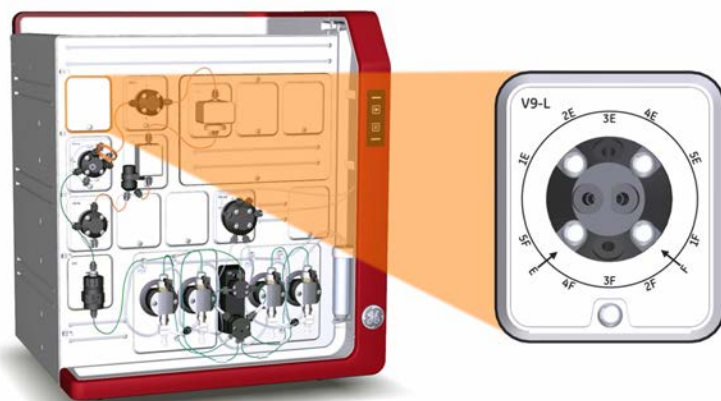

Ports and flow paths of the Loop valve

The illustration and tables below describe the ports and different flow paths through the Loop valve.

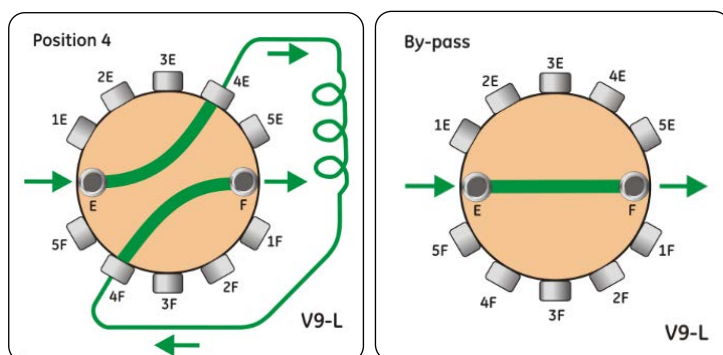

In the **Position 4** example, the loop is connected to loop position 4 and the loop is being emptied.

Port	Description
F	Port connected to the LoopF port of the Injection valve.
1F and 1E	Ports for connection to loop 1.
2F and 2E	Ports for connection to loop 2.
3F and 3E	Ports for connection to loop 3.
4F and 4E	Ports for connection to loop 4.
5F and 5E	Ports for connection to loop 5.
E	Port connected to the LoopE port of the Injection valve.

Note: Ports denoted by the letter *F* are used for filling the loop and ports denoted by the letter *E* are used for emptying the loop.

Flow path	Description
Position 1-5	The flow direction depends on the Injection valve position.
By-pass	The flow bypasses the loop(s). By-pass is the default flow path.

Connect tubing

The table below shows recommended tubing and connectors.

Tubing label	Connection	Tubing		Connector	Tubing length (mm)
		ÄKTA pure 25	ÄKTA pure 150		
L1	Injection valve position LoopF to Loop valve position F	PEEK, o.d. 1/16", i.d. 0.50 mm	PEEK, o.d. 1/16", i.d. 0.75 mm	Fingertight connector, 1/16"	160
L2	Injection valve position LoopE to Loop valve position E	PEEK, o.d. 1/16", i.d. 0.50 mm	PEEK, o.d. 1/16", i.d. 0.75 mm	Fingertight connector, 1/16"	160

Connect a Loop valve

The Loop valve is connected to the Injection valve instead of a loop, as described below.

Step	Action
1	Connect port E on the Loop valve to port LoopE on the Injection valve.
2	Connect port F on the Loop valve to port LoopF on the Injection valve.
3	Connect one or many loops to the Loop valve. See Section 5.7 Sample application, on page 177 .
	Note: <i>Always use the the first positions of the valve for the connected loops (e.g., if three loops will be used, use port 1F-3F and the corresponding ports 1E-3E) to avoid cross-contamination.</i>
Note:	<i>It is possible to place the Loop valve in other positions in the flow path than the one described above. However, the volume used for washes will then be incorrect, just as the system configuration shown in the process picture.</i>

2.4.8 Column valves

Function of the Column valves

The Column valves are used to connect columns to the system, and to direct the flow onto the column. The Column valves available for ÄKTA pure and their functions are described in the table below.


Label in		Function
ÄKTA pure 25	ÄKTA pure 150	
V9-C	V9H-C	Connects columns to the system and allows the user to choose column, flow direction through the column, or to bypass the columns. Up to five columns can be connected to the valve.
V9-Cs	V9H-Cs	Connects columns to the system and allows the user to choose flow direction through the column, or to bypass the column. One column can be connected to the valve.

The inlet and outlet ports of Column valves **V9-C** and **V9H-C** have built in pressure sensors that measures the actual pressure over the column. For further information on the pressure sensors, see [Function of pressure monitors integrated in Column valves V9-C or V9H-C, on page 68](#).

Column valves **V9-Cs** and **V9H-Cs** lack built-in pressure sensors. See [Section 5.5 Connect a column, on page 170](#) for information on how to set pressure alarms that protects the column when no Column valve **V9-C** or **V9H-C** is installed.

Location and illustration of Column valves

The illustration below shows the recommended location of the Column valves and a detailed view of the valves. In this example the valves are labeled **V9-Cs** and **V9-C**.

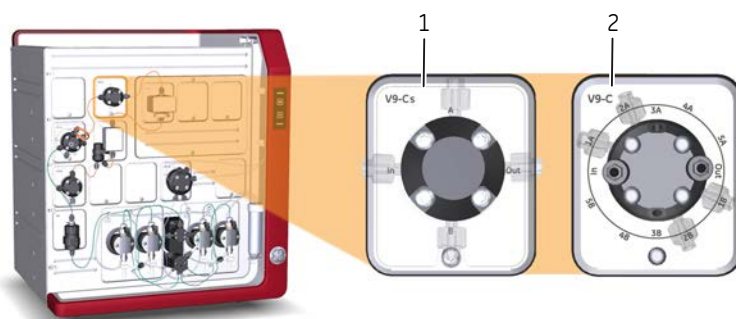


Part	Function
1	Column valve V9-Cs or V9H-Cs (no integrated pressure sensors)

Part	Function
2	Column valve V9-C or V9H-C (integrated pressure sensors)

Note: Maximum one column valve can be installed in ÄKTA pure at any given time.

Ports and flow paths of
Column valves V9-C and V9H-C

The illustration and tables below describe the different ports of and flow paths through Column valves **V9-C** and **V9H-C**. In the example below the column is connected to column position 4 and the valve is labeled **V9-C**.

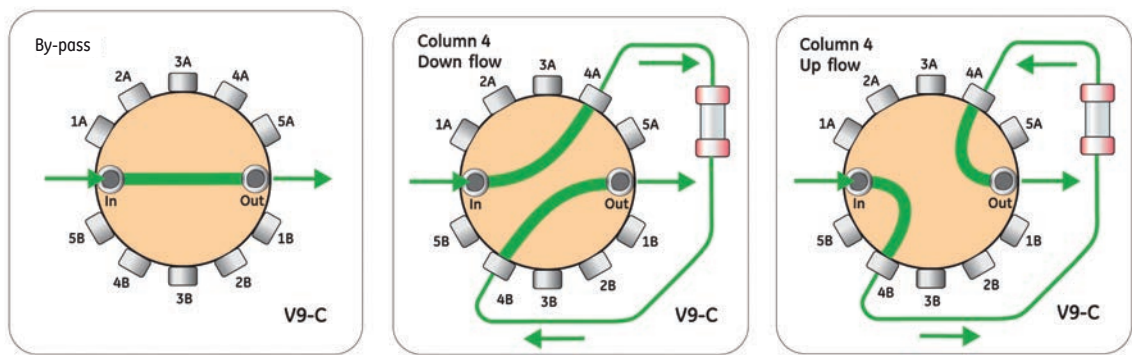


Port	Description
In	Inlet from Injection valve via a built-in pressure monitor.
1A-5A	Ports for connection to the top of columns.
1B-5B	Ports for connection to the bottom of columns.
Out	Outlet to UV monitor via a built-in pressure monitor.

Flow path	Description
By-pass	The flow bypasses the column(s). By-pass is the default flow path.
Down flow	The flow direction is from the top of the column to the bottom of the column. Down flow is the default flow direction.
Up flow	The flow direction is from the bottom of the column to the top of the column.

Ports and flow paths of Column valves V9-Cs and V9H-Cs

The illustration and tables below describe the different ports and flow paths of Column valve **V9-Cs**.

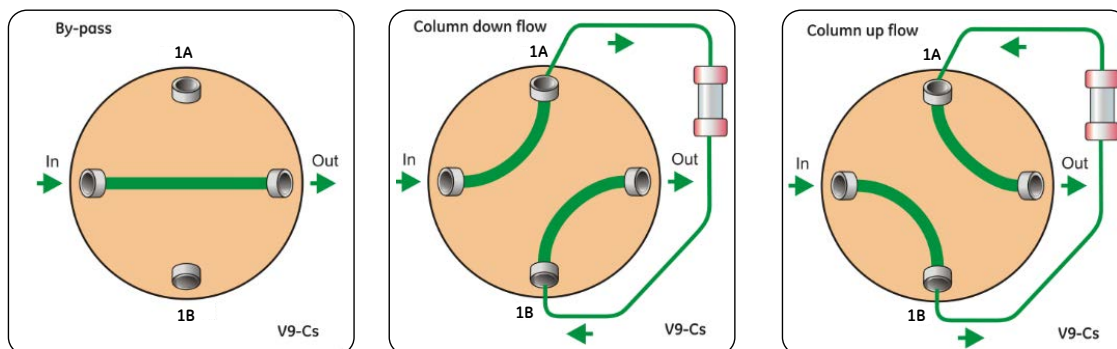

Port	Description
In	Inlet from Injection valve.
1A	Port for connection to the top of a column.
1B	Port for connection to the bottom of a column.
Out	Outlet to UV monitor.

Flow path	Description
By-pass	The flow bypasses the column. By-pass is the default flow path.
Down flow	The flow direction is from the top of the column to the bottom of the column. Down flow is the default flow direction.
Up flow	The flow direction is from the bottom of the column to the top of the column.

Connect tubing

The table below shows recommended tubing and connectors.

Tubing label	Connection	Tubing		Connector	Tubing length (mm)
		ÄKTA pure 25	ÄKTA pure 150		
5	Injection valve to Column valve	PEEK, o.d. 1/16", i.d. 0.50 mm	PEEK, o.d. 1/16", i.d. 0.75 mm	Fingertight connector, 1/16"	100
6	Column valve to UV monitor	PEEK, o.d. 1/16", i.d. 0.50 mm	PEEK, o.d. 1/16", i.d. 0.75 mm	Fingertight connector, 1/16"	160

2 The ÄKTA pure instrument

2.4 Instrument modules

2.4.8 Column valves

Follow the instructions below to connect tubing to the column valves.

Step	Action
1	If no Column valve is installed, remove the Union F/F between tubing 5 and tubing 6
2	Connect tubing between Injection valve, Column valve and UV monitor according to the table above.

Note: *The built-in pressure sensors for Column valve **V9-C** and **V9H-C** have to be re-calibrated after installation. See [Calibrate the monitors, on page 302](#).*

2.4.9 Versatile valve


Function of the Versatile valve

The Versatile valve is a 4-port, 4-position valve, which can be used to add extra features to the flow path. For example, the valve can be used to connect external equipment to the flow path during parts of a run. The versatile valve can be installed in any position. The versatile valve is labeled **V9-V** or **V9H-V**.

It is possible to install up to four versatile valves simultaneously in ÄKTA pure. The configuration is defined by the module's Node ID.

Ports and flow paths of the Versatile valve

The illustration and table below describe the different ports of and flow paths through the Versatile valve. The valve has four ports (**1-4**).

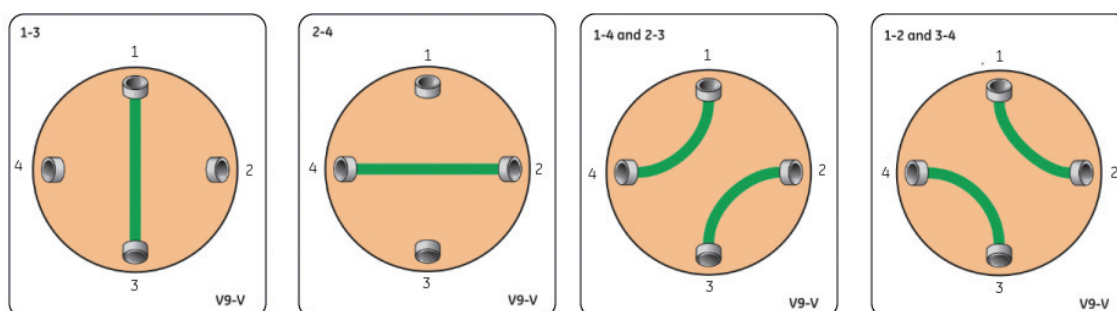

The Versatile valve has four available sets of flow paths; two where a single flow channel is used and two where the flow can be directed through two different channels simultaneously.

Flow path	Description
1-3	A single flow channel where the flow is directed between port 1 and port 3 .
2-4	A single flow channel where the flow is directed between port 2 and port 4 .
1-4 and 2-3	Two simultaneously used flow channels where the flow is directed between port 1 and port 4 and between port 2 and port 3 .
1-2 and 3-4	Two simultaneously used flow channels where the flow is directed between port 1 and port 2 and between port 3 and port 4 .

2.4.10 pH valve

Function of the pH valve

The pH valve is used to direct the flow to a pH electrode when inline monitoring of pH is desired during a run. The pH valve is labeled **V9-pH** for ÄKTA pure 25 and **V9H-pH** for ÄKTA pure 150.

The pH valve has an integrated flow cell in which the pH electrode can be installed.

It is recommended to connect a Flow restrictor to the pH valve. The flow restrictor is used to generate a back pressure high enough to prevent the formation of air bubbles in the UV flow cell.

The valve directs the flow to the pH electrode and to the flow restrictor, or bypasses one or both.

Note: The Flow restrictor is normally included in the flow path after the Conductivity monitor. When installing the pH valve on ÄKTA pure, the flow restrictor should be moved from its normal position on the conductivity monitor to the pH valve.

Location and illustration of the pH valve


The illustration below shows the recommended location, together with a detailed view of the pH valve.



Part	Description
1	pH valve
2	pH electrode
3	pH flow cell
4	Flow restrictor

Ports and flow paths of the pH valve

The illustration and table below describe the different ports of and flow paths through the pH valve, in this example labeled **V9-pH**.

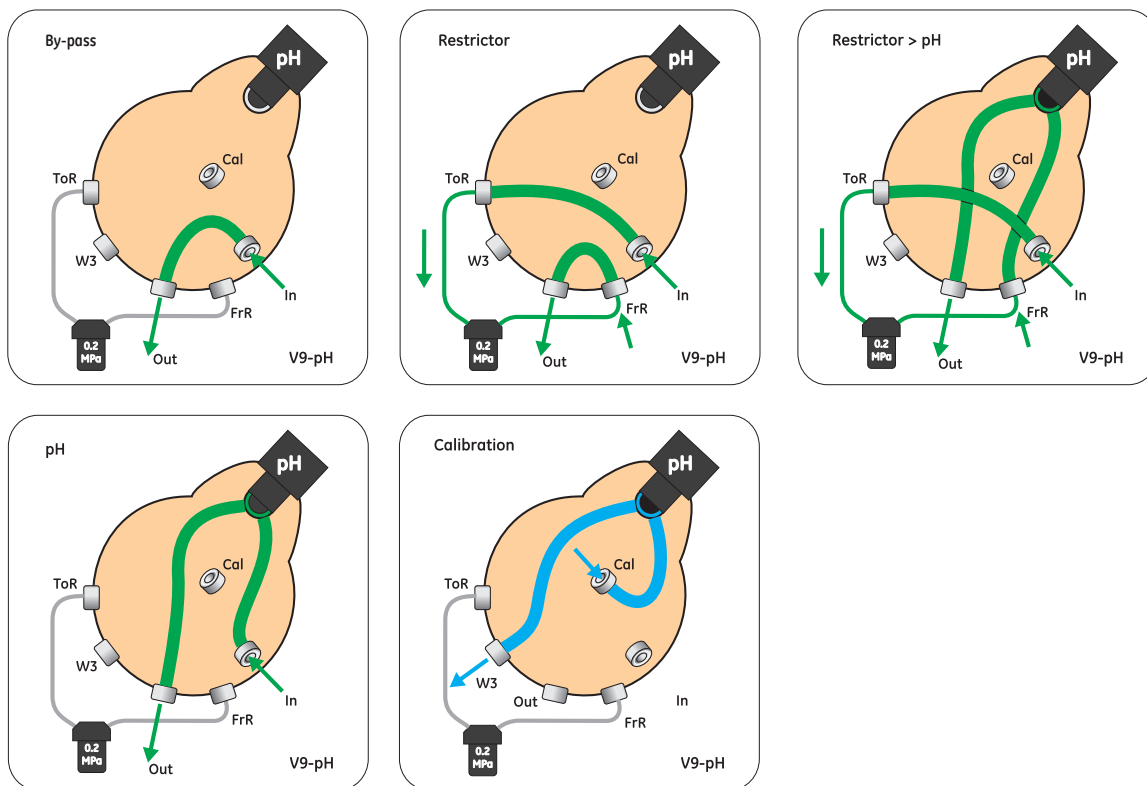

- Primary flow path
- Flow path for calibrations
- Closed flow path

Port	Description
In	From Conductivity monitor
ToR	To Flow restrictor
FrR	From Flow restrictor
Out	To Outlet valve
Cal	Calibration port
W3	To Waste

2 The ÄKTA pure instrument

2.4 Instrument modules


2.4.10 pH valve

Flow path	Description
By-pass	Both pH electrode and Flow restrictor are bypassed.
Restrictor	Flow restrictor is in use and pH electrode is bypassed.
Restrictor and pH	Both pH electrode and Flow restrictor are in use.
pH	pH electrode is in use and Flow restrictor is bypassed.
Calibration	Flow path used when calibrating the pH monitor and when filling the pH flow cell with storage solution. The Cal port is used to inject solution into the flow cell using a syringe. Excess solution leaves the valve through port W3 .

pH monitor

The pH monitor continuously measures the pH of the buffer and eluted proteins when the pH electrode is inline. A pH electrode can be installed in the pH flow cell. For instruction on how to install the pH electrode, see [Section 7.5.2 Replace the pH electrode, on page 272](#). The pH electrode should not be exposed to more than 0.5 MPa during a normal run, but can withstand pressure spikes of 0.8 MPa. It is therefore important to place it after the column.

The illustration below shows the location of the pH flow cell and a pH electrode installed in the pH valve.

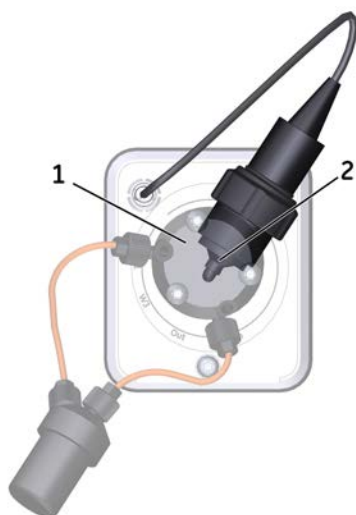

Part	Description
1	pH flow cell
2	pH electrode

Connect tubing

The table below shows recommended tubing.

Tubing label	Connection	Tubing		Connector	Tubing length (mm)
		ÄKTA pure 25	ÄKTA pure 150		
8pH	Conductivity monitor to port In	PEEK, o.d. 1/16", i.d. 0.50 mm	PEEK, o.d. 1/16", i.d. 0.75 mm	Fingertight connector, 1/16"	180
1R	Flow restrictor to port ToR	PEEK, o.d. 1/16", i.d. 0.50 mm	PEEK, o.d. 1/16", i.d. 0.75 mm	Fingertight connector, 1/16"	80
2R	Flow restrictor to port FrR	PEEK, o.d. 1/16", i.d. 0.50 mm	PEEK, o.d. 1/16", i.d. 0.75 mm	Fingertight connector, 1/16"	80
9pH	Port Out to Outlet valve	PEEK, o.d. 1/16", i.d. 0.50 mm	PEEK, o.d. 1/16", i.d. 0.75 mm	Fingertight connector, 1/16"	160
N/A	to Calibration port Cal	N/A	N/A	N/A	N/A
W3	Port W3 to Waste	ETFE I.D. 1 mm	ETFE I.D. 1 mm	Fingertight connector, 1/16"	1500

Note: The dimensions of the PEEK tubing depends on which tubing kit that is used. See [Section 9.3 Tubing and connectors, on page 419](#) for more information.

2.4.11 Outlet valves

Function of the outlet valves

The outlet valve is used to direct the flow to the fraction collector, to an outlet port, or to waste. The table below shows the labeling of the outlet valves for ÄKTA pure 25 and ÄKTA pure 150.

Label in		Description
ÄKTA pure 25	ÄKTA pure 150	
V9-O	V9H-O	10 outlet ports
V9-Os	V9H-Os	1 outlet ports


Location and illustration of outlet valves

The illustration below shows the recommended location, together with a detailed view of the outlet valves. In this example the valves are labeled **V9-Os** and **V9-O**.



Ports of Outlet valves V9-O and V9H-O

The illustration below shows the ports of Outlet valve **V9-O** and **V9H-O**, in this example labeled **V9-O**.

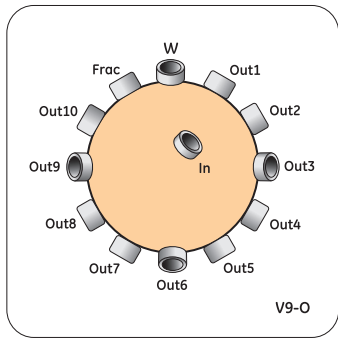


Port	Description
In	Inlet port

Port	Description
Out1 - Out10	Outlet ports 1 - 10
Frac	Port to Fraction collector Note: <i>If a secondary Fraction collector F9-R is used it should be connected to port Out10.</i>
W	Waste port

Ports of Outlet valves V9-Os and V9H-Os

The illustration below shows the ports of Outlet valve **V9-Os**.

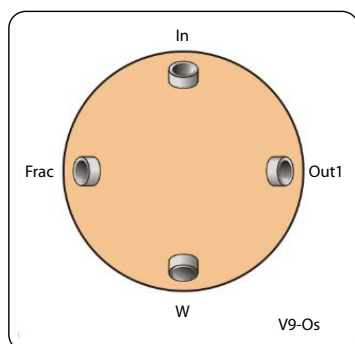

Port	Description
In	Inlet port
Out1	Outlet port
Frac	Port to fraction collector Note: <i>If a secondary Fraction collector F9-R is used it should be connected to port Out1.</i>
W	Waste port

Connect tubing

The table below shows recommended tubing and connectors.

Tubing label	Connection	Tubing		Connector	Tubing length (mm)
		ÄKTA pure 25	ÄKTA pure 150		
9	Flow restrictor to Outlet valve	PEEK, o.d. 1/16", i.d. 0.50 mm	PEEK, o.d. 1/16", i.d. 0.75 mm	Fingertight connector, 1/16"	135
9pH	pH valve to Outlet valve	PEEK, o.d. 1/16", i.d. 0.50 mm	PEEK, o.d. 1/16", i.d. 0.75 mm	Fingertight connector, 1/16"	160
Out1 - Out10	Outlets from the outlet valves	ETFE, o.d. 1/8", i.d. 1 mm	ETFE, o.d. 1/8", i.d. 1 mm	Fingertight connector, 1/16"	1500

Note: If ÄKTA pure previously has been configured without an Outlet valve, remove the Union F/F between tubing **9** and tubing **W** before installation of the Outlet valve. Then connect tubing **9** to the **In** port on the Outlet valve and the waste tubing **W** to the **W** port on the Outlet valve.

2.4.12 Pressure monitors

Introduction

This section describes the location and function of the pressure monitors.
 Up to four pressure monitors are included in ÄKTA pure.

Function of the system pump and the sample pump pressure monitors

Up to four pressure monitors are included in ÄKTA pure. One pressure monitor is always connected to the system pumps and one pressure monitor is part of the Sample pump (**S9** or **S9H**). The monitors of the pumps are both labelled **R9**.

The System pump pressure monitor measures the pressure after the system pumps, the system pressure. The pressure monitor of the sample pump measures the pressure after the sample pump, the sample pressure. To provide a reading of the highest pressure in the system there are connections to all pump cylinders.

The pressure monitor also contains pump flow restrictors in order to stop siphoning effects. Siphoning effects can occur if tubing in the system is disconnected while the inlet tubing is immersed in buffers that are placed on a higher level than the pump.

Location and illustration of System pressure monitor

The illustration below shows the location, together with a detailed view of System pressure monitor.



Part	Description
1	Pressure monitor
2	Pump flow restrictors

Function of pressure monitors integrated in Column valves V9-C or V9H-C


If Column valve C, labeled **V9-C** or **V9H-C**, is used, the two pressure monitors integrated in the valve can be used to monitor the column pressure.

Note: Column valve **V9-Cs** and **V9H-Cs** does not contain pressure monitors.

The pressure sensors integrated in the inlet and outlet ports of Column valve C measure the pressure before the column, Pre column pressure (A), and the pressure after the column, Post column pressure (B).

The Delta column pressure (C), which is the pressure drop over the column, is calculated as the difference between the Pre column pressure and the Post column pressure.

Pressure alarms can be set for both the Pre column pressure and the Delta column pressure. Pressure control of the flow may be based on either the Pre column pressure or the Delta column pressure.

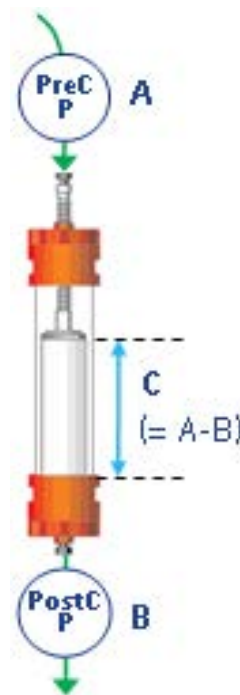

2.4.13 UV monitors

Introduction

This section describes the design and function of UV monitors **U9-M** and **U9-L**.
The modules include a monitor unit and a detector with a UV flow cell.

Function of UV monitor U9-M

UV monitor **U9-M** measures the UV absorbance at a wavelength range of 190 to 700 nm.
A flip-mode enables measuring of UV/Vis absorbance at three wavelengths simultaneously during a run. The second and third wavelength can be turned off or on in method phase properties, by manual instructions or in system settings.


Note: Installation of UV monitor **U9-M** should only be performed by GE Service personnel.

Note: The resolution is decreased when more than one wavelength is used simultaneously due to lower sampling frequency per wavelength. Do not use more wavelengths than necessary.

Location and illustration of UV monitor U9-M

The illustration below shows the location of UV monitor **U9-M**, together with a detailed view of the monitor unit and detector. The monitor unit is labelled **U9-M** and the detector **U9-D**.

Note: When UV monitor **U9-M** is used, the entire Multi-module panel shown in the illustration is replaced by **U9-M**.

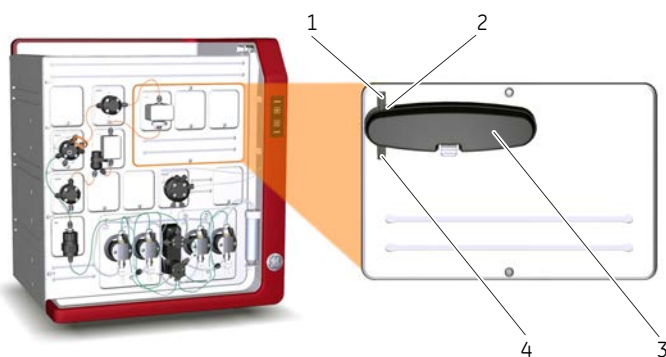

Part	Description
1	Inlet
2	UV flow cell. Three different path lengths are available: 0.5 mm, 2 mm (default) and 10 mm
3	UV detector
4	Outlet


Function of UV monitor U9-L

The UV monitor **U9-L** measures the UV absorbance at the fixed wavelength of 280 nm.

It is not possible to vary the wavelength, or turn on or off the **U9-L** monitor. This is therefore not shown in the **Phase Properties** pane in **Method Editor**.

Location and illustration of UV monitor U9-L

The illustration below shows the recommended location of UV monitor **U9-L**, together with a detailed view of the monitor and detector. The UV monitor **U9-L** requires that the Multi-module panel is installed, see [Example of a typical configuration of the wet side, on page 15](#). The UV monitor can also be installed in an Extension box, see [Extension box, on page 85](#).

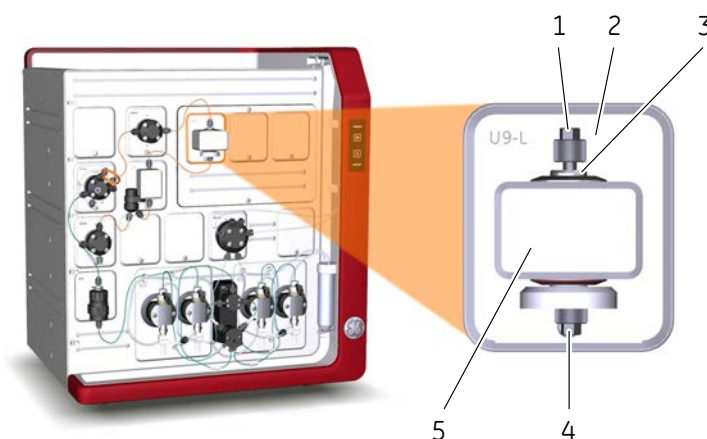

Part	Description
1	Inlet
2	UV monitor U9-L
3	UV flow cell. Two different path lengths are available: 2 mm (default) and 5 mm
4	Outlet
5	UV detector

Using two UV monitors

It is possible to use two UV monitors in ÄKTA pure, in two combinations. The configuration is defined by the module's Node ID.

- UV monitor U9-M together with UV monitor U9-L, 2nd
- UV monitor U9-L together with UV monitor U9-L, 2nd

Note: When using two UV monitors, the signal from the first UV monitor is by default used for peak fractionation. This can be changed by editing the text instruction **Fraction Collection:Peak fractionation parameters:Signal source** and choosing **UV 2nd** as **Signal source**.

Note: When using two UV monitors with different cell lengths to increase the UV absorption dynamic range, the U9-L signal comes from the real cell length and has to be calibrated for exact calculations. The U9-M signal is automatically calibrated to nominal cell length.

UV monitor U9-L, 2nd can be located anywhere in the flow path and is therefore shown in the **Process Picture** in UNICORN as a component without a fixed place. This means that it is possible to place U9-L, 2nd before the other UV monitor in the flow path.

Note: If **U9-L 2nd** is placed on the high pressure side of the column, pressure limits have to be considered. See [UV monitor options, on page 414](#)

Connect tubing

The table below shows the tubing and connectors to be used with UV monitor **U9-L**.

Note: If a second UV monitor is used, the tubing for this has to be cut manually.

Tubing label	Connection	Tubing		Connector	Tubing length (mm)
		ÄKTA pure 25	ÄKTA pure 150		
6	Tubing to UV monitor U9-L	PEEK, o.d. 1/16", i.d. 0.50 mm	PEEK, o.d. 1/16", i.d. 0.75 mm	Fingertight connector, 1/16"	160
7	Tubing from UV monitor U9-L	PEEK, o.d. 1/16", i.d. 0.50 mm	PEEK, o.d. 1/16", i.d. 0.75 mm	Fingertight connector, 1/16"	170

Note: To perform a run with the flow in reverse direction through UV monitor **U9-L**, a longer tubing **7** is needed. Replace the 170 mm tubing from the UV monitor with tubing that is 210 mm long and adjust the delay volume accordingly. For example, changing from 170 mm to 210 mm for 0.5 mm i.d. tubing increases the delay volume with 8 µl.

2.4.14 Conductivity monitor

Function of the Conductivity monitor

The Conductivity monitor continuously measures the conductivity of buffers and eluted proteins. The monitor is labelled **C9**.


The Conductivity flow cell has two electrodes positioned in the flow path of the cell. An alternating voltage is applied between the electrodes and the resulting current is measured and used to calculate the conductivity of the eluent.

The conductivity is automatically calculated by multiplying the measured conductance by the cell constant of the flow cell. The cell constant is factory-calibrated on delivery but can be re-calibrated if needed, see [Section 7.7.3 Calibrate the Conductivity monitor, on page 305](#).

As variation in temperature influences conductivity readings, the conductivity flow cell is fitted with a temperature sensor that measures the temperature of the eluent. A temperature compensation factor is used to report the conductivity in relation to a set reference temperature.

Location and illustration of the Conductivity monitor

The illustration below shows the recommended location of Conductivity monitor **C9**, together with a detailed view of the monitor.

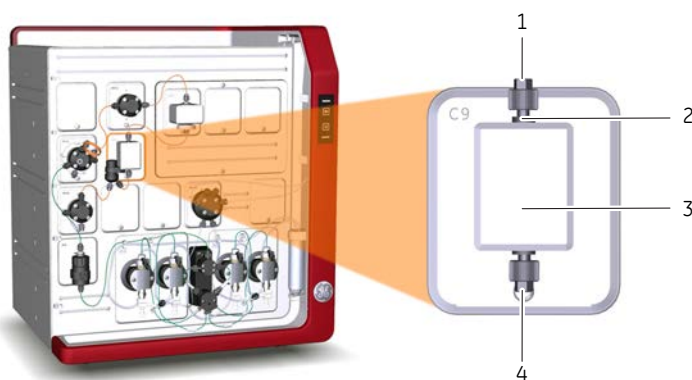

Part	Description
1	Inlet
2	Conductivity flow cell
3	Conductivity monitor
4	Outlet

Connect tubing

The table below shows recommended tubing and connectors.

Tubing label	Connection	Tubing		Connector	Tubing length (mm)
		ÄKTA pure 25	ÄKTA pure 150		
7	UV monitor U9-L to Conductivity monitor C9	PEEK, o.d. 1/16", i.d. 0.50 mm	PEEK, o.d. 1/16", i.d. 0.75 mm	Fingertight connector, 1/16"	170
8	Conductivity monitor C9 to Flow restrictor	PEEK, o.d. 1/16", i.d. 0.50 mm	PEEK, o.d. 1/16", i.d. 0.75 mm	Fingertight connector, 1/16"	95

2.4.15 Flow restrictor

Function of Flow restrictor FR-902


The Flow restrictor is included in the flow path to generate a steady back pressure of approximately 0.2 MPa, to prevent formation of air bubbles in the UV flow cell.

Note: Do not remove the flow restrictor to lower the pressure in the system. There is a risk that air bubbles cause large disturbances in the UV flow cell. Use the automatic pressure control function to avoid pressure alarms, see [Recommended pressure control parameters, on page 500](#)

Location and illustration of Flow restrictor FR-902

The Flow restrictor is normally included in the flow path after the Conductivity monitor. The Conductivity monitor is equipped with a special holder for the Flow restrictor.


The illustration below shows Flow restrictor **FR-902** fitted on the Conductivity monitor.

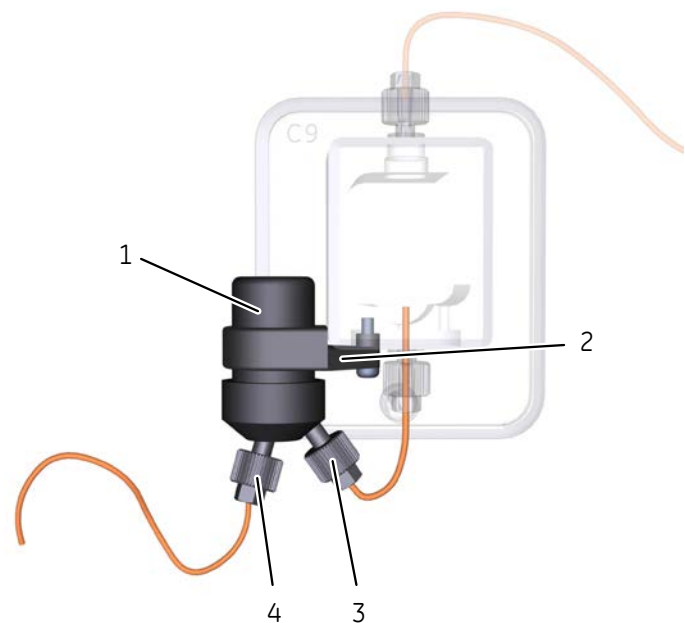

Part	Function
1	Flow restrictor
2	Holder
3	Inlet
4	Outlet

If ÄKTA pure is fitted with pH valve **V9-pH** or **V9H-pH** the Flow restrictor has to be moved from the Conductivity monitor to the pH valve.

The illustration below shows Flow restrictor **FR-902** fitted on the pH valve.

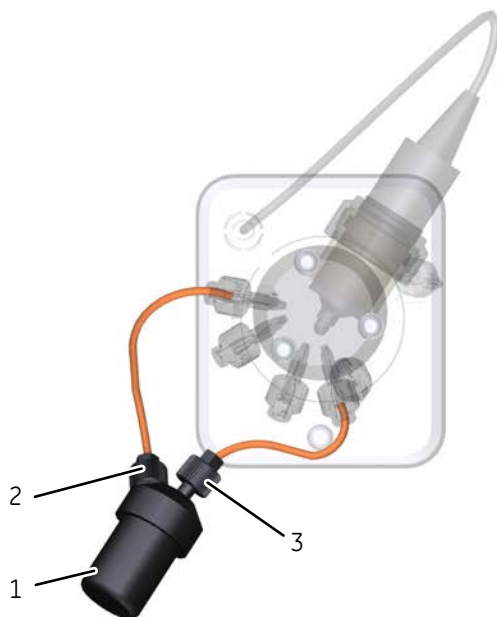

Part	Function
1	Flow restrictor
2	Flow restrictor inlet connection from pH valve ToR port
3	Flow restrictor outlet connection to pH valve FrR port

2.5 Installation of internal modules

Introduction

Optional modules and valves are easy to install in the instrument. The existing module or Module Panel is removed with a Torx T20 screwdriver and the cable is disconnected. The cable is then connected to the optional module, which is subsequently inserted into the instrument. The newly installed module is then added to the **System properties** in UNICORN.


Node ID

All of the available optional modules are preconfigured to give the desired function. However, the function of a module or valve can be changed by changing its Node ID. Node ID is a unit number designation that is used by the instrument to distinguish between several units of the same type.

In a troubleshooting situation it may be useful to check a valve's or module's Node ID. Refer to [Section 9.16 Node IDs, on page 501](#) for a list of Node IDs for valves and modules.

Note: *The function of a valve or module is defined by its Node ID, not by its physical position.*

The Node ID is set by positioning the arrows of the one or two rotating switches at the back of the valve. Use a screwdriver to set the arrows of the switches to the desired number.

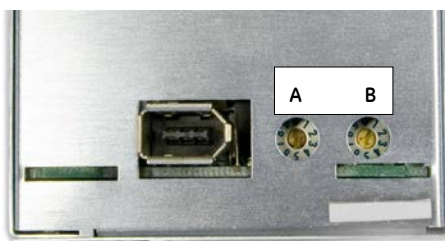

The illustration shows an example of a valve module with two rotating switches.

- The first rotating switch, labeled **A**, sets the tens
- The second switch, labeled **B**, sets the units.

Hardware installation of a module

The instruction below describes how to install a module in the instrument.

Note: *The illustrations show the principle how to install an optional module. The position of the module on the instrument and the used type of module will depend on the module being installed.*



CAUTION

Disconnect power. Always switch off power to the ÄKTA pure instrument before replacing any of its components, unless stated otherwise in the user documentation.

Step	Action
1	Disconnect power from the instrument by switching off the instrument power switch.
2	Loosen the connectors and remove the tubing from the existing module. Note: <i>This step does not apply for a Module Panel.</i>
3	Loosen the module with a Torx T20 screwdriver.



- 4 Remove the module.



- 5 Disconnect the cable and secure it in the slit.




Step	Action
------	--------


- | | |
|---|--|
| 6 | Connect the cable to the module to be installed. |
|---|--|



- | | |
|---|--------------------|
| 7 | Insert the module. |
|---|--------------------|

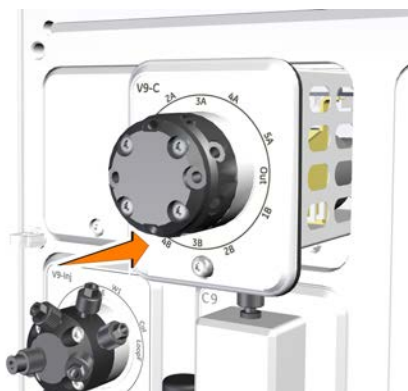

- | | |
|---|--|
| 8 | Fasten it with a Torx T20 screwdriver. |
|---|--|

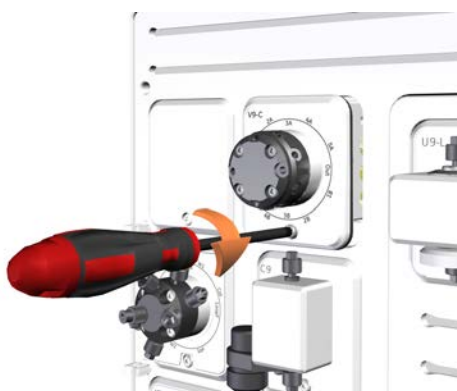

Note: A warning message is displayed at start up if a module has been installed in the instrument but not added to the current system configuration in UNICORN.

Install internal modules in the Extension box

The Extension box can be used to install extra modules on the ÄKTA pure instrument. See [Extension box, on page 85](#) for more information.


2.6 Accessories

Introduction

This section describes the holders and other available accessories. These are used to attach and organize columns, tubing and bottles to the ÄKTA pure instrument. The holders are attached to the instrument using the holder rails on the left side and the front of the instrument.

Rail extension

The Rail extension rod can be used to attach accessories, eg., column holders or a Multi-purpose holder. The rod has extra rails on both sides. Push the button of the rod to attach it to a holder rail. The illustration below shows the Rail extension rod.

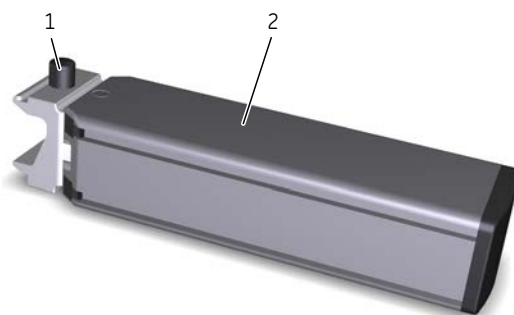


Part	Function
1	Button
2	Extension rod

Multi-purpose holder

The Multi-purpose holder can be used to attach accessories, eg., a Loop holder or a cassette. Attach the holder to a holder rail.

The illustration below shows the Multi-purpose holder.

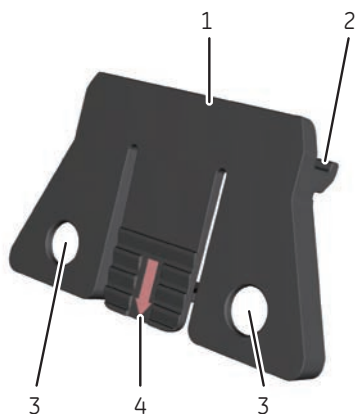

Part	Function
1	Attachment point for accessories
2	Snap-in to holder rails
3	Attachment points for tubing holders
4	Tab

Loop holder

The Loop holder can be used to attach up to five 10 ml sample loops. Use two Multi-purpose holders to attach the holder to a holder rail.

The illustration below shows the Loop holder.




Part	Function
1	Upper attachment to multi-purpose holder
2	Lower attachment to multi-purpose holder

Column holder

The Column holder has one position for medium sized columns and one position for small sized columns. The Column holder can also be used for bottles. Use two holders to attach long columns.


The illustration below shows the Column holder.

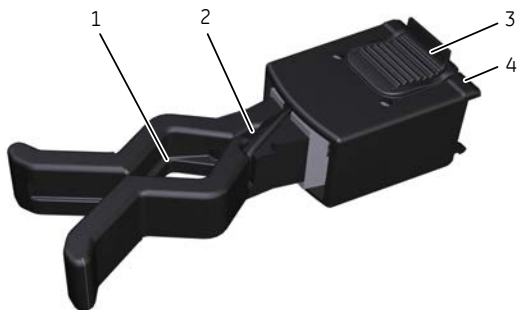

Part	Description
1	Position for a medium sized column or bottle
2	Position for a small sized column
3	Tab
4	Snap-in to holder rails

Column clamp

The column clamp can be used to attach small sized columns. Use two clamps to attach long columns. The illustration below shows the Column clamp.

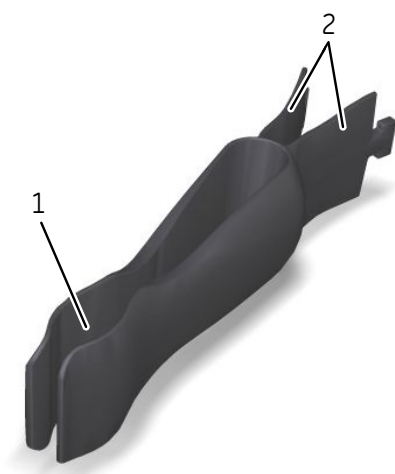


Part	Description
1	Position for a column
2	Inner end tabs

Column holder rod

The Column holder rod can be used to attach several HiTrap™ columns. The holder has threaded ports for HiTrap columns and tubing connectors. Push the button of the holder to attach the holder to a holder rail.


The illustration below shows the Column holder rod.

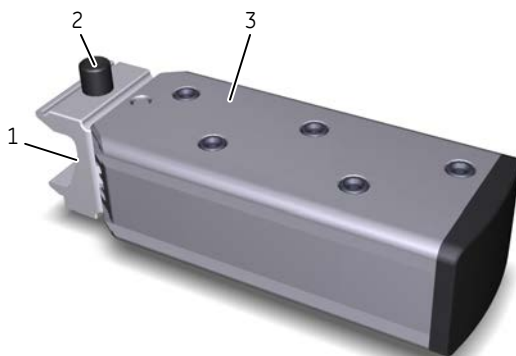

Part	Description
1	Snap-in to holder rails
2	Button
3	Column holder rod

Flexible column holder


The Flexible column holder can be used to attach, for example, HiScreen™ columns.
The illustration below shows the Flexible column holder.

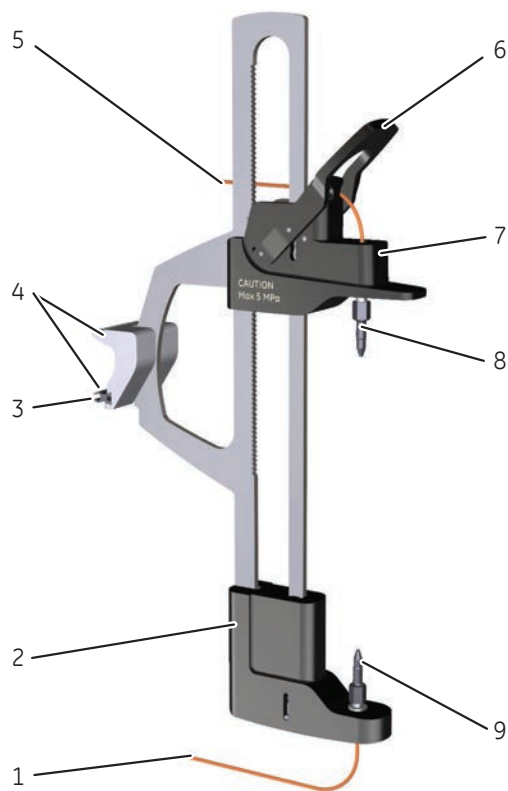

Part	Function
1	Lower tubing
2	Lower part
3	Snap-in-strips
4	Attachment part
5	Upper tubing
6	Lever
7	Upper part
8	Upper connector
9	Lower connector

Tubing holder spool

The Tubing holder spool is used to hold and arrange tubing.
The illustration below shows the Tubing holder spool.

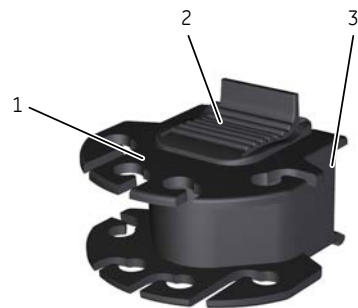

Part	Description
1	Positions for tubing
2	Tab
3	Snap-in to holder rails

Tubing holder comb

The Tubing holder comb is used to hold and arrange tubing.
The illustration below shows the Tubing holder comb.



Part	Description
1	Positions for tubing
2	Tab
3	Snap-in to holder rails

Bottle holder


The Bottle holder is used for holding bottles. For example, the Bottle holder can be attached to the holder rails to hold a sample bottle.
The illustration below shows the Bottle holder.



Part	Description
1	Position for bottle
2	Snap-in to holder rails

Adapter for air sensor

The adapter for air sensor is used to hold an optional air sensor.
The air sensor with adapter is connected to the Bottle holder, see illustrations below.

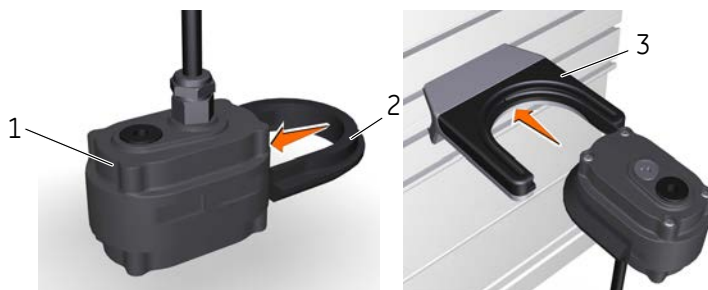

Part	Description
1	Air sensor
2	Air sensor adapter
3	Bottle holder

Module Panel

Description


All positions in ÄKTA pure must be occupied. Positions not used for core or optional modules must be fitted with a Module Panel.

Module Panels are installed in the same way as the other optional modules and the cable inside must be connected to the Module Panel, see [Hardware installation of a module, on page 76](#).

When an optional module is replaced by a Module panel, the removed module has to be deselected in the software configuration, see [Edit system properties, on page 125](#).

Illustration

The illustration shows the Module Panels installed in the example configuration used in this manual.

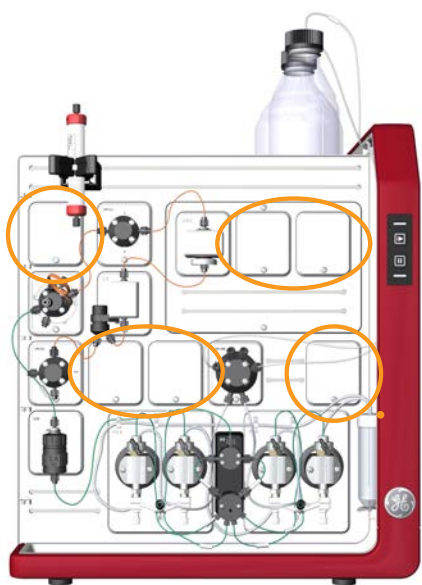


Extension box

Description

The Extension box can be used to install extra modules on the ÄKTA pure instrument outside the system chassis when the positions on the chassis are filled. It is possible to install up to six Extension boxes with extra modules when using ÄKTA pure. See the Extension box instruction for more information.

Location

The illustration below shows an Extension box with a module mounted on the side of ÄKTA pure.

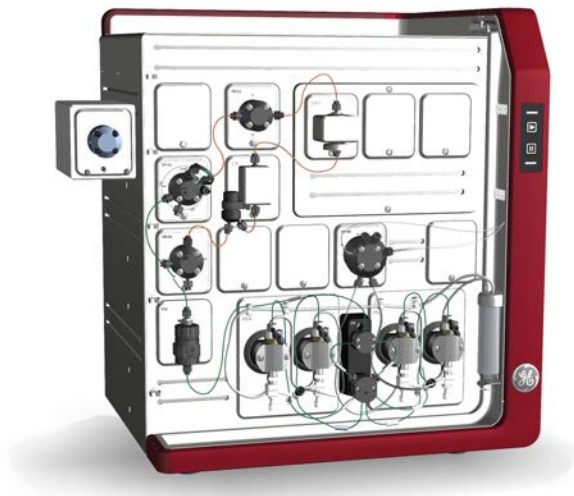

The Extension box can be mounted in three ways.

- On the side of ÄKTA pure.
- Standing on top of or next to ÄKTA pure.
- On a Rail extension rod (29-0113-52) on ÄKTA pure.

3 ÄKTA pure external modules

About this chapter

This chapter provides an overview of the external modules that can be connected to the ÄKTA pure instrument. A brief description of how to connect external modules is also provided.

In this chapter

This chapter contains the following sections:

Section	See page
3.1 External air sensors	87
3.2 Fraction collector F9-C	89
3.3 Fraction collector F9-R	103
3.4 Sample pump S9 and S9H	107
3.5 I/O-box E9	111
3.6 Connection of external modules	119

3.1 External air sensors

Introduction

Up to four external air sensors can be added to ÄKTA pure, and there are two different versions to choose from. They differ in internal diameter and optimal position on the instrument.

The air sensors can be attached to the instrument using the rails and holders, see [Adapter for air sensor, on page 83](#). No Module Panels need to be removed.

In addition to be used for preventing air from entering the system, the external air sensors can be used together with System pump A, or an Sample pump to load the entire sample volume.

Air sensor L9-1.5

L9-1.5 has a 1.5 mm inner diameter and is designed for i.d. 1.6 mm FEP, ÄKTA pure 25, and for i.d. 2.9 mm FEP tubing, ÄKTA pure 150, at the low pressure side before the pumps. It is installed in the flow path before the system pumps or the sample pump and is used to prevent air entering the subsequent module.

Air sensor L9-1.2

L9-1.2 has a 1.2 mm inner diameter and is designed for o.d. 1/16" tubing at the high pressure side after the pumps. It is installed after the injection valve and is used to prevent air entering the column.

Note: **L9-1.2** can be used in the same fashion as **L9-1.5** if O.D. 1/16" ETFE tubing is used between the air sensor and the inlet valve.

Tubing connections

Air sensor L9-1.5

Connection between...	Tubing		Connector		Tubing length (mm)
	ÄKTA pure 25	ÄKTA pure 150	ÄKTA pure 25	ÄKTA pure 150	
L9-1.5 and inlet valves	FEP, o.d. 1/8", i.d. 1.6 mm	FEP, o.d. 3/16", i.d. 2.9 mm	Tubing connector, 5/16" + Ferrule (yellow), 1/8"	Tubing connector, 5/16" + Ferrule (blue), 3/16"	See note

Note: When sample is loaded at high flow rate and the external air sensor is placed before the pump that is used for loading the sample, it is necessary to use longer tubing to ensure that no air reaches the pump. Use tubing with the minimum lengths given below between the valve located before the pump and the external air sensor. The length applies for maximum flow rate, but shorter tubing can be used at lower flow rates.

- Sample pump S9: 40 cm.
- Sample pump S9H: 20 cm.

Air sensor L9-1.2

Connection between...	Tubing	Connector	Tubing length (mm)
Injection valve and L9-1.2	PEEK, o.d. 1/16"	Fingertight connector, 1/16"	100
L9-1.2 and Column valve/the connected column	PEEK, o.d. 1/16"	Fingertight connector, 1/16"	100

3.2 Fraction collector F9-C

About this section

This section describes the design and function of **Fraction collector F9-C**.

In this section

This section contains the following subsections:

Section	See page
3.2.1 Function	90
3.2.2 Fraction collector F9-C illustrations	92
3.2.3 Cassettes, Cassette tray and racks	96
3.2.4 Connect tubing to the ÄKTA pure instrument	102

3.2.1 Function

Introduction

Fraction collector F9-C can collect fractions in deep well plates, tubes of different sizes or bottles. Up to six cassettes for deep well plates and tubes can be used. The cassettes can be used in any combination and are placed on the Cassette tray. A rack for 50 ml tubes and a rack for 250 ml bottles are also available.

Scanner functions detect which types of trays, racks, cassettes and deep well plates that are used in each run.

The Cassette tray or one of the racks is placed inside the fraction collector. A height exclusion bar ensures that the bottles, tubes and deep well plates are correctly positioned and cannot damage the Dispenser head. The Tray catch and positioning discs on the floor of the fraction collector guide the Cassette tray or the rack into the correct position.

Scanning of Cassettes

When the door of the fraction collector is closed automatic scanning is performed. There are two types of scanning procedures:

- **Full scan:** Scanning of Cassette type codes to determine which types of Cassettes are used, and scanning of rows and columns in deep well plates to identify which types of plates are used (24, 48, or 96 wells). Full scan is performed only when the system is in state **Ready**.
 - **Quick scan:** Scanning of Cassette type codes to determine which type of Cassettes are used. Quick scan is performed during the run to ensure that correct Cassettes are placed in the Fraction collector.
-

Fractionation modes to avoid spillage

Three fractionation modes are available, all of which avoid spillage between wells or tubes during fractionation:

- **Accumulator:** The accumulator is used to collect liquid during movement between wells, tubes or bottles. The liquid is then dispensed in the next well or tube. Fractionation with accumulator can be used at all flow rates.
 - **DropSync:** When using **DropSync** the sensors in the Dispenser head detect when a drop is released from the nozzle. The Dispenser head moves to the next well or tube just after a drop is released. Fractionation with **DropSync** can be used at flow rates up to 2 ml/min. If the cassettes are placed near the waste funnel the **DropSync** mode can be used at higher flow rates. Volatile solutions and solutions with low surface tension may require a lower flow.
 - **Automatic:** The fraction collector uses the Drop Sync mode for flow rates up to 2 ml/min and automatically switches to Accumulator mode for higher flow rates.
-

Fractionation arm positions

- **Home position:** The home position is used when the fraction collector is idle. The Fractionation arm is positioned in the front of the interior of the fraction collector and the Dispenser head is positioned over the waste funnel. This position is called **Waste (Frac)** in UNICORN.
 - **Frac cleaning position:** The Frac cleaning position is used for convenient cleaning of the Dispenser head. The Fractionation arm is positioned in the front of the interior of the fractionation collector and the Dispenser head is moved to the center of the Fractionation arm.
-


3.2.2 Fraction collector F9-C illustrations

Introduction

This section provides illustrations of Fraction collector F9-C. The main features and components are indicated.

Front view

The illustration below shows the main parts of the exterior of Fraction collector F9-C.

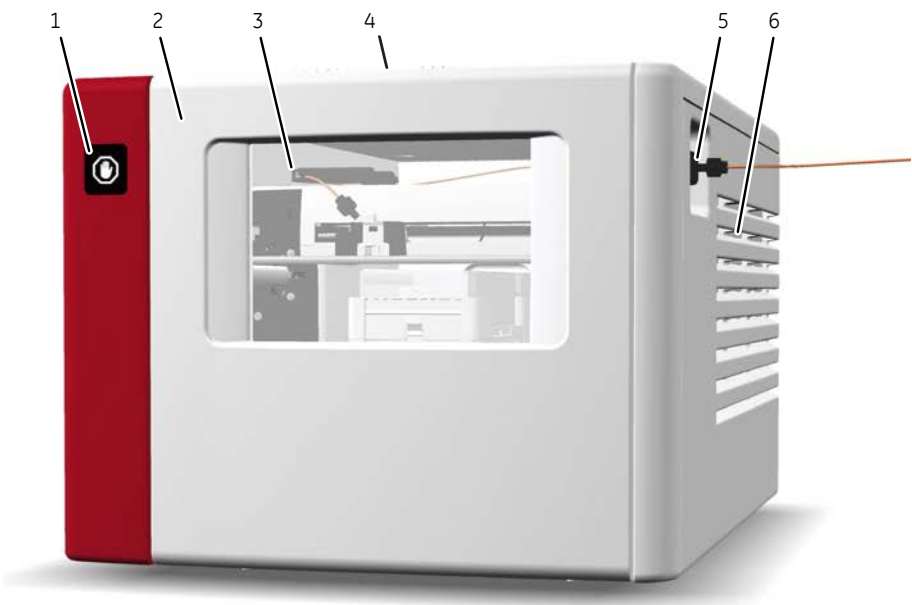

Part	Description
1	Fractionation indicator Symbol indicating that fractionation is ongoing. Do not open the door while the indicator is lit.
2	Door
3	Window
4	Door handle
5	Tubing connector for outlet valve tubing
6	Vents

Rear view


The illustration below shows the rear view of Fraction collector F9-C.



Part	Description
1	Vents
2	UniNet-9 D-type connector (for communication and power supply)
3	Waste tube

Interior


The illustration below shows the main parts of the interior of Fraction collector F9-C.

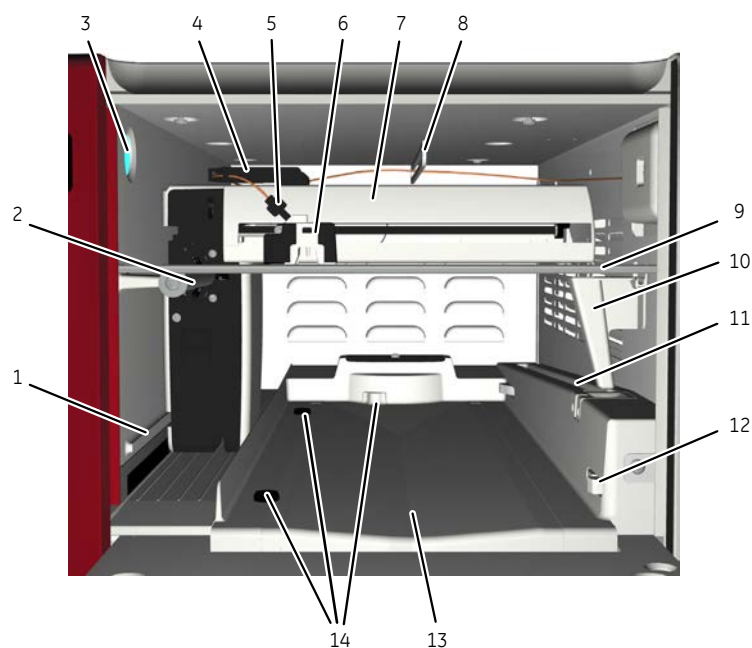

Part	Description
1	Fractionation arm guide rail
2	Fractionation arm main rail
3	Lamp
4	Tubing guide
5	Tubing connection
6	Dispenser head
7	Fractionation arm
8	Tubing guide
9	Height exclusion bar
10	Waste funnel
11	Waste tube
12	Tray catch
13	Waste groove, in case of overflow
14	Tray guides

Dispenser head

The illustration below shows the Dispenser head of Fraction collector F9-C.

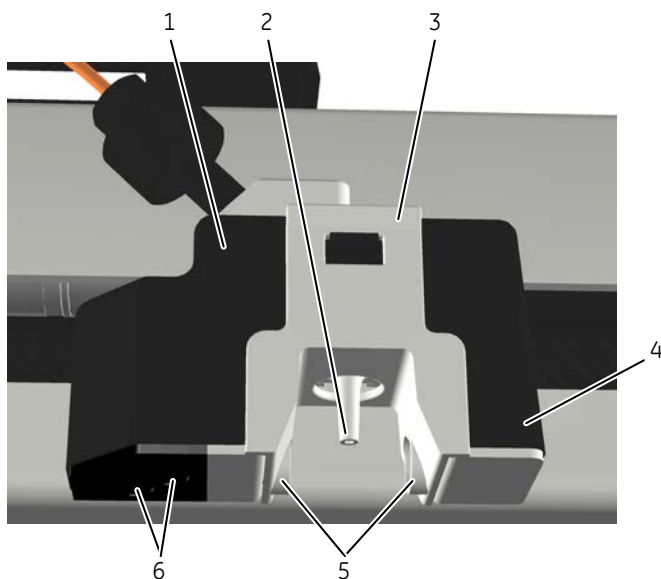

Part	Description
1	Dispenser head
2	Nozzle
3	Dispenser head cover
4	Accumulator (back part of Dispenser head)
5	Drop sync sensor
6	Type code reader

3.2.3 Cassettes, Cassette tray and racks

Introduction

Fractions can be collected in deep well plates and in tubes of different sizes. A number of cassettes and racks for different tubes and deep well plates are available. The cassettes are placed on a rack with six cassette positions. The Cassette type codes are scanned by the Cassette code reader to determine the type of Cassette.

Available cassettes, trays and racks

The following Cassettes and racks are available:


- Cassette 3 ml tubes (for 40 tubes)
- Cassette 8 ml tubes (for 24 tubes)
- Cassette 15 ml tubes (for 15 tubes)
- Cassette 50 ml tubes (for 6 tubes)
- Cassette for deep well plate (24, 48, 96 wells)
- Cassette tray (for six cassettes)
- Rack for 50 ml tubes (for 55 tubes)
- Rack for 250 ml bottles (for 18 bottles)

For information on dimension requirements for tubes and deep well plates to be used in the fraction collector, see [Fraction collector tubes and bottles, on page 99](#) and [Deep well plates, on page 100](#) respectively.


Illustrations of Fraction collector F9-C tray and racks

The illustrations below show the Cassette tray, the Rack for 50 ml tubes and the Rack for 250 ml bottles. The fronts of the tray and the racks are marked with the GE-logotype.


In the Cassette tray, the cassette positions are marked 1 to 6.

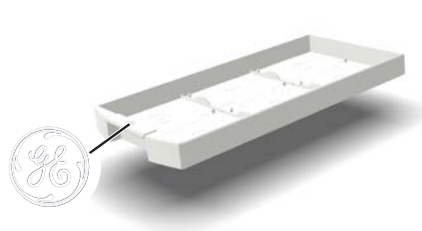

Cassette tray

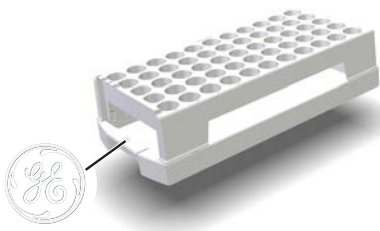

Rack for 50 ml tubes

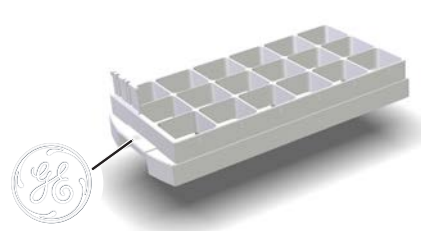


Rack for 250 ml bottles

Note: The tray and racks are inserted into the fraction collector with the GE-logotype facing outwards.

Note: Do not use the Cassette tray when a rack for tubes or bottles is placed in the fraction collector.

Illustration of Cassettes on the Cassette tray

The illustration below shows Cassettes placed on the Cassette tray.

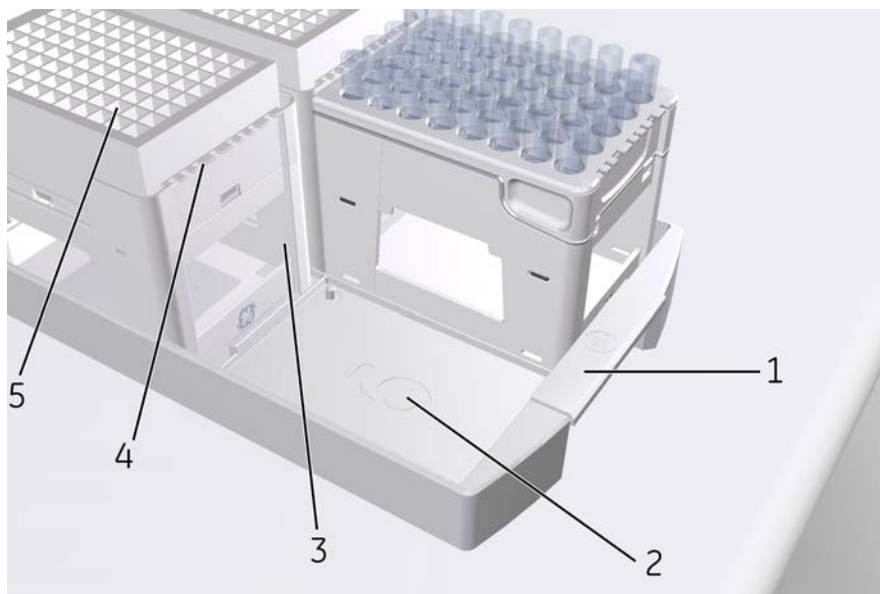


Part	Description
1	Cassette tray
2	Cassette position number
3	Cassette
4	Cassette type code
5	Tubes or deep well plates placed in a Cassette

QuickRelease function

The Cassettes for the smaller tube sizes (3, 8, and 15 ml) have a built-in QuickRelease function. The QuickRelease function enables easy handling of tubes in the Cassettes. With the QuickRelease device in lock position the tubes are fastened in the Cassette and can easily be emptied. With the QuickRelease function in release position, the Cassette can easily be loaded with tubes and used tubes can easily be discarded.

Step	Action
1	Load the Cassette with tubes before fractionation: • Pull the QuickRelease device to the release position. • Load the Cassette with tubes, and press the QuickRelease device to the locked position.

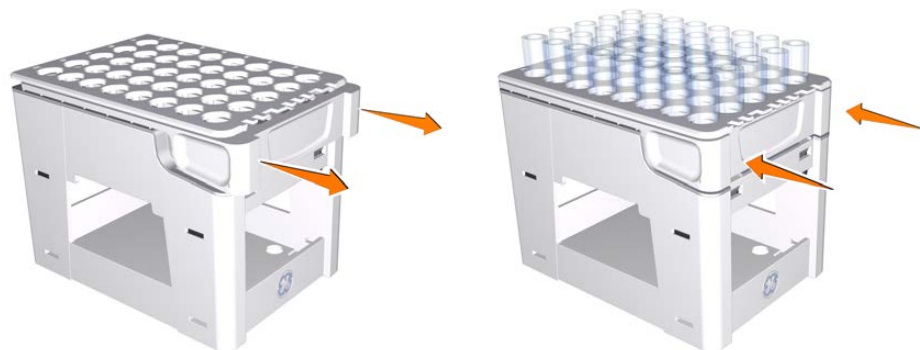

Release position

Locked position

3	After fractionation, pull the QuickRelease device to the release position and remove the tubes containing the fractions of interest.
---	--

Step	Action
------	--------

- | | |
|---|--|
| 4 | <p>Empty and discard the remaining tubes:</p> <ul style="list-style-type: none"> Press the QuickRelease device to the lock position, and empty the remaining tubes. Pull the QuickRelease device to the release position, and discard the tubes. |
|---|--|



Empty the tubes



Discard the tubes

Fraction collector tubes and bottles

The tubes and bottles used in Fraction collector F9-C must fulfill the requirements listed in the table below. Examples of manufacturers are also listed in the table.

Tube/bottle size [ml]	Diameter [mm]		Height [mm]		Max. volume [ml]	Examples of manufacturers
	Min.	Max.	Min.	Max.		
3	Ø: 10.5	Ø: 11.5	50	56	3	NUNC
8	Ø: 12	Ø: 13.3	96	102	8	BD Biosciences, VWR
15	Ø: 16	Ø: 17	114	120	15	BD Biosciences
50	Ø: 28	Ø: 30	110	116	50	BD Biosciences
250	L: 55 W: 55	L: 64.5 W: 64.0	-	121	250	Nalgene™ Kautex™

Maximum flow rate

Fraction collection can be performed at different maximum flow rates depending on the size of the tubes that are used. The table below lists the maximum flow rates for the Fraction collector tubes.

Tube size [ml]	Maximum flow rate [ml/min]
3	15
8	25
15	50
50	150
250	150

Deep well plates

Requirements

The deep well plates used in Fraction collector F9-C must fulfill the requirements listed in the table below.

Property	Specification
No. of wells	24, 48, or 96
Shape of wells	Square, not cylindrical
Well volume	10, 5, or 2 ml

Approved deep well plates

The plates listed in the table below are tested and approved by GE to be used with Fraction collector F9-C.

Plate type	Manufacturer	Part no.
96 deep well plate	GE	7701-5200 (Whatman™)
	Eppendorf™	951033405/ 0030 501.306
	BD Biosciences	353966
	Greiner Bio-One	780270
	Porvair Sciences	219009
	Seahorse Bioscience™	S30009
48 deep well plate	GE	7701-5500 (Whatman)
	Seahorse Bioscience	S30004

Plate type	Manufacturer	Part no.
24 deep well plate	GE	7701-5102 (Whatman)
	Seahorse Bioscience	S30024

Maximum flow rate

Fraction collection can be performed at different maximum flow rates depending on what type of deep well plates that are used. The table below lists the maximum flow rates for the different plate types.

Plate type	Maximum flow rate [ml/min]
96 deep well plate	10
48 deep well plate	15
24 deep well plate	25


3.2.4 Connect tubing to the ÄKTA pure instrument

Connect tubing

Fraction collector F9-C is delivered with all internal tubing in place. The tubing between the fraction collector and ÄKTA pure need to be installed.

Follow the instructions in the table below to connect the tubing from the ÄKTA pure instrument to the fraction collector.

Step	Action
1	Connect the tubing Frac to the Frac port on the outlet valve on the ÄKTA pure instrument.
2	Connect the other end of the Frac tubing to the inlet port on the fraction collector.

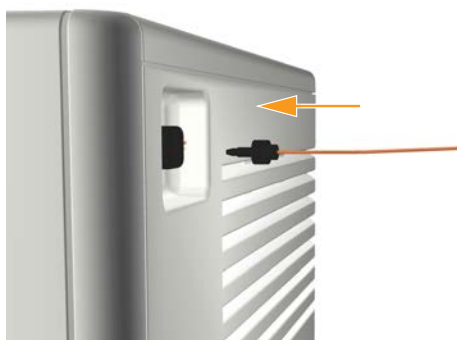

3	Adjust the delay volume setting in UNICORN, see Section 9.8.8 System settings - Tubing and Delay volumes, on page 458 for more details.
---	---

3.3 Fraction collector F9-R

About this section

This section shows an overview of Fraction collector F9-R.

Technical details are found in [Fraction collector options, on page 417](#).

Function

The fraction collector collects fractions from ÄKTA pure purification runs.

The fraction collector can be used for:


- Fixed volume fractionation
- Peak fractionation
- Combined fixed volume fractionation and peak fractionation

Fraction collector F9-R has the following function for reducing sample spill during fractionation:

- Drop Sync

Front view illustration

The illustration below shows the main parts of the Fraction collector.

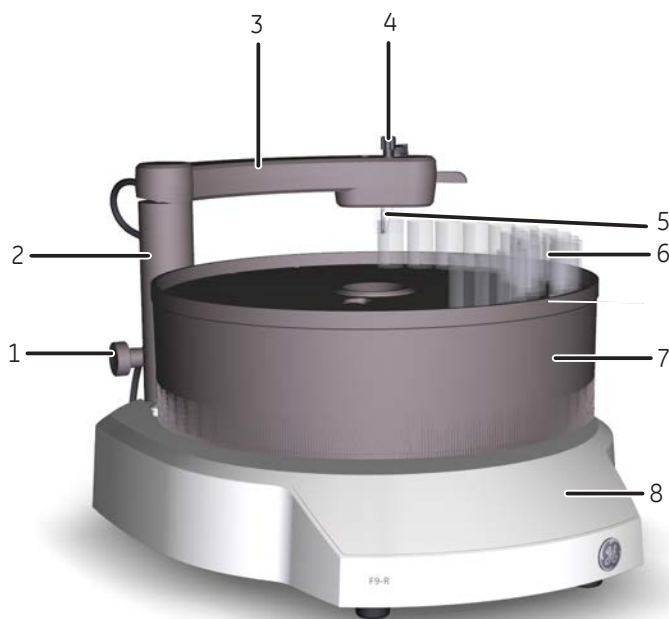

Part	Function
1	Lock knob
2	Stationary part of delivery arm
3	Delivery arm
4	Tubing connector
5	Tube sensor
6	Collection tubes
7	Tube rack
8	Base unit

Connector panel illustration

The illustration below shows the main parts of the connector panel on the fraction collector.



Part	Function
1	Node ID switch
2	UniNet-9 F-type connector (for communication and power supply)

Available tubes

For Fraction collector F9-R the fractions are collected in tubes of different sizes.


Tubes with the following diameter can be used with Fraction collector F9-R:

- 12 mm
- 18 mm
- 30 mm

The tubes can have a tube length between 50-180 mm.

Illustration of the Fraction collector F9-R Tube rack

Each tube rack is made up of a combination of a Bowl, Tube support, Tube guide and Tube holder. For more information on the assembly of the tube rack, see [Assemble the Tube rack, on page 197](#). For information on which Tube rack to use, see [Tube rack inserts, on page 198](#).

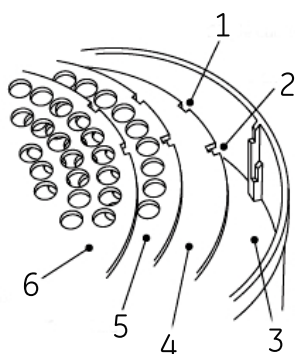


Part	Function
1	Single cutout
2	L-shaped cutout
3	Bowl
4	Tube support
5	Tube guide
6	Tube holder

Note: Note that the tube guide has both single and L-shaped cutouts, while the tube holder only has single cutouts. See [Single and L-shaped cutouts, on page 198](#) for more information.

Connect tubing to the ÄKTA pure instrument

Step	Action
------	--------

- | | |
|---|---|
| 1 | Lift out the Tubing holder (4) from the Delivery arm (1). |
|---|---|

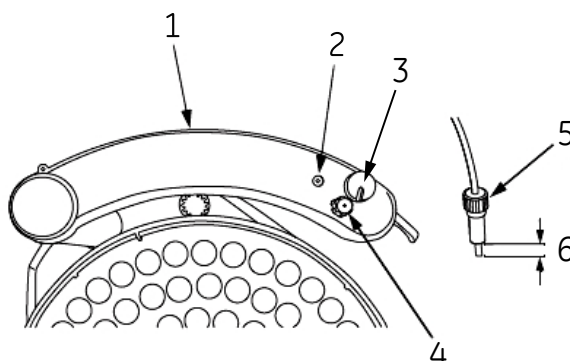

- | | |
|---|--|
| 2 | Loosen the nut of the Tubing holder. Do not remove the Tubing holder nut (5) from the Tubing holder. |
| 3 | Insert the tubing through the Tubing holder. |
| 4 | Place the Tubing holder with the tubing over the Tube adjustment cavity (2) of the Delivery arm. Push the tubing down against the bottom of the Tube adjustment cavity, and then fingertighten the Tubing holder nut. This ensures the correct length of the exposed tubing end (6). |
| 5 | Re-install the tubing holder in the Delivery arm. |
| 6 | For Fraction collector F9-R : Connect the tubing from the fraction collector to the port Frac on the outlet valve.
For Fraction collector F9-R, 2nd : Connect the tubing from the second fraction collector to:
<ul style="list-style-type: none"> port Out 10 on Outlet valve V9-O or V9H-O port Out 1 on Outlet valve V9-Os or V9H-Os |
| 7 | Adjust the delay volume setting in UNICORN to the volume of the tubing, see Section 9.8.8 System settings - Tubing and Delay volumes, on page 458 for more details. |

3.4 Sample pump S9 and S9H

Introduction

This section describes the design and function of Sample pump S9 and S9H.

Function of the Sample pump


The Sample pump is dedicated to direct loading of sample onto a column, or to filling of sample loops or Superloops. The pump consists of two pump heads that work alternately to give a continuous, low pulsation, liquid delivery. There are two sample pump configurations available, one for ÄKTA pure 150 and one for ÄKTA pure 25. To ensure delivery of correct liquid volume, the pumps must be free from air. Each pump head is equipped with a purge valve that is used for this purpose.

The Sample pump also comprises a pressure monitor.

The table below contains the operating limits and labels of the sample pump configurations.


Configuration	Pump label	Pump type	Flow rate	Max. pressure
Sample pump S9 , ÄKTA pure 25	P9-S	P9-S	0.001 to 50 ml/min	10 MPa
Sample pump S9H , ÄKTA pure 150	P9H S	P9H	0.01 to 150 ml/min	5 MPa

Front view

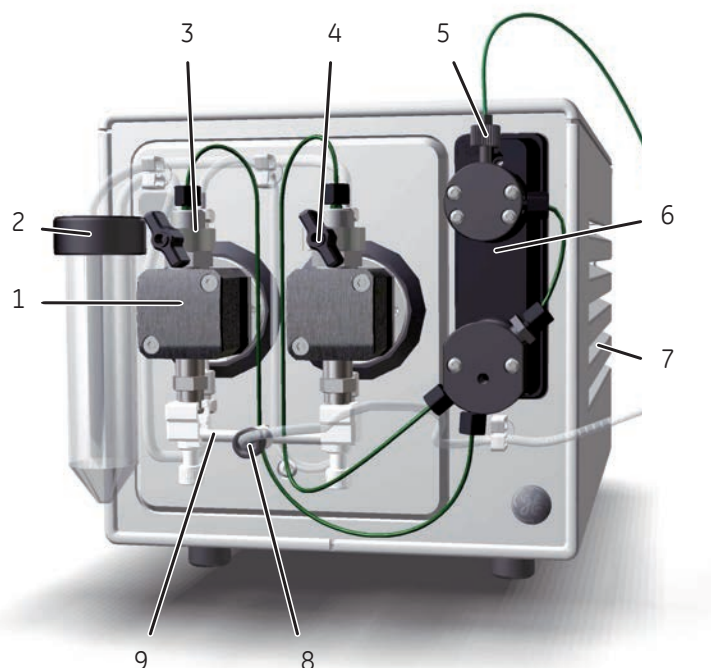

Part	Function
1	Pump head: Encapsulates the inner parts of the pump
2	Pump rinsing liquid tube holder
3	Outlet port with check valves
4	Purge valve: Used to remove air from the pump
5	Sample pump outlet port
6	Sample pressure monitor
7	Vents
8	Sample pump inlet port
9	Inlet manifold

Rear view

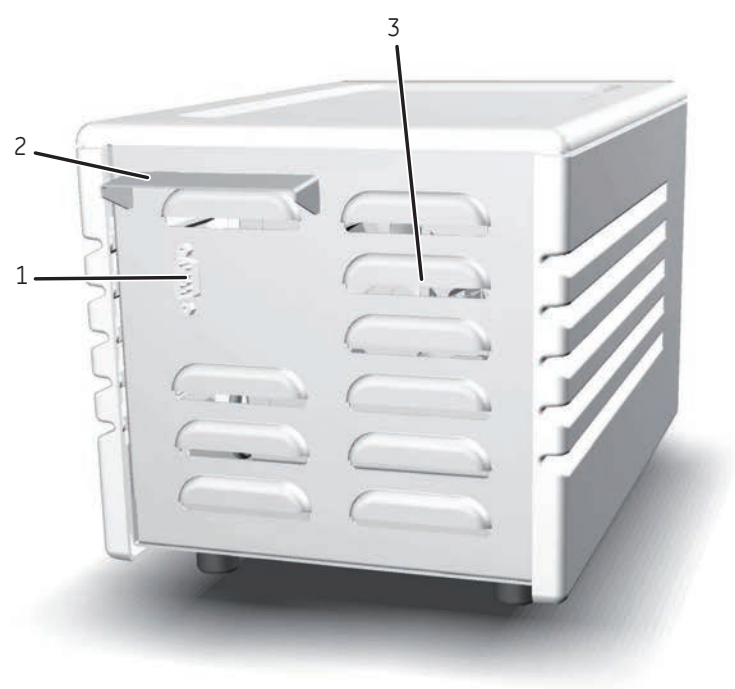

Part	Function
1	UniNet-9 type D port
2	IP cover: Protects pump electronics from liquid spill
3	Vents


Sample pump piston rinsing system

A seal prevents leakage between the pump chamber and the drive mechanism. The seal is continuously lubricated by the presence of solvent. The pump piston rinsing system continuously flushes the low pressure chamber behind the piston with a low flow of 20% ethanol. This prevents any deposition of salts from aqueous buffers on the pistons and prolongs the working life of the seals.


For instructions on how to fill the rinsing system, see [Section 7.3.1 Change pump rinsing solution, on page 259](#)

Illustrations of the sample pump piston rinsing system

The illustrations below show the parts, tubing and flow path of the sample pump piston rinsing system.

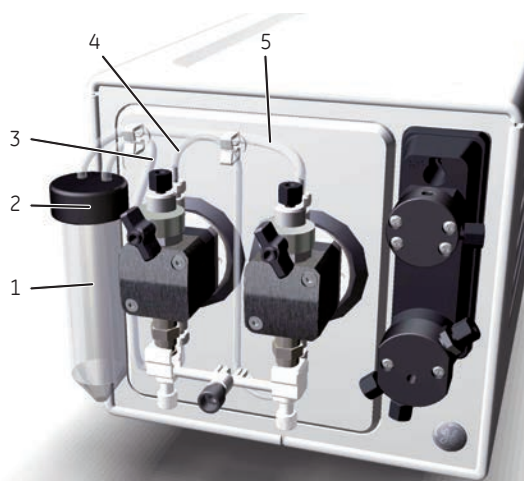

Parts and tubing



Rinsing system flow path

Part	Function
1	Pump rinsing liquid tube
2	Pump rinsing liquid tube holder
3	Inlet tubing, from the rinsing liquid tube to the left pump head (lower rinsing system connection) .
4	Tubing between the left pump head (upper rinsing system connection) and the right pump head (lower rinsing system connection).
5	Outlet tubing, from the right pump head (upper rinsing system connection) to the rinsing liquid tube.

Connect tubing to the ÄKTA pure instrument

The table below shows recommended tubing and connectors.

Tubing label	Connection	Tubing		Connector		Tubing length (mm)
		ÄKTA pure 25	ÄKTA pure 150	ÄKTA pure 25	ÄKTA pure 150	
InS	Sample inlet valve port Out to sample pump inlet manifold	FEP o.d. 1/8", i.d. 1.6 mm	FEP o.d. 3/16", i.d. 2.9 mm	Tubing connector 5/16" with Ferrule (yellow), 1/8"	Tubing connector 5/16" with Ferrule (blue), 3/16"	580
No label	Sample container to sample pump inlet manifold (sample inlet valve not used)	FEP o.d. 1/8", i.d. 1.6 mm	FEP o.d. 3/16", i.d. 2.9 mm	Tubing connector 5/16" with Ferrule (yellow), 1/8"	Tubing connector 5/16" with Ferrule (blue), 3/16"	optional
3S	Sample pump pressure monitor to Inlet valve port SaP	PEEK, o.d. 1/16", i.d. 0.75 mm	PEEK, o.d. 1/16", i.d. 1 mm	Fingertight connector, 1/16"	Fingertight connector, 1/16"	530

Note: The recommended location of the sample pump is on the bench to the left of the ÄKTA instrument. If the sample pump is placed elsewhere, longer tubing may be needed.

3.5 I/O-box E9

About this section

This section describes the design and the function of the I/O-box E9

In this section

This section contains the following subsections:

Section	See page
3.5.1 Overview of the I/O-box	112
3.5.2 Analog connector and signals	114
3.5.3 Digital connector and signals	116
3.5.4 Connect the I/O-box	118

3.5.1 Overview of the I/O-box


Function of the I/O-box

The **I/O-box E9** is used to interface other equipment in order to measure parameters such as refractive index, light scattering and fluorescence. See [Requirements on connected equipment, on page 118](#) for information on requirements of the equipment that can be connected to ÄKTA pure. The I/O-box can control external equipment by a digital output signal, as well as detecting the state of them by digital inputs. It is also possible to send out internal detector signals to external equipment.

It is possible to install up to two **I/O-box E9** when using ÄKTA pure. If two I/O-boxes are to be used, the second one has to be configured as I/O-box E9, 2nd. The configuration is defined by the I/O-box E9 Node ID.

Location

The illustration below shows the I/O-box, its recommended location and connection.

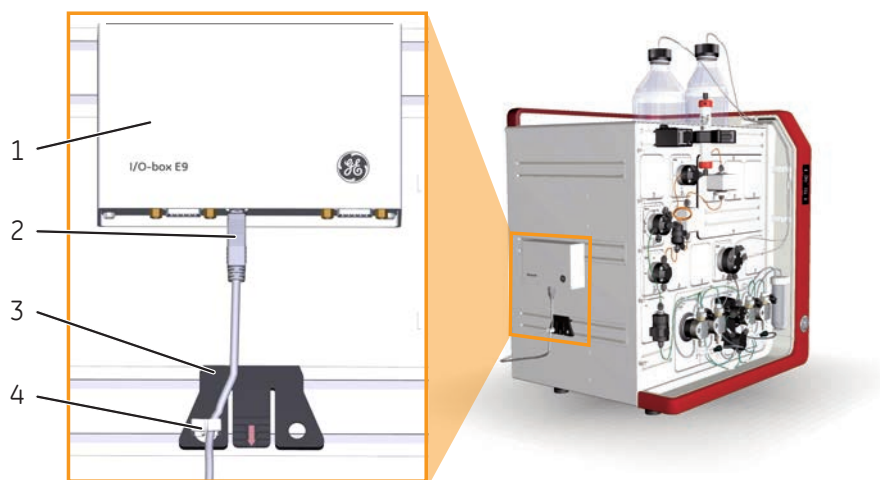

Part	Description
1	I/O-box
2	UniNet-9 F-type cable
3	Multi-purpose holder
4	Clip


Connectors



Part	Description
Analog in/out	Signal connector for analog input and output signals.
UniNet-9	Connector used to connect the I/O-box to the ÄKTA pure instrument.
Status	Status indicator for service purposes.
Node ID	Switches used to configure I/O-box E9 as I/O-box E9 or I/O-box E9, 2nd.
Digital in/out	Signal connector for digital input and output signals.

3.5.2 Analog connector and signals

Analog connector pins

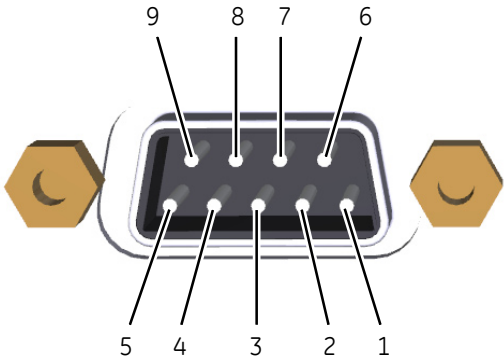

Part	Function
1	Analog in signal 1 +
2	Analog in signal 1 -
3	Signal ground
4	Analog in signal 2 +
5	Analog in signal 2 -
6	Calibration pin for service purposes Analog out signal (1.9 V) Note: <i>Do not use for other purposes.</i>
7	Analog out signal 1
8	Signal ground
9	Analog out signal 2

Analog signals

All analog input and output signals are confined to the same **Analog in/out** connector.

Analog input signals

There are two analog input channels from which analog input signals can be used for peak detection, or data collection in UNICORN. It is possible to auto-zero the input signals, which means that the current value will be displayed as 0 V in UNICORN. This can be done individually for the two analog input channels. The auto-zero value is saved between runs and power-offs. The auto-zero value can be reset.

Parameter	Description
Input signal range	-2000 to 2000 mV

Analog output signals


There are two analog output channels from which analog output signals and system parameters, that is, UV, cond, conc B, temperature and pH, are transferred to the external connected equipment, for example, light scattering detectors or plotters.

Parameter	Description
Output signal range	-1000 to 1000 mV
Default output	The user defines the default output level for the selected signal.
Full scale output	The user sets the desired output signal value of, e.g., mAU, % or mS, which will corresponds to the full scale output voltage 1000 mV.
Negative full scale output	The corresponding negative full scale output value is set automatically. For example, if the full scale output is set to 2000 mAU, a UV value of 500 mAU will give an output voltage of 250 mV, and -100 mAU will give -50 mV output voltage. A signal value of 0 mAU, 0% or 0 mS will always give an output voltage of 0 mV.
Fix point	Zero is always a fix point. A desired output signal of, i.e., 0 mAU, 0% or 0 mS corresponds to an output voltage of 0 mV. At power-on, an output signal of 0 mV is transferred to the connected equipment, until the output signal range values are set.

Note: No warning will be displayed in UNICORN if the analog output signal exceeds the set full scale output value or is less than the set negative full scale output value.

3.5.3 Digital connector and signals

Digital connector pins

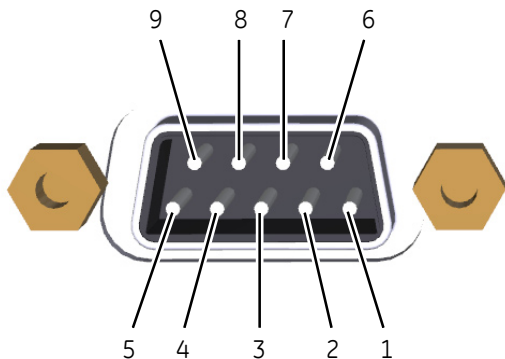

Part	Function
1	Digital in signal 1
2	Digital in signal 2
3	Digital in signal 3
4	Digital in signal 4
5	Signal ground
6	Digital out signal 1
7	Digital out signal 2
8	Digital out signal 3
9	Digital out signal 4

Digital signals

All digital input and output signals will be confined to the same D-sub connector and have a common ground. The four input signals will be scanned synchronously, and the outputs will be set synchronously.

Digital input signals

The digital in-signal can be used to monitor external equipment by registering, for example, error signals or event marks. An event mark can be used as a trigger for watches. The measured digital signals can be shown as a curve in UNICORN. The unit will handle both open/closed circuit and TTL-type voltage signals. An open circuit is interpreted as logical 1 and a closed circuit as logical 0.

Note: A closed circuit is always closed against signal ground.

Input connection	UNICORN interpretation
Open circuit	Logical 1
Applied voltage 3.5 to 5.0 V	
Closed circuit	Logical 0
Applied voltage 0 to 0.8 V	

Digital output signals

The digital output signal can be used to control external equipment that can receive digital signals, such as pumps or fraction collectors. The digital output signals define an open or closed circuit, where a logical 1 will result in an open circuit and a logical 0 will give a closed circuit. The default level, 1 or 0, is set by the user. The level can be changed by instructions either manually, in **System Settings** or by a method. It is possible to send pulses from the current level, with a pulse length of 0.1 s to 10 s.

Note: A closed circuit is always closed against signal ground.

3.5.4 Connect the I/O-box

Connect the I/O-box

See *Instructions - Install I/O box E9* for instructions on connecting the I/O-box to the instrument.

Requirements on connected equipment

The physical requirements for the connected equipment is described in the following tables. All connected equipment must have a common grounding.

Analog input

Parameter	Value
Channels	2
Range	± 2000 mV
Input impedance	1 M Ω
Accuracy	$\pm(0.1\% + 0.2$ mV)

Analog output

Parameter	Value
Channels	2
Range	± 1000 mV
Input impedance	100 k Ω
Accuracy	$\pm(0.3\% + 1$ mV)

Digital input

Parameter	Value
Channels	4
Compatibility	TTL, open/closed circuit

Digital output

Parameter	Value
Channels	4
Compatibility	Open/closed circuit

3.6 Connection of external modules

Introduction

The external modules are not installed in the instrument cabinet, but are connected via a UniNet-9 cable at the back of the system. It is possible to install up to six external modules with F-type connectors and up to two external modules with D-type connectors at the same time.

Some of the external modules are also connected to the ÄKTA pure instrument by tubing. See the appropriate section in [Chapter 3 ÄKTA pure external modules, on page 86](#) for detailed instructions on how to install this tubing, if applicable.

F-type and D-type connectors

The illustrations below show the F-type and D-type connectors.



F-type



D-type

Constraints

The table below indicates usage constraints for the different external modules.


External module	Connector	Constraints
I/O-box E9	F-type	I/O-box E9 has no constraints.
I/O-box E9, 2nd	F-type	I/O-box E9, 2nd requires I/O-box E9.
External air sensor L9	F-type	External air sensor L9 has no constraints.
External air sensor L9, 2	F-type	External air sensor L9, 2 requires External air sensor L9.
External air sensor L9, 3	F-type	External air sensor L9, 3 requires External air sensor L9, 2.
External air sensor L9, 4	F-type	External air sensor L9, 4 requires External air sensor L9, 3.
Fraction collector F9-C	D-type	Fraction collector F9-C requires an Outlet valve.
Fraction collector F9-R	F-type	Fraction collector F9-R requires an Outlet valve.

External module	Connector	Constraints
Fraction collector F9-R, 2nd	F-type	Fraction collector F9-R, 2nd requires Fraction collector F9-R or Fraction collector F9-C.
Sample pump S9 and S9H	D-type	Cannot be used at the same time as Mixer valve V9-M or V9H-M.

Note: To optimize signal quality, the total cable length connecting all external modules to the ÄKTA pure instrument should not exceed 10 m.

ÄKTA pure connector plate

The connector plate with the UniNet-9 connectors is located on the back of the ÄKTA pure instrument.

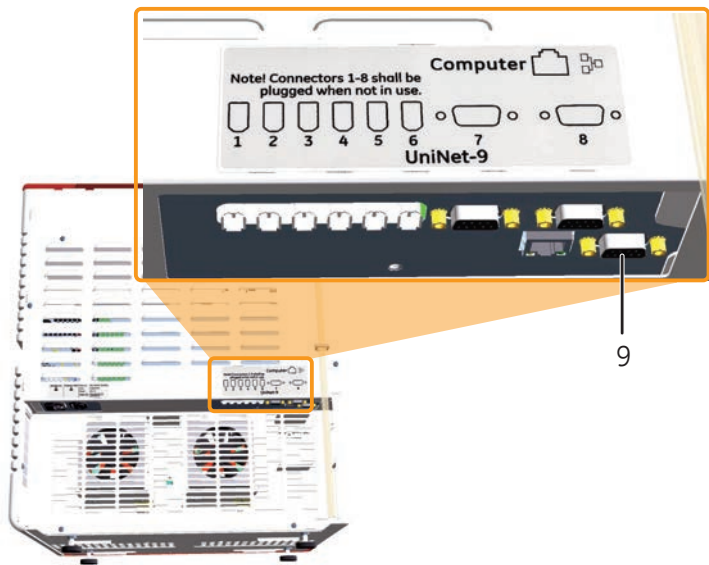

Connector	Connector name	Function
9	Test	Connector point for service.



NOTICE

Do not connect any module to the connector **Test** on the ÄKTA pure instrument.

Note: Plug all unused UniNet-9 ports (ports 1 to 8) on the ÄKTA pure instrument with jumpers.

Note: The connector **Test** should be protected by a plastic lid. Do not plug the connector with a jumper.

4 System configuration

About this chapter

This chapter describes hardware configuration of the ÄKTA pure instrument and how to install optional modules and add them in UNICORN.

In this chapter

This chapter contains the following sections:

Section	See page
4.1 Configuration overview	122
4.2 Configure modules	128
4.3 General system settings	143

4.1 Configuration overview

Introduction

ÄKTA pure is a flexible system that allows the user to configure both hardware and software to meet many purification needs. The instrument can be easily extended with additional valves, detectors and fraction collectors. There are a large number of different hardware modules to choose from in order to customize the number of columns, inlets, outlets, detectors and ways to apply and collect samples.


System configuration steps

The system configuration consists of four main steps:

- 1 Select modules and positions
- 2 Install the module(s)
- 3 Edit system properties
- 4 Edit system settings

Select modules and positions

Optional modules can be placed in any of the available positions in the cabinet. Its function is determined by the module type and node ID. However, to achieve an optimal flow path for a purification run, most modules have a dedicated location in the cabinet. The dedicated location for all modules and, if applicable, any constraints are described in the table below. Each location is marked with a number, which can be seen in the illustration below.

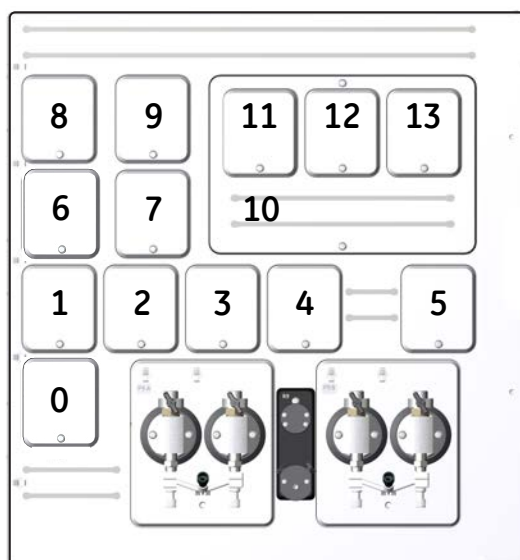

All positions in ÄKTA pure must be occupied. Positions not used for core or optional modules should be fitted with a Module Panel.

Recommended module position

Module	Recommended location	Constraints
Column valve V9-C or V9H-C	9	Column valve V9-C or V9H-C cannot be used at the same time as Column valve V9-Cs or V9H-Cs .
Column valve V9-Cs or V9H-Cs	9	Column valve V9-Cs or V9H-Cs cannot be used at the same time as Column valve V9-C or V9H-C .
Conductivity monitor C9	7	Conductivity monitor C9 has no constraints.
Injection valve V9-Inj or V9H-Inj	6	Core module.
Inlet valve V9-IAB or V9H-IAB	4 5, if Inlet valve V9-IAB or V9H-IAB is used in combination with Inlet valve V9-IA or V9H-IA.	Possible combinations of inlet valves: - Inlet valve A and Inlet valve B. - Inlet valve AB together with Inlet valve A or Inlet valve B. - One Inlet valve AB. or - No installed inlet valves.
Inlet valve V9-IA or V9H-IA	4	
Inlet valve V9-IB or V9H-IB	5	
Sample inlet valve V9-IS or V9H-IS	8	Cannot be used at the same time as Mixer valve V9-M or V9H-M .
Inlet valve V9-X1 or V9H-X1	None	Inlet valve V9-X1 or V9H-X1 has no constraints, and has no support in the method phases.
Inlet valve V9-X2 or V9H-X2	None	Inlet valve V9-X2 or V9H-X2 requires Inlet valve V9-X1 or V9H-X1 , respectively. It has no support in the method phases.
Loop valve V9-L or V9H-L	8	Loop valve V9-L or V9H-L has no constraints, but is connected with the injection valve by replacing the loop.
Mixer M9	0	Core module.
Mixer valve V9-M or V9H-M	3	Cannot be used at the same time as Sample pump S9 or S9H .
Outlet valve V9-Os or V9H-Os	1	Cannot be used at the same time as Outlet valve V9-O or V9H-O .
Outlet valve V9-O or V9H-O	1	Cannot be used at the same time as Outlet valve V9-Os or V9H-Os .

Module	Recommended location	Constraints
pH valve V9-pH or V9H-pH	2	pH valve shall always be connected after the column due to pressure constraints and fractionation control. The delay volume calculations will be effected if the valve is located elsewhere. Normally it is situated between the monitor and the Outlet valve.
Versatile valve V9-V or V9H-V	None	- Versatile valve V9-V or V9H-V has no constraints. - Versatile valve 2 requires Versatile valve V9-V. - Versatile valve 3 requires Versatile valve 2. - Versatile valve 4 requires Versatile valve 3.
Versatile valve 2		
Versatile valve 3		
Versatile valve 4		
UV monitor U9-M	10	UV monitor U9-M cannot be used at the same time as UV monitor U9-L. Note: <i>UV monitor U9-L, 2nd can be used at the same time as UV monitor U9-M.</i>
UV monitor U9-L	11	UV monitor U9-L: - Cannot be used at the same time as UV monitor U9-M. - Requires the Multi-module panel. Note: <i>UV monitor U9-L, 2nd can be used at the same time as UV monitor U9-L.</i>
UV monitor U9-L , 2nd	None	UV monitor U9-L , 2nd requires UV monitor U9-L or UV monitor U9-M .

Install the modules

Detailed information about installation of the modules is found in [Chapter 2 The ÄKTA pure instrument, on page 13](#) and [Chapter 3 ÄKTA pure external modules, on page 86](#).

Below is a quick guide of how to perform a module hardware installation.

Step	Action
1	Switch off the power.
2	Check/set node ID. See NodeID list.
3	Install the module.
4	Connect tubing.

Edit system properties

When a new module has been installed, the system properties have to be updated in UNICORN. The system will restart automatically when the configuration has been changed in **System Properties** and the system can be reconnected.


The following instruction gives a general description of how to update the system properties in UNICORN.

Step Action

- 1
- In the **Administration** module, choose **Tools: System Properties** or click the **System Properties** icon to open the dialog.
Result: The **System Properties** dialog is displayed.
 - Select the system of interest in the **System Properties** dialog.
 - Click the **Edit** button.

Note:
Only active systems can be edited.

Result: The **Edit** dialog is displayed.

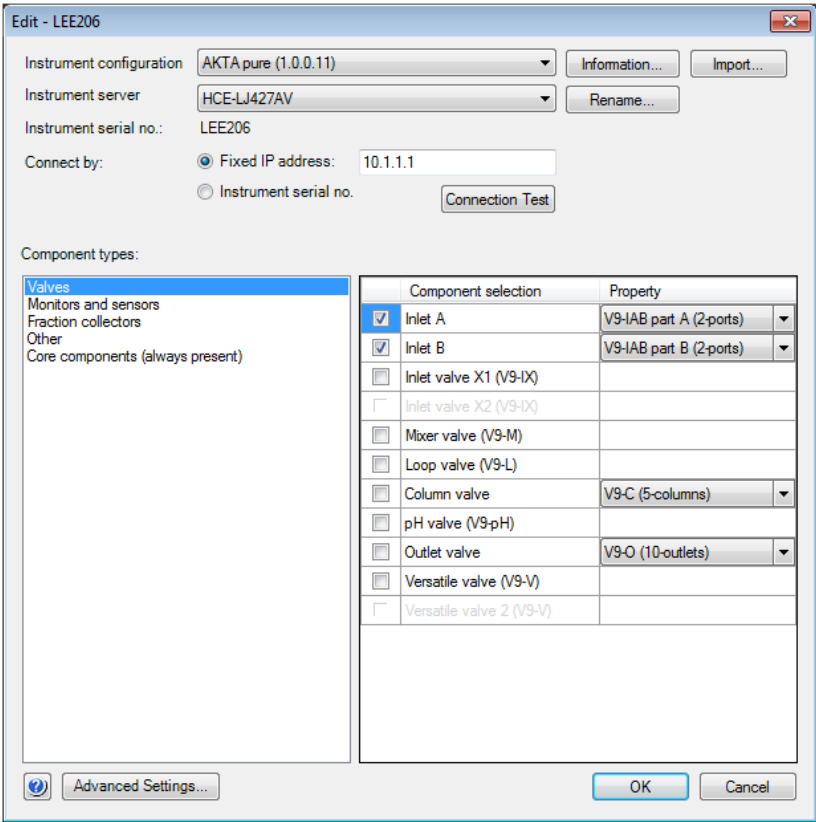

- 2
- Select the component type of interest from the **Component types** list.
Result: All available components are shown in the **Component selection** list.
- Click the checkbox to select the added component.
 - When applicable, choose the appropriate **Property**.

Note:
*Instrument modules are referred to as **Components** in UNICORN.*

- 3
- Click the **OK** button to apply the changes.

There are five main types of modules (named components in UNICORN) to select from:

- Valves and pumps
- Monitors and sensors
- Fraction collectors
- Other (e.g., I/O-box)
- Core components (always present)


Multiple choices are not shown unless a component has been selected. The second component is only available when the first has been selected. The selection made is reflected in which instructions and phase properties that are available.

Edit system settings

It may be necessary to edit the **System Settings** when the configuration of the system is changed. For example, if the change in configuration affects the delay volume following the UV monitor (or other monitor connected via the I/O-box) the appropriate system settings for **Tubing and delay volumes** have to be updated. This is to ensure that the fractions marked in the chromatogram corresponds to the actual collected fractions.

Other system settings might also need to be edited for some optional modules.

The **Edit** dialog in which to edit the system settings is shown below.

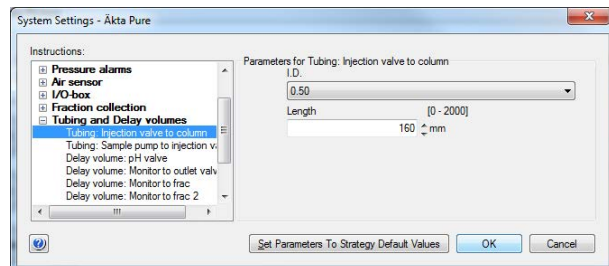

In this dialog it is possible to set the parameters for the available instructions.

All system settings available for ÄKTA pure are found in [Section 9.8 System settings, on page 447](#).

4.2 Configure modules

In this section

This section describes the software configuration that must be set for the individual modules that are to be used for a specific run.

A general description of how to update the system properties are found in [Edit system properties, on page 125](#).

A general description of how to edit system settings are found in [Edit system settings, on page 127](#).

Section	See page
4.2.1 Configuration of inlet valves	129
4.2.2 Configuration of Mixer valves	130
4.2.3 Configuration of Loop valves	131
4.2.4 Configuration of column valves	132
4.2.5 Configuration of Versatile valves	134
4.2.6 Configuration of pH valves	135
4.2.7 Configuration of outlet valves	136
4.2.8 Configuration of UV monitors	137
4.2.9 Configuration of Conductivity monitor	138
4.2.10 Configuration of external air sensors	139
4.2.11 Configuration of fraction collectors	140
4.2.12 Configuration of I/O-box	142

4.2.1 Configuration of inlet valves

System properties

Follow the instruction below to update the system properties.

Step	Action
------	--------

- | | |
|---|--|
| 1 | Open the system properties Edit dialog. |
| 2 | Select Valves and pumps from the Component types list. |
| 3 | Select components and properties according to the following table: |

Valve	Component selection	Property
Inlet valve V9-IA	Inlet A	V9-IA (7-ports)
Inlet valve V9H-IA		V9H-IA (7-ports)
Inlet valve V9-IB	Inlet B	V9-IB (7-ports)
Inlet valve V9H-IB		V9H-IB (7-ports)
Inlet valve V9-IAB or V9H-IAB used for inlet A	Inlet A	V9-IAB part A (2-ports) or V9H-IAB part A (2-ports)
Inlet valve V9-IAB or V9H-IAB used for inlet B	Inlet B	V9-IAB part B (2-ports) or V9H-IAB part B (2-ports)
Sample inlet valve V9-IS	Sample inlet V9-IS	N/A
Sample inlet valve V9H-IS	Sample inlet V9H-IS	N/A
Inlet valve V9-IX	Inlet valve X1 (V9-IX)	N/A
Inlet valve V9H-IX	Inlet valve X1 (V9H-IX)	N/A
Inlet valve V9-IX , 2nd	Inlet valve X2 (V9-IX)	N/A
Inlet valve V9H-IX , 2nd	Inlet valve X2 (V9H-IX)	N/A

System settings

There are no system settings available for the inlet valves.

4.2.2 Configuration of Mixer valves

System properties

Follow the instruction below to update the system properties.

Step	Action
1	Open the system properties Edit dialog.
2	Select Valves and pumps from the Component types list.
3	Select Mixer valve (V9-M) or Mixer valve (V9H-M) in the Component selection list.

System settings

The flow rate for Mixer by-pass wash can be set.

Instruction name	Description
Mixer by-pass wash settings	Sets the flow rate used during Mixer by-pass wash and defines wash volumes for mixer by-pass wash options. Note: <i>The flow rate should not exceed 10 ml/min if narrow inlet tubing (i.d. 0.75 mm) is used.</i>

4.2.3 Configuration of Loop valves

System properties

Follow the instruction below to update the system properties.

Step	Action
1	Open the system properties Edit dialog.
2	Select Valves and pumps from the Component types list.
3	Select Loop valve (V9-L) or Loop valve (V9H-L) in the Component selection list.

System settings

The flow rate for Loop wash can be set.

Instruction name	Description
Loop wash settings	Sets the flow rate used during Loop wash. Note: <i>The flow rate should not exceed 10 ml/min if narrow inlet tubing (i.d. 0.75 mm) is used.</i>

4.2.4 Configuration of column valves

System properties

Follow the instruction below to update the system properties.

Step	Action
------	--------

- | | |
|---|--|
| 1 | Open the system properties Edit dialog. |
| 2 | Select Valves and pumps from the Component types list. |
| 3 | Select components and properties according to the following table: |

Valve	Component selection	Property
Column selection valve V9-C	Column valve	V9-C (5-columns)
Column selection valve V9H-C	Column valve	V9H-C (5-columns)
Column control valve V9-Cs	Column valve	V9-Cs (1-column)
Column control valve V9H-Cs	Column valve	V9H-Cs (1-column)

System settings

After selecting Column valve **V9-Cs**, **V9H-Cs** or no column valve, in UNICORN, the tube length has to be defined.

The instructions **Tubing: Injection valve to column** and **Tubing: Sample pump to injection valve** are used in calculations of pre-column pressure when Column valve **V9-C** or **V9H-C** (5-columns) is NOT mounted onto the system. In such cases, there is no pre-column pressure sensor present. The estimated pre-column pressure is calculated using the measured system pressure and the length of the tubing between the system pressure sensor and the Column.

The instructions are available only when the Column valve **V9-C** or **V9H-C** (5-columns) is not selected in the component list. The instruction **Tubing: Sample pump to injection valve** is in addition only available if the sample pump is selected in the list.

Follow the instructions below to set the tube length between the Injection valve and the Column and between the sample pump and the injection valve.

Step	Action
------	--------


- | | |
|---|---|
| 1 | <ul style="list-style-type: none"> In the System Control module, choose System:Connect to Systems or click the Connect to Systems icon. <p><i>Result:</i> The Connect to Systems dialog opens.</p> |
|---|---|

Step	Action
------	--------

- | | |
|---|---|
| 2 | <ul style="list-style-type: none"> • Select a system. • Select Control mode. • Click OK. |
|---|---|

Result: The selected instrument can now be controlled by the software.

- | | |
|---|---|
| 3 | <ul style="list-style-type: none"> • Select Tubing and Delay Volumes and select Tubing: Injection valve to column. • Select the I. D. from the drop-down list. • Type in the length of the tube in the Length field and click OK. |
|---|---|

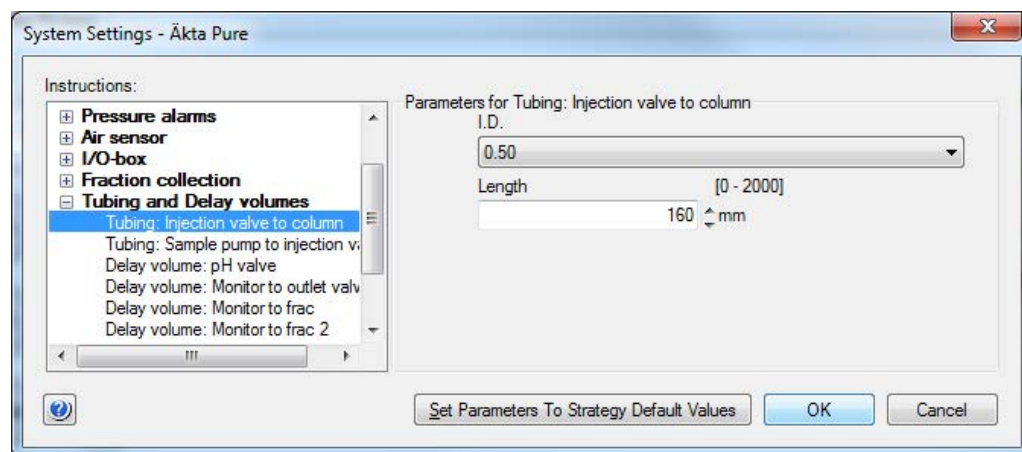

- | | |
|---|--|
| 4 | Perform step 3 for the instruction Tubing: Sample pump to injection valve . |
|---|--|

- Note:** The built-in pressure sensors for Column valves **V9-C** and **V9H-C** have to be re-calibrated after installation. See [Calibrate the monitors, on page 302](#).
- Note:** A Pre-Column pressure alarm shall always be set to protect the column, see [Section 5.6 Pressure alarms, on page 174](#). Column valve **V9-Cs** and **V9H-Cs** does not contain pressure monitors. See [Section 5.6 Pressure alarms, on page 174](#) for how to protect columns when not using Column valves **V9-C** and **V9H-C**.

4.2.5 Configuration of Versatile valves

System properties

Follow the instruction below to update the system properties.

Step	Action
1	Open the system properties Edit dialog.
2	Select Valves and pumps from the Component types list.
3	Select Versatile valve (V9-V) , Versatile valve 2 (V9-V) , Versatile valve 3 (V9-V) or Versatile valve 4 (V9-V) in the Component selection list.

System settings

If the valve is placed in the flow path between the UV monitor and the outlet valve, the delay volume must be set. See [Check/Set delay volume, on page 143](#).

4.2.6 Configuration of pH valves

System properties

Follow the instruction below to update the system properties.

Step	Action
1	Open the system properties Edit dialog.
2	Select Valves and pumps from the Component types list.
3	Select pH valve (V9-pH) or pH valve (V9H-pH) in the Component selection list.

System settings

If the valve is placed in the flow path between the UV monitor and the outlet valve, the delay volume must be set. See [Check/Set delay volume, on page 143](#).

Note: *It is recommended not to alter the default values for restrictor and pH cell delay volumes when standard modules and standard tubing for flow restrictor are used.*

4.2.7 Configuration of outlet valves

System properties

Follow the instruction below to update the system properties.

Step	Action
------	--------

- | | |
|---|--|
| 1 | Open the system properties Edit dialog. |
| 2 | Select Valves and pumps from the Component types list. |
| 3 | Select components and properties according to the following table: |

Valve	Component selection	Property
Outlet fractionation valve V9-O	Outlet valve	V9-O (10-outlets)
Outlet fractionation valve V9H-O	Outlet valve	V9H-O (10-outlets)
Outlet control valve V9-Os	Outlet valve	V9-Os (1-outlet)
Outlet control valve V9H-Os	Outlet valve	V9H-Os (1-outlet)

System settings

If the valve is not placed in the recommended position using the standard tubing kit, the delay volume must be set. See [Check/Set delay volume, on page 143](#).

4.2.8 Configuration of UV monitors

Using two UV monitors

The UV monitor **U9-L** module can be used in two configurations, UV monitor **U9-L** and UV monitor **U9-L, 2nd**. The configuration is defined by the module's Node ID.

It is possible to use two UV monitors in ÄKTA pure, in the following combinations:

- UV monitor **U9-M** together with UV monitor **U9-L, 2nd**
- UV monitor **U9-L** together with UV monitor **U9-L, 2nd**

UV monitor **U9-L, 2nd** can be located anywhere in the flow path and is therefore shown in the **Process Picture** as a component without a fixed place. This means that it is possible to place **U9-L, 2nd** before the other UV monitor in the flow path.

Note: If **U9-L, 2nd** is placed on the high pressure side of the column, pressure limits have to be considered. See [UV monitor options, on page 414](#) for pressure limits.

System properties

Follow the instruction below to update the system properties.

Step	Action
1	Open the system properties Edit dialog.
2	Select Monitors and sensors from the Component types list.
3	Select components and properties according to the following table:

- Open the system properties **Edit** dialog.
- Select **Monitors and sensors** from the **Component types** list.
- Select components and properties according to the following table:

Monitor	Component selection	Property
UV monitor U9-L	UV monitor	U9-L (fixed)
UV monitor U9-M	UV monitor	V9-M (variable)
UV monitor U9-L, 2nd	UV monitor 2nd (U9-L)	N/A

System settings

If the monitor is not placed in the recommended position using the standard tubing kit, the delay volume must be set. See [Check/Set delay volume, on page 143](#).

For UV monitor **U9-L** the flow cell length must be set. This is done as a calibration. See [Perform the calibration, on page 310](#).

4.2.9 Configuration of Conductivity monitor

System properties

Follow the instruction below to update the system properties.

Step	Action
1	Open the system properties Edit dialog.
2	Select Monitors and sensors from the Component types list.
3	Select Conductivity monitor (C9) in the Component selection list.

System settings

If the monitor is placed in the flow path between the UV monitor and the outlet valve, the delay volume must be set. See [Check/Set delay volume, on page 143](#).

4.2.10 Configuration of external air sensors

System properties

Follow the instruction below to update the system properties.

Step	Action
1	Open the system properties Edit dialog.
2	Select Monitors and sensors from the Component types list.
3	Select External air sensor (L9) in the Component selection list, or the appropriate component if multiple external air sensors are used.
4	Select Property according to where the air sensor is placed.
Note: <i>The available system properties are the same, regardless of which type of air sensor that is used, L9-1.2 or L9-1.5.</i>	

System settings

The sensitivity of the air sensor can be set.

Parameter	Air volume detected		Usage
	ÄKTA pure 25	ÄKTA pure 150	
Normal (default)	30 µl	100 µl	Detect empty buffer/sample vessels
High	10 µl	30 µl	Detect even small air bubbles

Note: The sensitivity should be set to **Normal** when the air sensor is located before the System pump (**Air sensor ext - Before pump A** or **Air sensor ext - Before pump B**). Due to higher pressure and risk of small air bubbles, the sensitivity should be set to **High** when the air sensor is located after the Injection valve (**Air sensor ext - after Injection valve**).

4.2.11 Configuration of fraction collectors

System properties

Follow the instruction below to update the system properties.

Step	Action
1	Open the system properties Edit dialog.
2	Select Fraction collectors from the Component types list.
3	Select components and properties according to the following table:

Fraction collector	Component selection	Property
Fraction collector F9-C	Fraction collector	Fraction collector F9-C
Fraction collector F9-R	Fraction collector	Fraction collector F9-R
Fraction collector F9-R, 2nd	Fraction collector 2 (F9-R)	N/A

Note: *Fraction collector 2* is only available in the **Component selection** list if **Fraction collector** is already selected.

System settings

If non-standard tubing is used between the outlet valve and the fraction collector, the delay volume must be set. See [Check/Set delay volume, on page 143](#).

Fraction settings and numbering mode can be set.

Fraction collector F9-C

Instruction name	Description
Fractionation settings	Fractionation settings comprises fractionation mode and fractionation order. Fractionation mode (Automatic, Accumulator or DropSync). Fractionation order (Row-by-row, Column-by-column, Serpentine-row, Serpentine-column). For fractionation mode DropSync, only the Serpentine option is available.
Last tube filled	Last tube filled: Action when last tube is filled (pause, direct the flow to one of outlets or direct the flow to waste).
Cassette configuration	Cassette configuration: Automatic or Manual configuration. If Automatic is selected, a Quick scan or a Full scan will be performed when the door of the fraction collector is closed to determine which type of cassettes and plates are used. If Manual is selected, used plates and tubes in each tray position are entered.

Instruction name	Description
Fraction collector lamp	Fraction collector lamp: Lamps in the fraction collector chamber on or off.
Peak fractionation parameters	The Peak fractionation parameters set the detection parameters for peak collection, that is they decide when a peak starts and ends. This information is used by the instructions Peak fractionation and Peak frac in outlet valve in order to start/end the peak collection.

Fraction collector F9-R

Instruction name	Description
Fractionation settings	Drop sync synchronises tube change to drop release. The available settings are on or off. It is recommended to use Drop sync for flow rates below 2 ml/min. Higher flow rates can however be used, depending on the properties (for example viscosity) of the liquid.
Fractionation numbering mode	Determines whether the fraction number is reset at the end of a method or not. Note: <i>The default setting is Reset.</i>
Fractionation settings frac 2	Drop sync on or off. It is recommended to use this setting for flow rates below 2 ml/min. Higher flow rates can be however be used, depending on the properties (e.g. viscosity) of the liquid.
Fractionation numbering mode frac 2	Determines whether fraction number for the second fraction collector is reset at the end of a method or not. Note: <i>The default setting is Reset.</i>
Peak fractionation parameters	Peak fractionation parameters sets the detection parameters for peak collection, i.e. it determines when a peak starts and ends. This information is used by the instructions Peak fractionation , Peak fractionation frac 2 and Peak frac in outlet valve in order to start/end the peak collection.

4.2.12 Configuration of I/O-box

System properties

Follow the instruction below to update the system properties.

Step	Action
1	Open the system properties Edit dialog.
2	Select Monitors and sensors from the Component types list.
3	Select I/O-box (E9) or I/O-box 2 (E9) in the Component selection list.

System settings

Default values for digital out ports, noise reduction and configuration of analog out ports can be set.

Instruction name	Description
Digital out X	Sets the value of the signal sent out by digital port number X to either 0 or 1. The default value is 1.
Noise reduction analog in X	Filters the noise in the analog signal in port number X.
Alarm analog in X	Enables or disables the alarm for the analog signal in port number X. When enabled, it sets the alarm limits for the analog signal. If the alarm is enabled and the analog signal falls outside the set limits, an alarm will be triggered and the method will be paused.
Alarm digital in X	Enables or disables the alarm for the signal in digital port number X. The alarm can be triggered by either of the signal values, 0 or 1. If the alarm is enabled and the condition set in 'Value' occurs, an alarm will be triggered and the method will be paused.
Configure analog out X	Enables the user to send one of the pre-defined signals (UV signal, conductivity, temperature, pH or concentration of eluent B) to the analog out port number X, and also to set the range of that signal.

Note: The delay volume has to be updated if an external component is added to the flow path.

4.3 General system settings

Check/Set delay volume


When a module has been installed after the UV monitor in the flow path, the delay volume has to be adjusted in the **System Setting** dialog in UNICORN, to make sure that the collected fractions correspond to the fractions indicated in the chromatogram.

Delay volumes can be set for the options **Monitor to outlet valve**, **Monitor to frac**, **Monitor to frac 2**, and **pH valve**. Depending on the system configuration used, different delay volume options will be available for selection in the **System Setting** dialog. The delay volume has to be set for all displayed options.

Delay volumes for modules and standard tubing configurations are found in [Section 9.13 Delay volumes, on page 492](#).

Follow the instructions below to check/set the delay volumes:

- | Step | Action |
|------|---|
| 1 | <ul style="list-style-type: none"> In the System Control module, choose System:Connect to Systems or click the Connect to Systems icon. <p><i>Result:</i> The Connect to Systems dialog opens.</p> |
| 2 | <ul style="list-style-type: none"> Select a system. Select Control mode. Click OK. <p><i>Result:</i> The selected instrument can now be controlled by the software.</p> |
| 3 | <ul style="list-style-type: none"> When the system is in state Ready, select System:Settings. <p><i>Result:</i> The System Settings dialog is displayed.</p> |

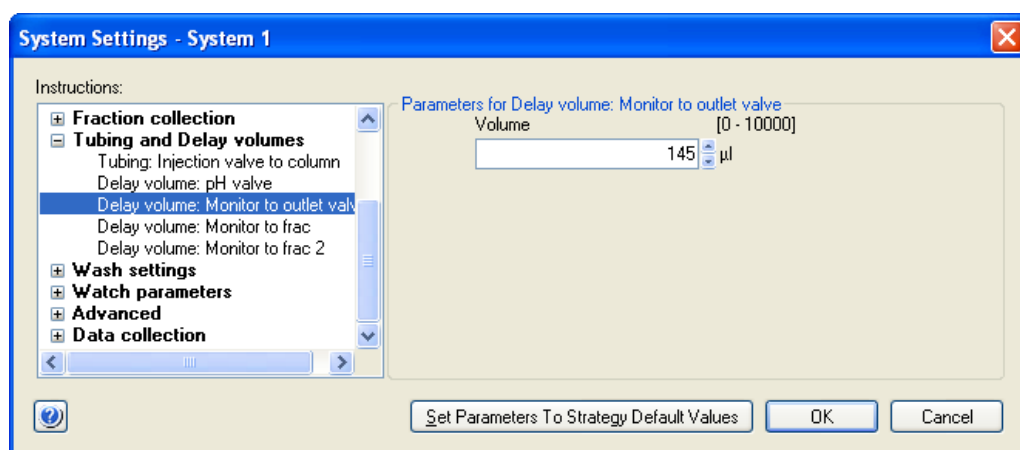


- | | |
|---|---|
| 4 | <ul style="list-style-type: none"> Select Tubing and Delay Volumes and select the delay volume option of interest. Check the delay volume in the Volume field and enter a new value if necessary. Click OK. |
|---|---|

Lock/Unlock function

Follow the instruction below to lock or unlock the **Pause** and **Continue** buttons of the Instrument control panel from UNICORN.

Step	Action
------	--------

- | | |
|---|--|
| 1 | In System Control , select System:Settings .
<i>Result:</i> The System Settings dialog opens. |
| 2 | In the System Settings dialog: <ul style="list-style-type: none">• Select Advanced:Instrument control panel.• Select Locked or Unlocked.• Click OK. |

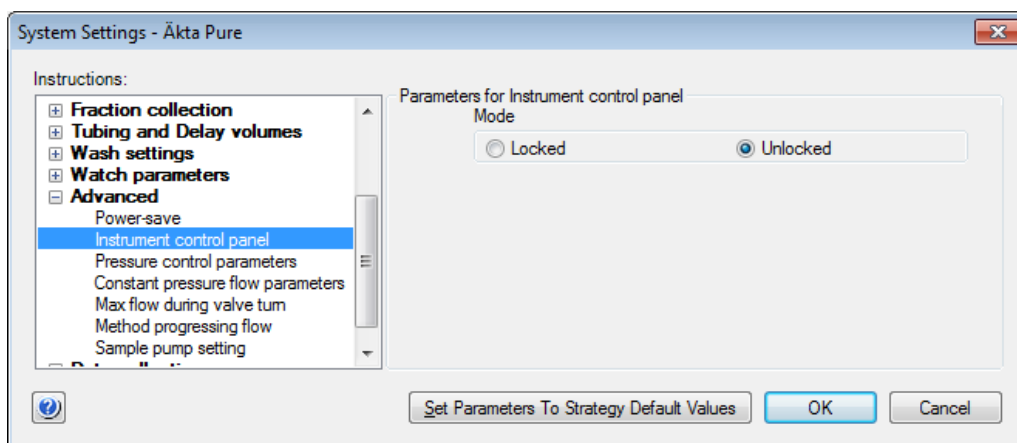

Power-save

ÄKTA pure has a power-save mode. The instrument enters **Power-save** after having been in the **Ready** state for a set period of time. **Power-save** can be used both in room temperature and in cold room temperature. The system enters the **Ready** state when a method run, a method queue or a manual run ends.

To enable **Power-save**, a system must be connected and in state **Ready**.


Follow the instructions below to activate **Power-save**.

Step	Action
------	--------

- | | |
|---|--|
| 1 | Select System:Settings in the System Control module. |
|---|--|

Result: The **System Settings** dialog opens.

- | | |
|---|---|
| 2 | <ul style="list-style-type: none"> • Select Advanced and • select Power-save |
|---|---|

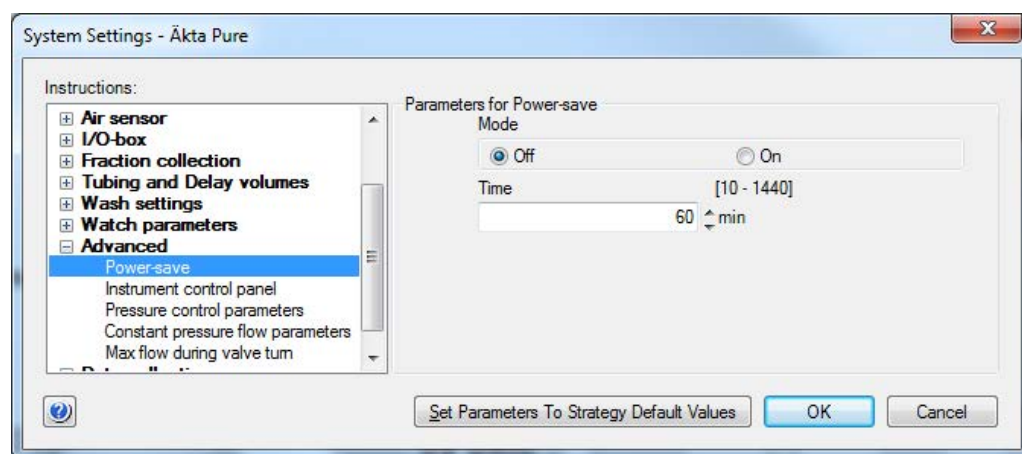

- | | |
|---|--|
| 3 | <ul style="list-style-type: none"> • Select On in the Mode field and • type the number of minutes in the Time field. |
|---|--|

Note:

*This is the time the instrument will be in state **Ready** before power-save mode is entered.*

- Click **OK**.

5 Operation

About this chapter

This chapter describes the steps involved when operating ÄKTA pure.

In this chapter

This chapter contains the following sections:

Section	See page
5.1 Before you prepare the system	147
5.2 Prepare the flow path	148
5.3 Start UNICORN and connect to system	155
5.4 Prime inlets and purge pump heads	158
5.5 Connect a column	170
5.6 Pressure alarms	174
5.7 Sample application	177
5.8 Fractionation	190
5.9 Create a method and perform a run	208

5.1 Before you prepare the system

Introduction

It is important to prepare the system in accordance with the settings in the method to be run. Before preparing the system, check the settings in the **Method Editor** and make sure that all accessories to be used are available.

Checklist

Make sure the system is prepared in accordance with the settings in the method to be run. Depending on configuration, remember to check:

- which valve ports to use for inlets and outlets
 - which column type to use
 - which column position to use
 - which buffers and samples to prepare
 - which sample application technique to use
 - that the pH electrode is connected and calibrated
-


5.2 Prepare the flow path

Introduction

The flow path is defined by the user and may contain tubing, valves, pumps and monitors. This section gives an overview of a flow path and describes how to prepare the flow path before a run.

Illustration of the flow path

The illustration below shows the flow path for a typical system configuration. The individual instrument modules are presented in the table below. The configuration of the system is defined by the user.

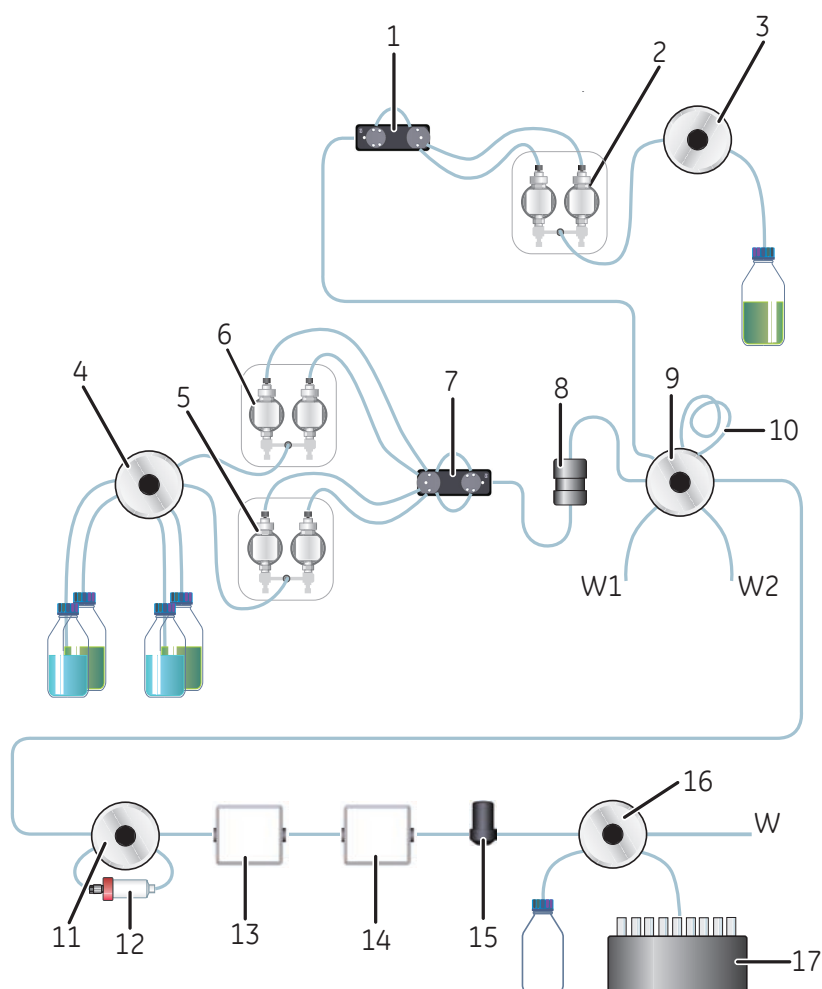

Part	Description
1	Pressure monitor
2	Sample pump
3	Sample inlet valve

Part	Description
4	Inlet valve
5	System pump B
6	System pump A
7	Pressure monitor
8	Mixer
9	Injection valve
10	Sample loop or Superloop
11	Column valve
12	Column
13	UV monitor
14	Conductivity monitor
15	Flow restrictor
16	Outlet valve
17	Fraction collector
W, W1, W2	Waste

Select Mixer chamber

To obtain a homogeneous buffer composition, it is important to use a Mixer chamber suitable for the flow rate of the method. The tables below show what Mixer chambers to use in ÄKTA pure at different flow rates.

If the liquids are difficult to mix, use a larger Mixer chamber to achieve optimal mixing. However, note that a larger Mixer chamber distorts and delays the gradient.

The default mixer size is 1.4 ml for both systems. ÄKTA pure 150 also includes a 5 ml mixer. Other mixer sizes are available as accessories.

Mixer chamber volume [ml]	Flow rate [ml/min], Binary gradient	
	ÄKTA pure 25	ÄKTA pure 150
0.6	0.1-5	<i>Not recommended</i>
1.4	0.5-15	0.5-15
5	2-25	2-50
15	<i>Not compatible</i>	15-150

**CAUTION**

Risk of explosion. Do not use Mixer chamber 15 ml with an ÄKTA pure 25 configuration. The maximum pressure for Mixer chamber 15 ml is 5 MPa.

Note: In ÄKTA pure 25 at low flow rates (below 0.2 ml/min) a gradient of sufficient quality may be achieved with the mixer bypassed. Similarly, for low flow rates in ÄKTA pure 150 the 0.6 ml mixer might be used.

Note: The 1.4 ml mixer in ÄKTA pure 25 or 5 ml mixer in ÄKTA pure 150 might work up to maximum flow rate provided that the buffers are easily mixed.

For information on how to install a Mixer chamber, refer to [Section 7.8.3 Replace the Mixer, on page 319](#).

Select UV flow cells

General considerations

Flow cells with shorter path lengths are suitable to use when high protein concentrations are used. Flow cells with longer path lengths are suitable to use when low protein concentrations are used.

UV flow cells for UV monitor U9-M

UV flow cells are available with three different path lengths; 0.5 mm, 2 mm (default) and 10 mm.

The real cell path length of the UV cell is automatically recognized by the monitor when a cell is fitted. The UV data is normalized to the nominal path length. This allows UV data from runs made with different UV flow cells (but with the same nominal path length) to be directly compared.

UV flow cells for UV monitor U9-L

UV flow cells are available with two different path lengths; 2 mm (default) and 5 mm. When replacing a UV flow cell, the path length must be set in the **System Control** module, in **System:Calibrate**. Use the nominal flow cell length if the UV flow cell is replaced but not calibrated. See [Update the cell path length, on page 311](#) to set the flow cell path length.

The path length of the UV flow cell might differ from the nominal length, which leads to incorrect results in the calculation of protein concentration in the eluate. The UV data is normalized to the nominal path length. This allows UV data from runs made with different UV flow cells (but with the same nominal path length) to be directly compared. To achieve normalized absorbance, the path length of the UV flow cell must be calibrated and the calculated flow cell path length set manually. See [Calibration of the UV monitor U9-L flow cell length, on page 309](#).

Prepare the inlet tubing

Connect inlet tubing to the inlet ports that are to be used, and place all inlet tubing that is to be used during the method run in the correct buffers.

Note: When using high viscosity buffers/samples in combination with high flow rates it is recommended to increase the tubing I.D. and/or shorten the length.

Prepare the outlet tubing

Connect outlet tubing to the outlet ports of Outlet valve that are to be used. If a fraction collector is to be used, make sure that tubing is connected as described in [Connect tubing, on page 102](#) and [Connect tubing to the ÄKTA pure instrument, on page 106](#), and prepare the fraction collector. Otherwise, place the outlet tubing in suitable tubes or flasks.

Prepare the waste tubing

The table below lists the waste tubing of the instrument and where it is located. Make sure that the waste tubing is connected to the correct positions on the modules.

Module	Tubing connections	Location of tubing
Injection valve	Waste ports W1 and W2	Front of the ÄKTA pure instrument.
pH valve (optional)	Waste port W3	Front of the ÄKTA pure instrument.
Outlet valve (optional)	Waste port W	Front of the ÄKTA pure instrument.
Buffer tray (Rescue drainage)	Drainage hole of the Buffer tray	Rear of the ÄKTA pure instrument.
Fraction collector F9-C (optional)	Fraction collector waste outlet	Rear of the fraction collector.

Instructions

Follow the instructions below to prepare the waste tubing.



CAUTION

Fasten the waste tubing. During operation at high pressure the ÄKTA pure instrument may release bursts of liquid in the waste tubing. Securely fasten all waste tubing to the ÄKTA pure instrument and to the waste vessel.



CAUTION


Make sure that the waste vessel will hold all the produced volume of the run. For ÄKTA pure, a suitable waste vessel should typically have a volume of 2 to 10 liters.




NOTICE

The maximum level of the waste vessel must be lower than the bottom of the ÄKTA pure instrument.

Step	Action
1	Insert the waste tubing from all installed modules, in this example Injection valve, Outlet valve (W , W1 and W2) and the fraction collector, in a vessel.
2	Make sure that the tubing is securely fastened to the ÄKTA pure instrument: • Fasten waste tubing from the valves with the clips on the front of the system.

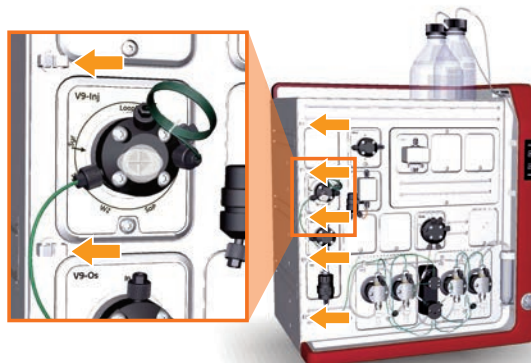

- Fasten waste tubing from the Buffer tray with the clips on the rear of the system.

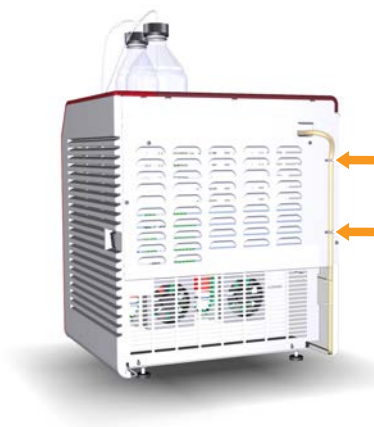

Step	Action
3	Cut the waste tubing to appropriate length. It is important that the tubing is not bent and will not be submerged in liquid during the run.



Note:

If the tubing is too short, replace it with new tubing. Do not lengthen the tubing as this might cause obstruction of the tubing.

4	Fasten all waste tubing securely to the waste vessel.
---	---

Plug unused valve ports

It is recommended to plug all unused valve ports with stop plugs before starting a run. See [Tubing connectors, on page 420](#) for information about connectors.

5.3 Start UNICORN and connect to system

Introduction

This section describes how to start and log on to UNICORN and how to connect the instrument to UNICORN.

Start UNICORN and log on

Follow the instructions to start UNICORN and log on to the program. A valid e-license must be available for the workstation. See UNICORN Administration and Technical Manual for more information about e-licenses.

Step	Action
------	--------

1	Double-click the UNICORN icon on the desktop.
---	---

Result: The **Log On** dialog opens.

Note:


*If there is no connection to the database it is still possible to log on to UNICORN and control a running system. The **Log On** dialog will give the option to start **System Control** without a database. Click **Start System Control** to proceed to the next **Log On** dialog.*

2	In the Log On dialog:
---	------------------------------

- Click a user name in the **User Name** list and
- enter the password in the **Password** field.

Note:

*It is also possible to select the **Use Windows Authentication** checkbox and enter a network ID in the **User Name** box.*

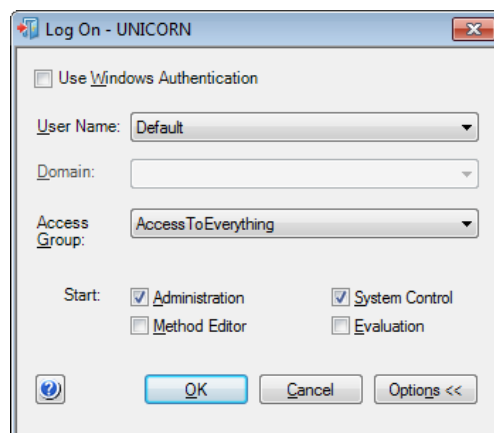

- select which UNICORN modules to start.
- click **OK**.

Result: The selected UNICORN modules open.

Connect to system

Follow the instructions to connect the instrument to UNICORN.

Step	Action
------	--------


- | | |
|---|--|
| 1 | In the System Control module, <ul style="list-style-type: none">Click the Connect to Systems button, |
|---|--|



or

- click **Connect to Systems** on the **System** menu.

Result: The **Connect to Systems** dialog opens.

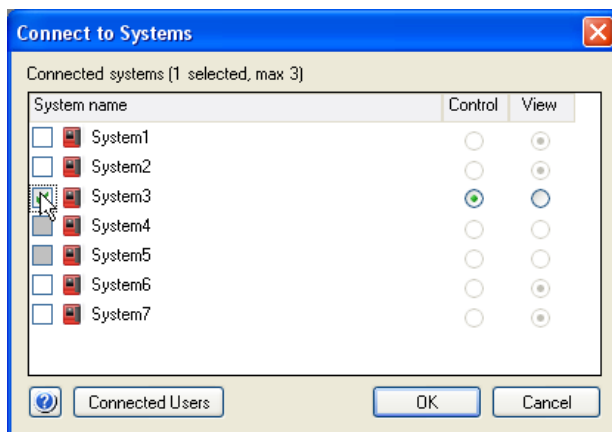

Step	Action
2	In the Connect to systems dialog: • Select the checkbox in front of the system name. • To control the selected system, click Control. • Click OK. <i>Result:</i> The instrument control panel displays a white, rapidly flashing light followed by a steady white light when the system is ready. The selected instrument can now be controlled by the software. Note: <i>Instruments that are turned off or disconnected from the network appear dimmed and cannot be connected.</i> Tip: <i>To view the users currently connected to systems, either in control or view mode, click the Connected Users button.</i> Tip: <i>Result: UNICORN states Connection = Connected in control or Connection = Connected in view in the status bar in the lower part of the System Control window.</i> 

5.4 Prime inlets and purge pump heads

About this section

Before usage of a pump, it is important to:

- Prime the inlets (fill the buffer inlets with liquid).
- Purge the pump (remove air from the pump heads).

This section describes how to prime inlets and purge the pump heads of the system pumps and the sample pump (the sample pump is an optional module).

Note: *Note that the procedures described in this section may have to be adapted if your system configuration differs from the one described in this manual.*

In this section

This section contains the following subsections:

Section	See page
5.4.1 System pumps	159
5.4.2 Sample pump	165

5.4.1 System pumps

Introduction

This section describes how to prime inlets and purge the System pumps.

Overview

The procedure consists of the following stages:

Stage	Description
1	Prime all inlet tubing to be used during the run
2	Purge System pump B
3	Validate purge of System pump B
4	Purge System pump A
5	Validate purge of System pump A
6	End the run

Tip: *The procedures for purging the pump heads and priming the inlets using the **Process Picture**, are described below. It is also possible to perform the procedures from the **Manual instructions** dialog.*

Prime inlet tubing



Follow the instructions below to fill all A and B inlet tubing to be used in the run with appropriate buffer/solution.

Step	Action
1	Make sure that all inlet tubing that is to be used during the method run is placed in the correct buffer.
2	Open the System Control module.

5 Operation

5.4 Prime inlets and purge pump heads

5.4.1 System pumps

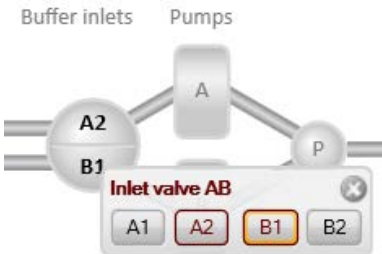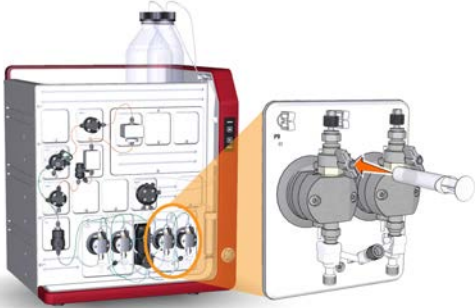Step	Action
3	In the Process Picture: - Click on the buffer inlets. - Select the position of the inlet to be filled. Select the positions in reverse alphabetical order and start with the highest number. For example, if all the four inlets in Inlet valve AB are to be filled, fill them in the following order: B2, B1, A2, A1.  <i>Result:</i> The inlet valve switches to the selected port.
4	Connect a 25 to 30 ml syringe to the purge valve of one of the pump heads of the pump that is being prepared. Make sure that the syringe fits tightly into the purge connector. 
5	Open the purge valve by turning it counter-clockwise about three quarters of a turn. Draw liquid slowly into the syringe until the liquid reaches the pump.
6	Close the purge valve by turning it clockwise. Disconnect the syringe and discard its contents.
7	Repeat steps 3 to 6 for each piece of inlet tubing that is to be used during the run.

Purge System pump B

Follow the instruction below to purge both pump heads of System pump B.

Step	Action
1	Make sure that the piece of waste tubing connected to the Injection valve port W1 is placed in a waste vessel.


Step	Action
------	--------

2

In the **Process Picture**:

- Click on the **Injection valve** and select **System pump waste**.


Result: The Injection valve switches to waste position. This is necessary to achieve a low back pressure during the purge procedure.

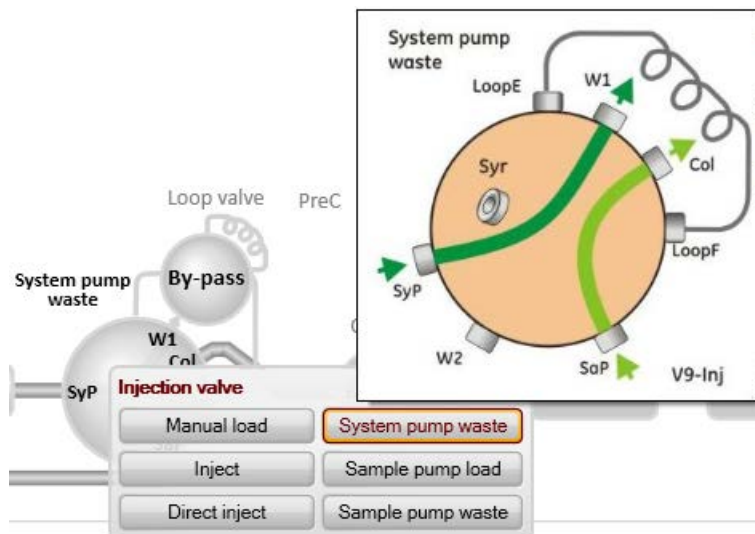

3

In the **Process Picture**:

- Click on the pumps.
- Set **Conc % B** to 100% B.

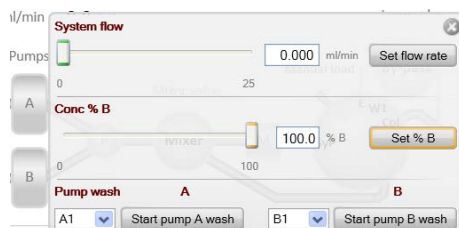




- Click **Set % B**.

Result: Only System pump B is active.


5 Operation

5.4 Prime inlets and purge pump heads

5.4.1 System pumps

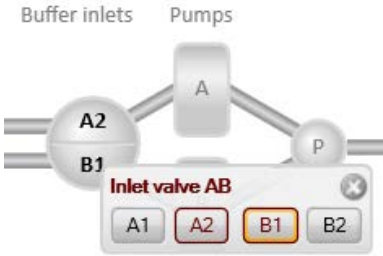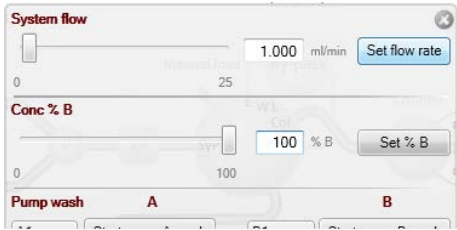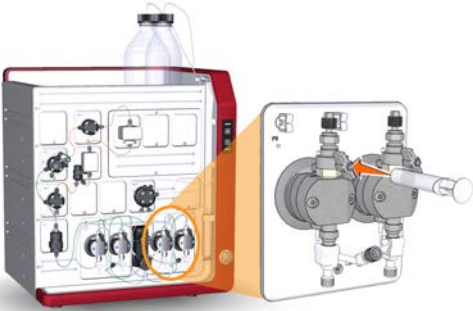- | Step | Action |
|------|--|
| 4 | <p>In the Process Picture:</p> <ul style="list-style-type: none">Click on the buffer inlets.Select the position of one of the inlets that will be used at the beginning of the run.  <p><i>Result:</i> The inlet valve switches to the selected port.</p> |
| 5 | <p>In the Process Picture:</p> <ul style="list-style-type: none">Click on the Pumps.Set the System flow to 1.0 ml/min for ÄKTA pure 25 or 10.0 ml/min for ÄKTA pure 150.Click Set flow rate.  <p><i>Result:</i> A system flow starts.</p> |
| 6 | <p>Connect a 25 to 30 ml syringe to the purge valve of the left pump head of System pump B. Make sure that the syringe fits tightly into the purge connector.</p>  |
| 7 | <p>Open the purge valve by turning it counter-clockwise about three quarters of a turn. Draw a small volume of liquid slowly into the syringe (with a rate of about 1 ml per second).</p> |
| 8 | <p>Close the purge valve by turning it clockwise. Disconnect the syringe and discard its contents.</p> |


Step	Action
9	Connect the syringe to the purge valve on the right pump head of System pump B, and repeat steps 6 to 8. Keep the system flow running.

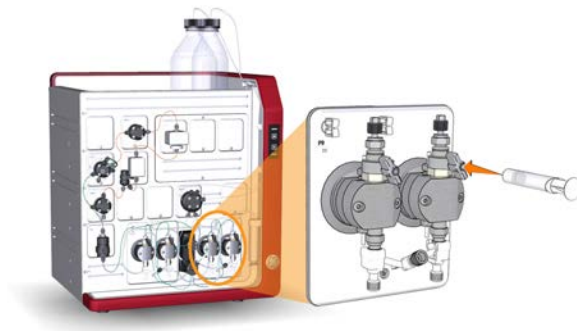

Validate purge of pump B

Follow the instructions below to check that there is no air left in the pump after performing a purge.

Step	Action
1	In the Process Picture: Click on the Injection valve and select Manual load. <i>Result:</i> The Injection valve switches to manual load position.

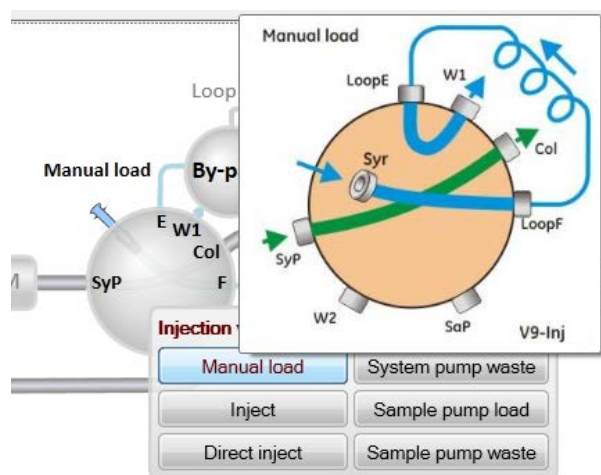

2	Make sure that the pump flow is on.
3	In the Chromatogram pane: Check the PreC pressure curve. If the PreC pressure do not stabilize within a few minutes there may be air left in the pump. Refer to Section 8.6 Troubleshooting: Pumps, on page 384.

5 Operation

5.4 Prime inlets and purge pump heads

5.4.1 System pumps

Purge System pump A

Purge both pump heads of System pump A by following the same procedure as in [Purge System pump B, on page 160](#), but replace step 3 with the following actions:

In the **Process Picture**:

- Click on the pumps.
- Set **Conc % B** to 0% B.



- Click **Set % B**

Result: Only System pump A is active.

Validate purge of pump A

Follow the procedure described in [Validate purge of pump B, on page 163](#) to check if there is air left in the pump.

End the run

Click the **End** button in the **System Control** toolbar to end the run.



5.4.2 Sample pump

Introduction

This section describes how to prime inlets and purge Sample pumps **S9** and **S9H**.

Overview

The procedure consists of the following steps:

- 1 Prime all sample inlet tubing to be used during the run
 - 2 Purge the Sample pump
 - 3 Validate purge
 - 4 End the run
-

Prime sample inlets

Follow the instructions below to fill all sample inlet tubing, to be used in the run, with appropriate buffer or solution. Skip steps three and four if no sample inlet valve is used.


Step	Action
1	Make sure that all sample inlet tubing that is to be used during the method run is immersed in the correct buffers.
2	Make sure that the waste tubing connected to Injection valve port W2 is immersed in a waste vessel.
3	Open the System Control module.

5 Operation

5.4 Prime inlets and purge pump heads


5.4.2 Sample pump

Step	Action
4	In the Process Picture : - Click on Sample inlet valve. - Select the position of the inlet to be filled. Start at the inlet position with the highest number and end at the position with the lowest number.

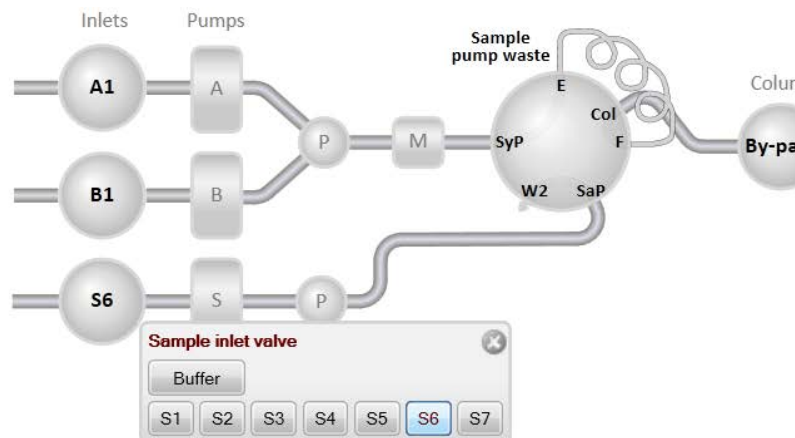

Result: the sample inlet valve switches to the selected port.

5	Connect a 25 to 30 ml syringe to one of the purge valves of the pump heads of the Sample pump. Make sure that the syringe fits tightly into the purge connector.
---	--

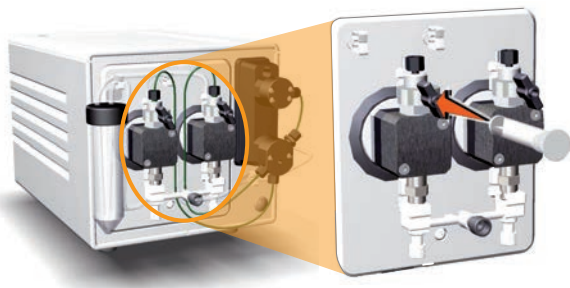


6	Open the purge valve by turning it counter-clockwise about three-quarters of a turn. Draw liquid slowly into the syringe until the liquid reaches the sample pump.
7	Close the purge valve by turning it clockwise. Disconnect the syringe and discard its contents.
8	Repeat steps 2-5 for each sample inlet that is to be used in the method run.

Purge the Sample pump


Follow the instruction below to purge both the pump heads of the Sample pump.

- | Step | Action |
|------|---|
| 1 | Make sure that all sample inlet tubing that is to be used during the method run is immersed in the correct buffers. |
| 2 | Make sure that the waste tubing connected to Injection valve port W2 is immersed in a waste vessel. |
| 3 | Open the System Control module. |
| 4 | In the Process Picture : <ul style="list-style-type: none"> Click on Injection valve and select Sample pump waste . |

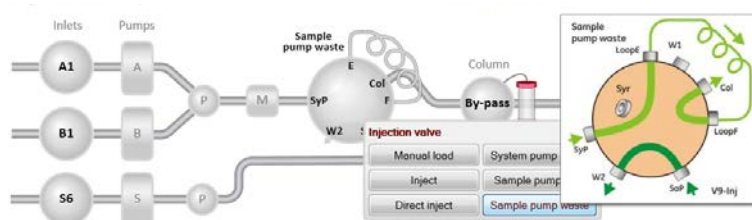

Result: The injection valve switches to waste position. This is necessary to achieve a low back pressure during the purge procedure.

- 5 In the **Process Picture**: Click on **Sample pump**.
- If Sample inlet valve **V9-IS** or **V9H-IS** is used: Click on the **Sample inlet valve** icon (if the valve is not used, the icon will not be present):
 Select the **Buffer** inlet.
 - Click on the **Sample pump** icon: Set the **Sample flow** to 1.0 ml/min for ÄKTA pure 25 or 10.0 ml/min for ÄKTA pure 150.

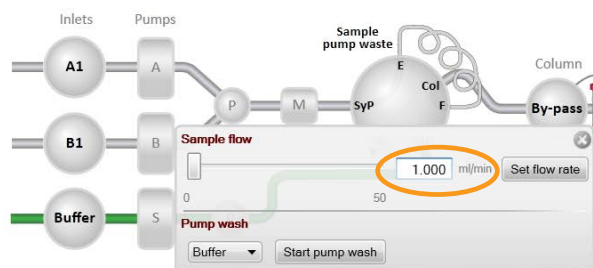

- Click **Set flow rate** and close the pop-up window.


Result: a sample pump flow starts.

5 Operation

5.4 Prime inlets and purge pump heads

5.4.2 Sample pump

Step	Action
6	Connect a 25 to 30 ml syringe to the left purge valve of the Sample pump. Make sure that the syringe fits tightly into the purge connector.

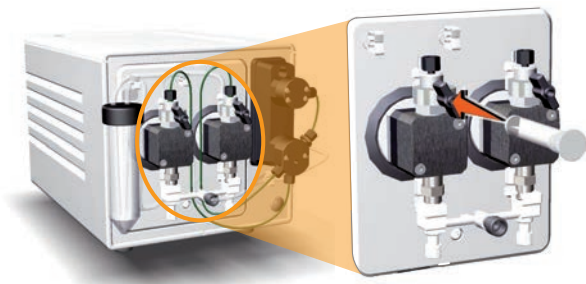

- 7 Open the purge valve by turning it counter-clockwise about three-quarters of a turn. Draw 5-10 ml of liquid slowly into the syringe with a rate of about 1 ml/s.
- 8 Close the purge valve by turning it clockwise. Disconnect the syringe and discard its contents.
- 9 Connect the syringe to the right purge valve on the Sample pump, and repeat step 6 to step 8.




Validate purge

Follow the instructions below to check that there is no air left in the pump after performing a purge.

Step	Action
------	--------

- | | |
|---|--|
| 1 | <p>In the Process Picture:</p> <ul style="list-style-type: none"> Click on the Injection valve and select Direct inject. <p><i>Result:</i> The Injection valve switches to direct inject position.</p> |
|---|--|

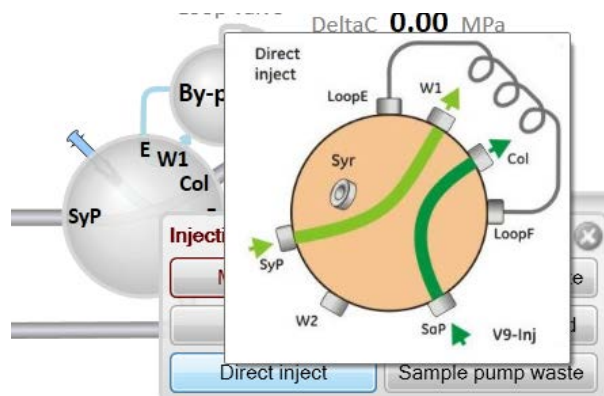

- | | |
|---|---|
| 2 | Make sure that the pump flow is on. |
| 3 | <p>In the Chromatogram pane:
 Check the PreC pressure curve.</p> <p>If the PreC pressure does not stabilize within a few minutes there may be air left in the pump. Refer to Section 8.6 Troubleshooting: Pumps, on page 384.</p> |

End the run

Click the **End** button in the **System Control** toolbar to end the run.



5.5 Connect a column

Introduction

This section describes how to connect a column to the instrument using a column holder and without introducing air into the flow path. Several types of column holders are available for ÄKTA pure.



WARNING

To avoid exposing the column to excessive pressure, make sure that the pressure limit is set to the specified maximum pressure of the column. Before connecting a column to the ÄKTA pure instrument, read the instructions for use of the column.

Methods automatically include a pressure alarm based on the specifications of the chosen column type. However, when running manual runs you have to set the pressure limits yourself. Also, to protect the column media, special settings are needed. See [Section 5.6 Pressure alarms, on page 174](#) for more information on pressure alarms.

Note: Do not overtighten when connecting columns. Overtightening might rupture the connectors or squeeze the tubing and thereby result in high back pressure.


Note: If no column valve is used, remove the column from the system before running a system wash. The pressure during a system wash may become too high for the column.

Attach a column holder and connect a column

Follow the instructions below to connect a column to the instrument. Always use a column holder. If a column valve is used, connect the column to the appropriate A and B ports on the valve. If no column valve is used, connect the column directly to the flow path tubing. Use appropriate tubing and connectors. The instructions below show a system configured with Column valve **V9-Cs**.

Step	Action
------	--------

- | | |
|---|--|
| 1 | Attach an appropriate column holder to the rail on the instrument. |
|---|--|

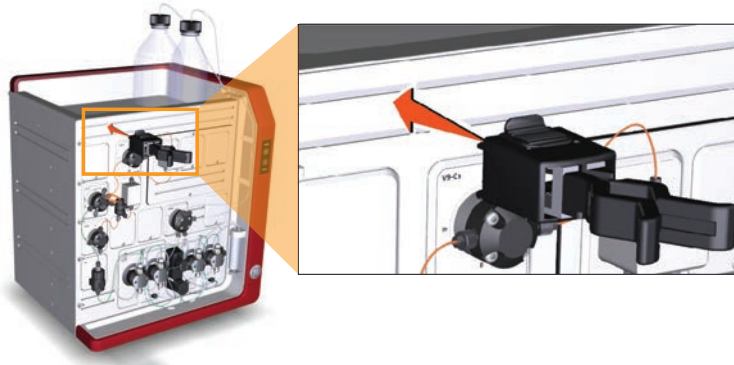

Step	Action
------	--------

2	Attach the column to the column holder.
---	---




3	Connect a suitable tubing to a Column valve port, in this example port 1A .
---	--

4	Open the System Control module.
---	--

5	In the Process Picture :
---	---------------------------------


- Click on the **Column**.
- Select **Column down flow**.

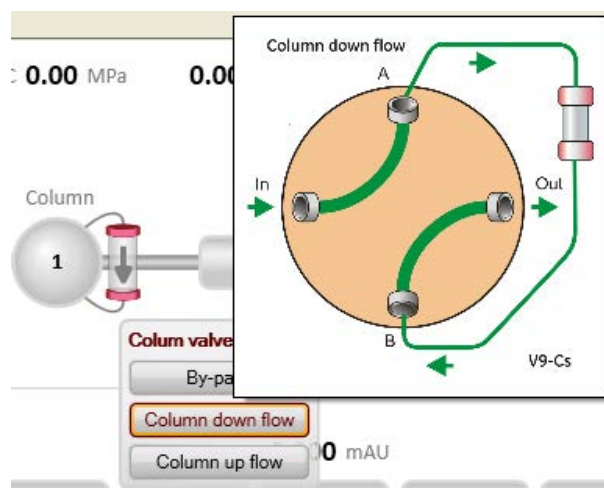

Result: The Column valve switches to position **1**.

Step	Action
------	--------

- | | |
|---|---|
| 6 | <p>In the Process Picture:</p> <ul style="list-style-type: none">• Click on the Pumps.• Enter a low System flow (e.g., 0.2 ml/min).• Click Set flow rate. |
|---|---|

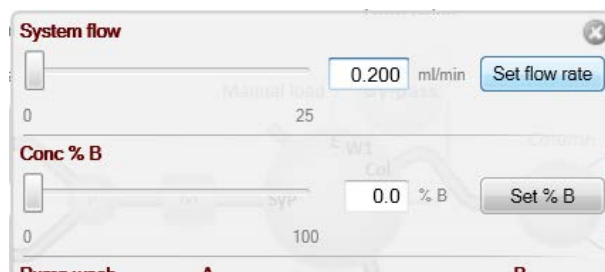

Result: A system flow of 0.2 ml/min starts.

- | | |
|---|--|
| 7 | <p>When buffer leaves the tubing in a continuous mode and the top part of the column is filled with buffer, connect the tubing to the top of the column.</p> |
|---|--|



- | | |
|---|---|
| 8 | <p>Connect a piece of tubing to the bottom of the column.</p> |
|---|---|



Step	Action
9	When buffer leaves the tubing at the bottom of the column in a continuous mode, connect this piece of tubing to the Column valve. Use the port opposite to the one already connected to the column, in this example port 1B . If no column valve is used, connect the tubing to the next module in the flow path.



10	Click the End icon in the System Control toolbar to end the run.
----	--



5.6 Pressure alarms

Introduction

The columns can be protected by two different types of pressure alarms:

- The pre-column pressure alarm protects the column hardware
- The delta-column pressure alarm (only available when **V9-C** or **V9H-C** is installed) protects the column media


Column valves **V9-C** and **V9H-C** have built-in pressure sensors that automatically measure the pre-column and delta-column pressure. If Column valve **V9-C** or **V9H-C** is not used (column is connected without a Column valve or to Column valve **V9-Cs** or **V9H-Cs**), the pre-column pressure is calculated from the system pressure and tubing dimensions.

See the instructions below to set the pressure alarm for the column to be used in the run and, if applicable, to set the parameters for the tubing dimensions.

Set tubing dimension parameters to calculate pre-column pressure

For instruments where there is no pre-column pressure sensor, i.e. the column is connected without a Column valve or to Column valve **V9-Cs** or **V9H-Cs**, the pre-column pressure is calculated from the system pressure and tubing dimensions. Follow the instructions below to set the tubing dimension parameters.

- | Step | Action |
|------|--|
| 1 | Select System:Settings in the System Control module.
<i>Result:</i> The System Settings dialog opens. |
| 2 | <ul style="list-style-type: none">• Select Tubing and Delay Volumesand• select Tubing: Injection valve to column |

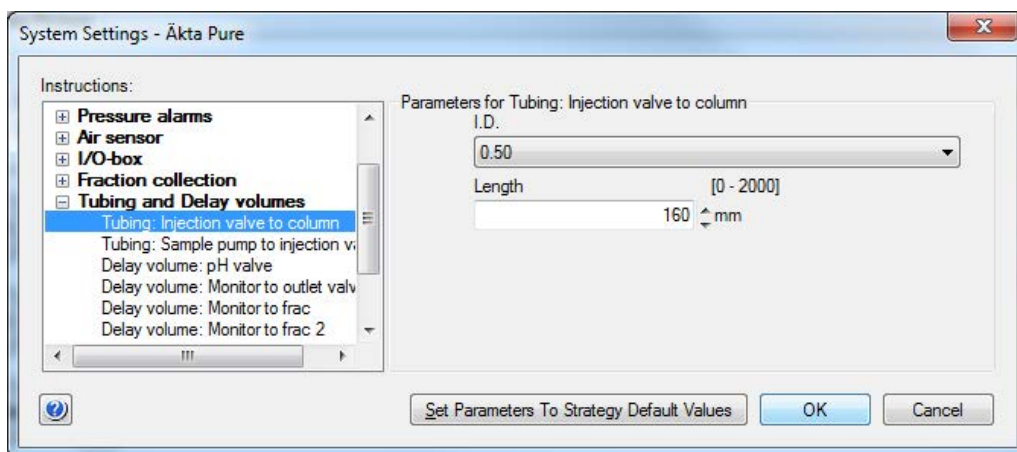

Step	Action
3	• Select the inner diameter of the tubing between the injection valve and the column from the I.D. drop-down list. • Type in the tubing Length.
4	If the sample pump is used: • Select Tubing: Sample pump to injection. • Set tubing i.d. and length, see step 3.
5	Click OK . Note: <i>The system now calculates the Pre-column pressure.</i>

Pre-column pressure alarms

It is important that the pre-column pressure alarm is set during all runs where a column is used. The pressure alarm can be set in:

- the method to be run,
- the **System Settings** dialog , or
- during a manual run

Pre-column pressure alarm limits are automatically set in the method when a column from the column list is selected in the method. Refer to UNICORN Method Manual for more information on pressure alarms.

For some columns the max delta-column pressure (media) is significantly lower than the max pre-column pressure (hardware). To protect the media if a delta-column pressure measurement is not available (that is, when column valve **V9-C** or **V9H-C** is not used), the pre-column pressure alarm must be manually set to the value in the column list that is the lowest of the max pre-column pressure and the max delta-column pressure.

Delta-column pressure alarms

If column valve **V9-C** or **V9H-C** is installed the delta-column pressure will be measured, but the alarm must be set manually if needed.


Set pressure alarms

Pressure alarm limits may be set manually in **System Control**. The example below describes how to set the high pressure limit for the column. Other alarms are set in a corresponding way.

Step	Action
1	Select Manual:Execute Manual Instructions... in the System Control module. <i>Result:</i> The Manual instructions dialog opens.

Step	Action
------	--------

- | | |
|---|---|
| 2 | <ul style="list-style-type: none">• Select Alarms
and• select Alarm pre column pressure. |
|---|---|

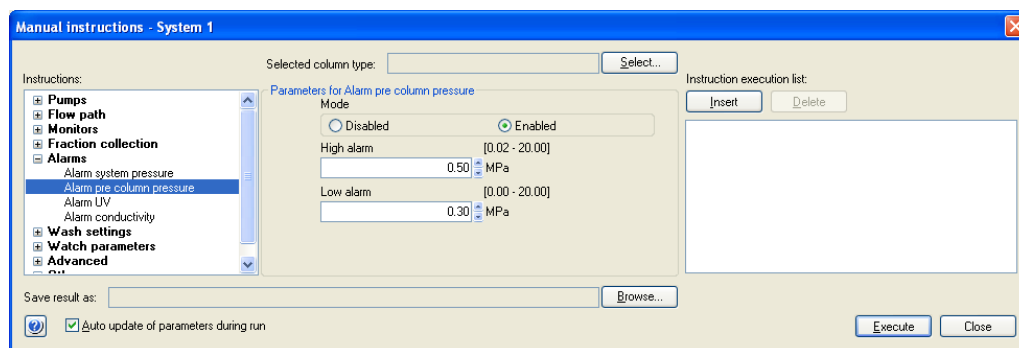

- | | |
|---|--|
| 3 | Select Enabled in the Mode field. |
| 4 | <ul style="list-style-type: none">• Type the high pressure limit in the High alarm field.• Click Execute. |

5.7 Sample application

Introduction

This section describes the different sample application techniques that can be used with ÄKTA pure. The table below shows the alternatives for sample application available in the **Sample application** phase of a method.

Sample application	Via	Compatible loops
Inject sample directly onto column	• Sample pump • System pump A • System pump A and Air sensor	• Not applicable
Inject sample from loop	• Syringe • Sample pump • Sample pump and Air sensor • System pump A • System pump A and Air sensor	• Sample loop • Superloop, 10 ml • Superloop, 50 ml • Superloop, 150 ml

Note: In order to avoid sample carry-over when switching techniques for loading samples, wash the valve with buffer between the loading of two different samples. For example, when switching from loading sample in the loop to loading sample directly onto the column with the valve in **Direct inject** position.

When using a pump for sample application, it is important to prime inlets and purge the pump before using the pump to load the sample:

- Sample pump, see further instructions in [Section 5.4.2 Sample pump, on page 165](#)
- System pump A, see further instructions in [Section 5.4.1 System pumps, on page 159](#)

When loading sample using System pump A and an external air sensor, the sensor should be installed according to [Adapter for air sensor, on page 83](#).

Note: When sample is loaded at high flow rate and the external air sensor is placed before the pump that is used for loading the sample, it is necessary to use longer tubing to ensure that no air reaches the pump. Use tubing with the minimum lengths given below between the valve located before the pump and the external air sensor. The length applies for maximum flow rate, but shorter tubing can be used at lower flow rates.

- Sample pump S9: 40 cm.
- Sample pump S9H: 20 cm.

5.7.1 Sample application using direct injection onto the column

Introduction

There are two ways to load sample directly onto a column:

- a fixed volume is loaded, or
- all the sample is loaded.

To inject all the sample, one of the following configurations is required:

- system pump, external air sensor, inlet valve A and the mixer valve, or
- sample pump and sample inlet valve.

Minimize sample loss

To minimize sample loss during direct injection of sample onto the column, sample remaining in the flow path will be pushed onto the column with buffer from the inlet valve. This step is called **Finalize sample injection** in the text instructions of the sample application phase of the method to be used. Refer to [Section 5.9 Create a method and perform a run, on page 208](#) for more information on methods and phases.

When preparing to inject...	Then...
a fixed volume of sample	• manually prime the sample inlet tubing with sample, see Prime sample inlets, on page 165. • in the Method editor, make the following selections for the Sample Application phase of the method to be run: - select Inject sample directly onto column, - select Inject fixed sample volume and set the volume to be injected. • make sure that the flow path from the sample inlet valve up to the injection valve will be filled with an appropriate buffer: - make sure that the buffer inlet tubing of the inlet valve is immersed in buffer, and - enable the function Wash sample flow path with buffer in the Sample application phase.

When preparing to inject...	Then...
all the sample	- in the Method editor, make the following selections for the Sample Application phase of the method to be run: - select Inject sample directly onto column, and - select Inject all sample using air sensor. - manually prime the sample inlet tubing with sample or buffer, see Prime sample inlets, on page 165, and make sure that the tubing is immersed in sample before starting the run. - make sure that the flow path from the sample inlet valve up to the injection valve is filled with sample or an appropriate buffer and that the buffer inlet tubing is immersed in buffer.

Maximize precision and accuracy

To achieve full precision and accuracy when a volume of sample is injected directly onto the column, make the following selections in the **Sample Application** phase of the method to be run (refer to [Section 5.9 Create a method and perform a run, on page 208](#) for more information on methods and phases):

- select **Inject sample directly onto the column**,

- select **Inject fixed sample volume** and set the volume to be injected,
- enable the function **Prime sample inlet with** and set the volume to be used for priming.

Result: the step **Finalize sample injection** is automatically deactivated in order to maximize precision and accuracy. See [Minimize sample loss, on page 178](#) for more information.

Note: If manual priming of the flow path up to the injection valve is preferred, enable **Prime sample inlet with** but set the volume to 0 ml.

- If the system pump is used to load the sample: enable the function **Wash sample flow path with buffer after sample application** in order to ensure that the correct sample volume is loaded onto the column.

5.7.2 Sample application using a Superloop™

Introduction

A Superloop allows injection of large sample volumes onto the column. A Superloop can also be used for multiple injections, for example in a scouting experiment when the same application conditions are required. Superloop models are available in 10 ml, 50 ml and 150 ml sizes.

A superloop can be connected to either the Injection valve or the Loop valve. When using the Loop valve, up to five loops can be connected simultaneously.

Note: After loading a Superloop, always plug the **Syr** port on the Injection valve with a Stop plug. With a Superloop connected to the valve, an over-pressure may be created during injection.

Prepare the Superloop

To avoid injecting air into the system flow path, the Superloop should be prefilled with buffer manually, before fitting the Superloop to the system.

Note: Read the instruction for the Superloop to be used.

Connect the Superloop

Follow the instruction below to connect the Superloop to the Injection valve or to the Loop valve.

Step	Action
------	--------

- | | |
|---|---|
| 1 | Attach the Superloop to the instrument using a Column holder. |
| 2 | Connect a piece of tubing from the <i>top</i> of the Superloop to: <ul style="list-style-type: none">port LoopE on the Injection valveora E port, eg., 1E, on the Loop valve |

Step	Action
------	--------

3	Connect a piece of tubing from the <i>bottom</i> of the Superloop to:
---	---

- port **LoopF** on the Injection valve



or

- the **F** port corresponding to the connected **E** port, eg., **1F**, on the Loop valve

Fill the Superloop using a syringe

Follow the instruction below to fill the Superloop using a syringe.


Step	Action
------	--------

1	Check if the system is in state Ready .
---	--

- If yes: The Injection valve is in position **Manual Load** per default. Continue to step 3.
- If no: Continue to step 2 to position the valve.

2	In the Process Picture :
---	---------------------------------

- Click the **Injection valve** and select **Manual Load**.

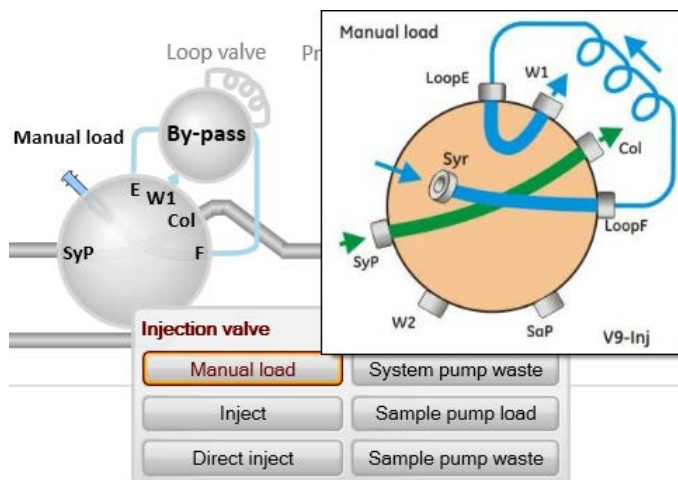

Result: The Injection valve switches to **Manual Load** position.

Step	Action
3	If the loop is connected to: - the Injection valve, continue to step 5. - the Loop valve, continue to step 4.
4	In the Process Picture: - Click the Loop valve. - Select the position the loop is connected to, for example Position 1. <i>Result:</i> The Loop valve switches to the selected position.
5	Fill a syringe with sample.
6	Connect the syringe to Injection valve port Syr .
7	Load sample into the Superloop by emptying the syringe into the Injection valve.
8	Disconnect the syringe and plug the Syr port with a Stop plug.

Fill the Superloop using the Sample pump

Follow the instruction below to fill the Superloop using the Sample pump.






NOTICE


Glass tube splinter. Make sure to set the sample pressure below the max pressure of the Superloop before executing a flow in the Manual instructions dialog when the Superloop is connected.

Tip: The Superloop can also be filled as part of a method run, as set in the **Sample Application** phase in the **Method Editor**. For multiple injections, it may be more convenient to fill the Superloop once, as described in the instruction below.

Step	Action
------	--------

- | | |
|---|--|
| 1 | <p>In the Manual instructions dialog:</p> <ul style="list-style-type: none"> • Select Flow path:Injection valve. • Select Sample pump load from the Position drop-down list. • Click . <p><i>Result:</i> The Injection valve switches to Sample pump load position.</p> |
| 2 | <p>Make sure that the sample inlet tubing from the sample vessel is connected to the Sample inlet valve.</p> |
| 3 | <p>In the Manual instructions dialog:</p> <ul style="list-style-type: none"> • Select Alarms:Alarm sample pressure. • Set Mode as Enabled. • Set a High alarm level that is below the maximum pressure of the Superloop. • Click . |
| 4 | <p>In the Manual instructions dialog:</p> <ul style="list-style-type: none"> • Select Pumps and pressures:Sample flow. • Set Flow rate to an appropriate value for the Superloop size, in this example 10 ml/min. |

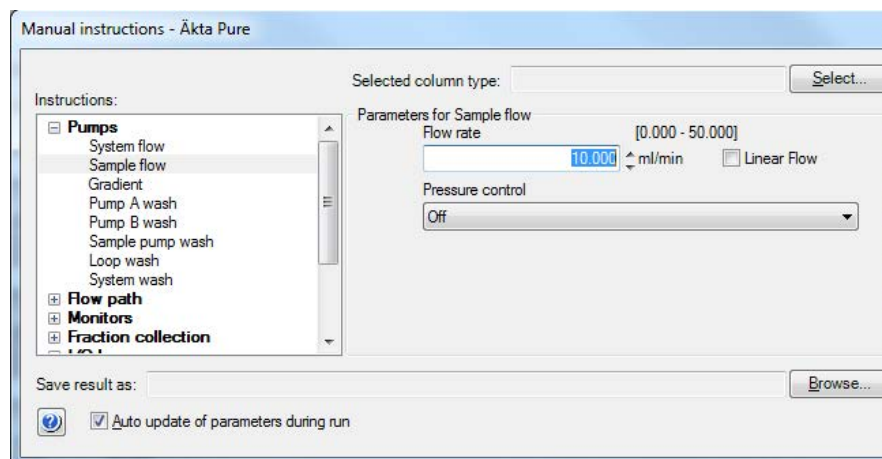

- | | |
|---|--|
| | <ul style="list-style-type: none"> • Click . <p><i>Result:</i> A sample flow starts, in this example of 10 ml/min.</p> |
| 5 | <p>When the Superloop is filled with as much volume as is needed, click the End icon in the System Control toolbar to end the run.</p> |



- | | |
|---|--|
| 6 | <p>Plug the Syr port on the Injection valve with a Stop plug.</p> |
|---|--|

Fill the Superloop using System pump A

Follow the instruction below to fill the Superloop using the System pump A. Note that Mixer valve has to be installed for this loop filling technique.




NOTICE

Glass tube splinter. Make sure to set the system pressure below the max pressure of the Superloop before executing a flow, when the Superloop is connected.

Tip: The Superloop can also be filled as part of a method run, as set in the **Sample Application** phase in the **Method Editor**. For multiple injections, it may be more convenient to fill the Superloop once, as described in the instruction below.


Step	Action
1	In the Manual instructions dialog: • Select Alarms:Alarm system pressure. • Set Mode as Enabled. • Set a High alarm level that is below the maximum pressure of the Superloop. • Click .
2	In the Process Picture : • Click the Injection valve and select Sample pump load.

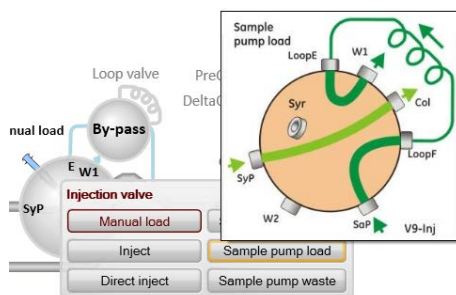

Result: The Injection valve switches to **Sample pump load** position.

Step	Action
------	--------

- | | |
|---|---|
| 3 | <p>In the Process Picture:</p> <ul style="list-style-type: none"> Click the Mixer valve and select By-pass. |
|---|---|

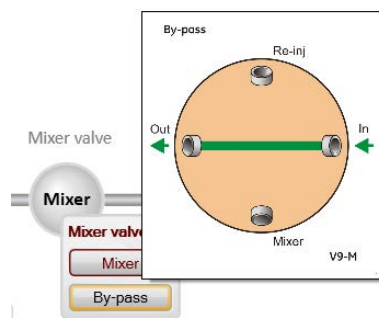

Result: The Mixer valve switches to **By-pass** position.


- | | |
|---|---|
| 4 | <p>If the loop is connected to:</p> <ul style="list-style-type: none"> the Injection valve, continue to step 6. the Loop valve, continue to step 5. |
|---|---|

- | | |
|---|--|
| 5 | <p>In the Process Picture:</p> <ul style="list-style-type: none"> Click the Loop valve. Select the position the loop is connected to, for example Position 1. |
|---|--|



Result: The Loop valve switches to the selected position.

- | | |
|---|---|
| 6 | <p>In the Process Picture:</p> <ul style="list-style-type: none"> Click on the buffer inlet valve A. Select the inlet position to be used for sample injection, for example A2. |
|---|---|

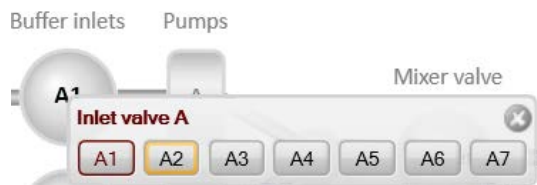

Result: Inlet valve A switches to the selected port.

5 Operation

5.7 Sample application

5.7.2 Sample application using a Superloop™

Step	Action
7	In the Process Picture: - Click on the Pumps. - Set the System flow to an appropriate value for the Superloop size, in this example 10 ml/min. - Click Set flow rate.  <i>Result:</i> A system flow starts, in this example of 10 ml/min.
8	When the Superloop is filled with as much volume as is needed, click the End icon in the System Control toolbar to end the run. 
9	Plug the Syr port on the Injection valve with a Stop plug.

5.7.3 Sample application using a sample loop

Introduction

A sample loop is recommended for injection of smaller sample volumes onto the column.

A sample loop can be connected to either the Injection valve or the Loop valve. When using the Loop valve, up to five loops can be connected simultaneously.

Note: Sample loop is called capillary loop in UNICORN.

How to fill a sample loop

Follow the instructions below to fill the sample loop with sample.

Step	Action
1	Connect a suitable sample loop to Injection valve ports LoopF (fill) and LoopE (empty).




- 2 Fill a syringe with sample.
- 3 Connect the syringe to the Injection valve port **Syr**.




Step	Action
------	--------

- | | |
|---|--|
| 4 | <p>In the Process Picture:</p> <ul style="list-style-type: none"> Click on the Injection valve and select Manual load. |
|---|--|

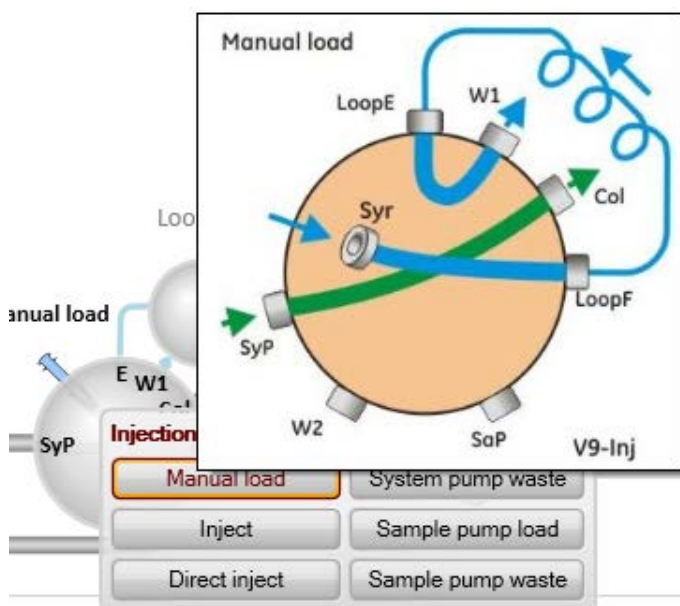

Result: Injection valve is set to manual load.

- | | |
|---|--|
| 5 | <p>If the loop is connected to:</p> <ul style="list-style-type: none"> the Injection valve, continue to step 7. the Loop valve, continue to step 6. |
| 6 | <p>In the Process Picture:</p> <ul style="list-style-type: none"> Click the Loop valve. Select the position the loop is connected to, for example Position 1. |

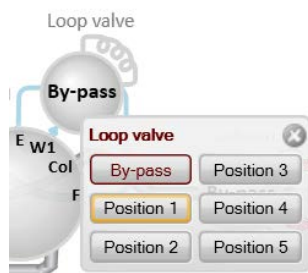

Result: The Loop valve switches to the selected position.

Step	Action
7	Load sample into the sample loop. To avoid sample loss due to siphoning, leave the syringe in the port until the sample has been injected onto the column during the run. Tip: <i>It is recommended to overfill the loop to make sure that the loop is completely filled. Excess of sample will leave the valve through port W1.</i>

Fill the sample loop using the Sample pump

Most often the sample loop is filled using a syringe. However, to fill it using the sample pump, follow the instructions for filling the Superloop, see [Fill the Superloop using the Sample pump, on page 182](#).

- Note:**
- It is not necessary to set the Alarm Sample Pressure when filling a sample loop.
 - It is recommended to overload the loop to make sure that the loop is completely filled.
 - Set **Flow rate** to an appropriate value for the loop size.
 - After loading, plug the **Syr** port on the Injection valve with a Stop plug.

Fill the sample loop using System pump A

Most often the sample loop is filled using a syringe. However, to fill it using System pump A, follow the instructions for filling the Superloop, see [Fill the Superloop using System pump A, on page 184](#).

Empty the loop

General considerations

During the method run, the sample is automatically injected onto the column. The loop is emptied and washed out using buffer from the system pumps. The total buffer volume to be used for emptying and washing the loop is set in the Method Editor.

Using a sample loop connected to Loop valve V9-L or V9H-L

For maximum reproducibility, use complete loop fill when loading the loop, that is, overfill the loop with a sample volume of up to 3-5 times the volume of the loop. For minimum sample loss, use partial loop fill, that is, fill only up to 50% of the loop volume. Empty the loop with 3-5 times the volume of the loop.

Volume used to empty a loop connected to Loop valve V9-L or V9H-L

To minimize the risk for carry over and to make sure that the complete sample volume reaches the column, the loop should be emptied with an excess of buffer. The tubing between the Loop valve port **E** and the Injection valve port **E** holds a small volume. If the loop is emptied with a volume equal to, or less than the loop volume this needs to be taken into account. It is also important to use a low flow rate to ensure that the correct volume is added to the column when injecting a small volume.

- Note:** *Partially emptying the loops that are attached to Loop valve V9-L or V9H-L can increase the risk for carry over from one loop position to the next.*

5.8 Fractionation

Introduction

Fraction collector F9-C and **Fraction collector F9-R** collect fractions from ÄKTA pure purification runs. The fraction collectors are connected to ÄKTA pure and controlled by UNICORN. Control of the fraction collector can be achieved automatically in a method run, or manually.

In this section

This section contains the following subsections:

Section	See page
5.8.1 Prepare Fraction collector F9-C	191
5.8.2 Prepare Fraction collector F9-R	197
5.8.3 Fractionation overview	204

5.8.1 Prepare Fraction collector F9-C

About this section

This section describes how to prepare and assemble Fraction collector F9-C before a run.

The fraction collector is connected to ÄKTA pure and controlled by UNICORN. Control of the fraction collector can be achieved automatically in a method run, or manually.



CAUTION

Fire Hazard. Do not fractionate flammable liquids using Fraction collector F9-C.

When running RPC methods, or other procedures using organic solvents, collect fractions through the outlet valve or Fraction collector F9-R.

Note: *The tray and racks can tilt slightly when not fully inserted into the fraction collector and may harm the fractionation arm. The tilt is due to the height difference between the door and the floor of the fraction collector. The tendency to tilt is affected by the placement and weight of the cassettes, tubes or bottles*

Prepare the fraction collector

Before starting to prepare Fraction collector F9-C, check the fractionation settings in the method to be run. Perform the steps described below according to the settings in the method.

- Insert the Cassette tray or a rack for tubes or bottles.
- Change the **System Settings** in UNICORN to set the fractionation mode and other settings for fraction collection.

How to insert a tray or a rack is shown below.

For information on how to change the **System Settings** before a run, see UNICORN System Control Manual. The available **System Settings** are described in [Section 9.8.7 System settings - Fraction collection, on page 456](#).

Prepare and insert the Cassette tray

Follow the instructions below to add cassettes to the Cassette tray and insert the tray into the fraction collector.

Step	Action
1	If you are to use cassettes with the QuickRelease function, open the cassettes. For more information on the QuickRelease function see QuickRelease function, on page 98 .




- 2 Place the tubes and deep well plates in the cassettes. Make sure that the deep well plates are rotated so that the well marked **A1** is positioned above the **A1** marking on the cassette.





Step	Action
------	--------

- | | |
|---|--|
| 3 | Close the cassettes that have the QuickRelease function. |
|---|--|

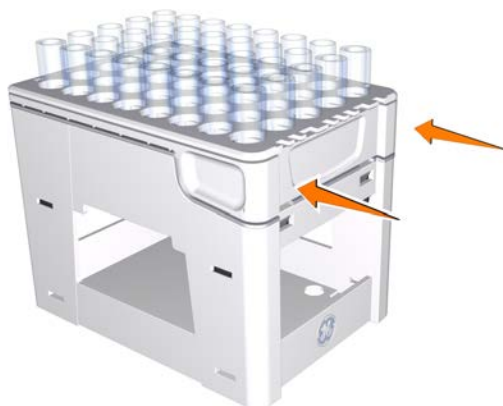


- | | |
|---|---|
| 4 | Place the cassettes on the Cassette tray. Make sure that the cassette type code (see illustration below) faces the front of the tray marked with the GE logo. |
|---|---|

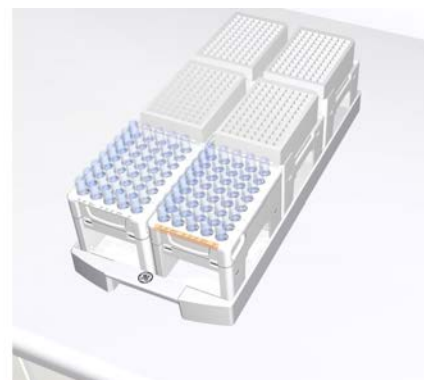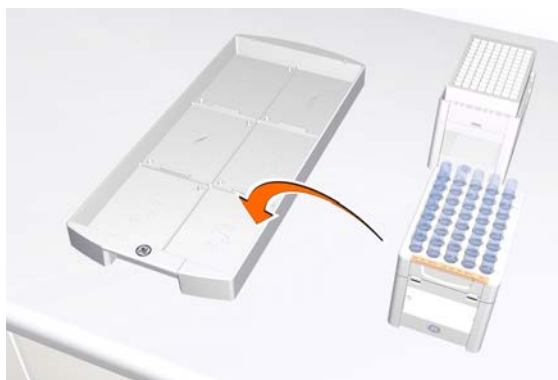


- | | |
|---|---|
| 5 | Open the door of the fraction collector using the handle. |
|---|---|

Step	Action
------	--------

- | | |
|---|---|
| 6 | <p>Insert the tray into the fraction collector:</p> <ul style="list-style-type: none"> • make sure that the front of the tray (marked with the GE logo) faces outwards • position the tray and slide it into the fractionation collector until it reaches the end |
|---|---|

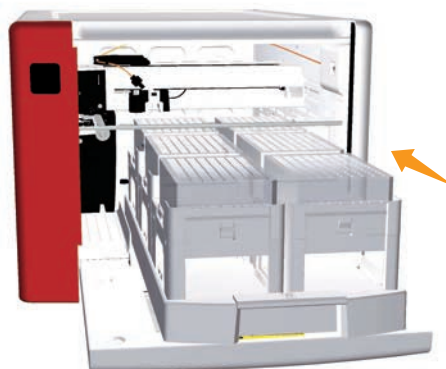

- make sure that the Tray catch snaps into closed position, as shown below.

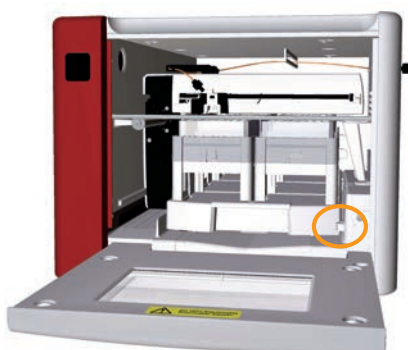

Note:

- The tray can tilt slightly when not fully inserted into the fraction collector and may harm the fractionation arm. The tilt is due to the height difference between the door and the floor of the fraction collector. The tendency to tilt is affected by the placement and weight of the cassettes.
- A height exclusion bar ensures that the tubes or deep well plates are correctly positioned and cannot damage the Dispenser head.

- | | |
|---|--|
| 7 | Close the door. Make sure that it closes properly. |
|---|--|

Result: After the door has been closed, the fractionation arm scans the cassette type code of each cassette to identify the cassette types. If deep well plates are used, the instrument also identifies the types of deep well plates.


Note:

If the tray is inserted with the front of the tray facing the wrong way it will not be possible to close the door.


Prepare and insert a rack for tubes or bottles

Follow the instructions below to insert a rack for tubes or bottles into the fraction collector.

Step	Action
1	Place the tubes or bottles in the rack.
2	Open the door of the fraction collector using the handle.
3	Insert the rack into the fraction collector: • make sure that the front of the rack (marked with the GE logo) faces outwards • position the rack and slide it into the fractionation collector until it reaches the end

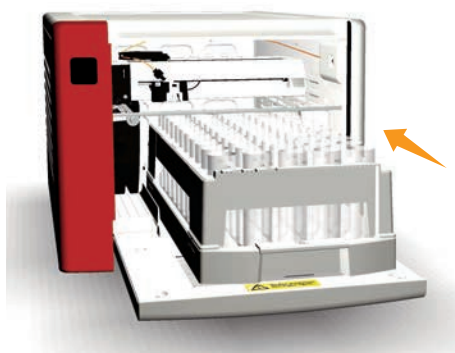

- make sure that the Tray catch snaps into closed position, as shown below.

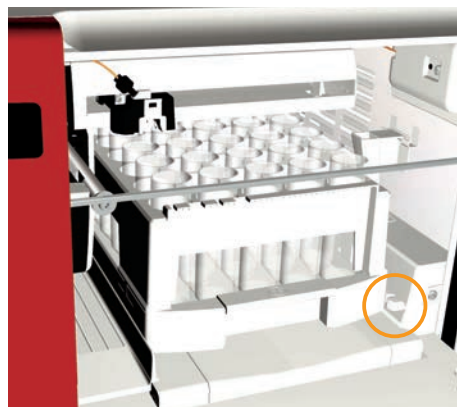

Note:

- The rack can tilt slightly when not fully inserted into the fraction collector and may harm the fractionation arm. The tilt is due to the height difference between the door and the floor of the fraction collector. The tendency to tilt is affected by the placement and weight of the tubes or bottles.
- A height exclusion bar ensures that the tubes or bottles are correctly positioned and cannot damage the Dispenser head.
- Do not use the Cassette tray when the Rack for 50 ml tubes or the Rack for 250 ml bottles is placed in the fraction collector.

5 Operation

5.8 Fractionation

5.8.1 Prepare Fraction collector F9-C

Step	Action
4	Close the door. Make sure that it closes properly. Note: <i>If the rack is inserted with the front of the rack facing the wrong way it will not be possible to close the door.</i>

5.8.2 Prepare Fraction collector F9-R

Introduction

This chapter describes how to prepare and assemble Fraction collector F9-R before a run.

Fraction collector F9-R is connected to ÄKTA pure and controlled by UNICORN. Control of the fraction collector can be achieved automatically in a method run, or manually.


Prepare the fraction collector

Before starting to prepare the Fraction collector F9-R, check the fractionation settings in the method to be run. Perform the steps described below according to the settings in the method.

- Assemble the Tube rack
- Insert collection tubes
- Adjust the Delivery arm
- Update **System Settings** in UNICORN

Assemble the Tube rack

Illustration of the Tube rack

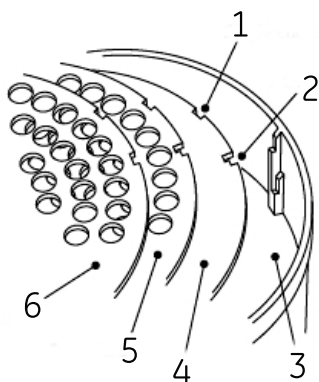

Part	Function
1	Single cutout
2	L-shaped cutout
3	Bowl
4	Tube support
5	Tube guide
6	Tube holder

Note: Note that the tube guide has both single and L-shaped cutouts, while the tube holder only has single cutouts.

Tube rack inserts

The Fraction collector F9-R is delivered with the 18 mm tube rack mounted. Each tube rack is made up of a combination of a Bowl, Tube support, Tube guide and Tube holder. Change the Tube holder and the Tube guide to collect fractions in 12 mm tubes or 30 mm tubes. The 12 mm tube rack is delivered with ÄKTA pure and the 30 mm tube rack is available as an accessory. The table below describes inserts and corresponding fraction collection tubes.

Inserts	Maximum number of tubes	Tube diameter	Tube length
12 mm Tube holder 12 mm Tube guide	175	12 mm	50 - 180 mm
18 mm Tube holder 18 mm Tube guide	95	18 mm	50 - 180 mm
30 mm Tube holder 30 mm Tube guide	40	30 mm	50 - 180 mm

Single and L-shaped cutouts

When assembling a tube rack, different cutouts are used for the various inserts depending on the length of the collection tubes. Which cutouts to use are summarized in the tables below.

12 mm and 18 mm Tube rack inserts

Inserts	50 - 85 mm tubes	85 - 180 mm tubes
Tube support	L-shaped cutout	Not required
Tube guide	Single cutout	L-shaped cutout
Tube holder	Single cutout	Single cutout

30 mm Tube rack inserts


Inserts	30 - 50 mm tubes ¹	50 - 85 mm tubes	85 - 180 mm tubes
Tube support	Single cutout	L-shaped cutout	Not required
Tube guide	Single cutout	Single cutout	L-shaped cutout
Tube holder	Single cutout	Single cutout	Single cutout

¹ For 30-50 mm tubes, first insert the tube guide from the 18 mm rack using the single cutout, before inserting the tube support for the 30 mm rack.

Assembly instructions

Follow the instructions below to assemble the Tube rack.


Step	Action
1	Insert the Tube support (4), if required, into the bowl (3). The circular marks on the Tube support should face down.




Note:

When assembling a Tube rack, Single cutouts (1) and L-shaped cutouts (2), are used for various inserts depending on the length of the collection tubes. See [Single and L-shaped cutouts, on page 198](#) for detailed information.

2	Insert the Tube guide (5) with the tube position numbers upwards. The Tube guide should rest about 1 cm above the Tube support.
3	Insert the Tube holder (6) with the tube position numbers upwards: Check that tube position 1 (7) is directly above tube position 1 (7) of the Tube guide.

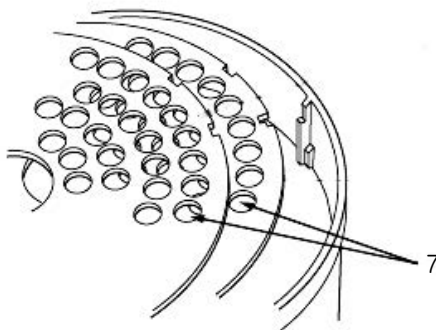


Step	Action
4	Push the flexible bowl out at each rib and snap the Tube holder under the top lip of the rib (8).

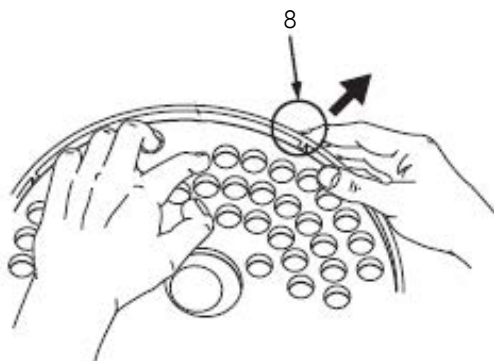

Note:

Do not force the tube holder into place as this may damage the lip.

- Check that the surface of the Tube holder is level.
- 5 Gently move the Delivery arm (10) out to the outer stop.
- 6 Place the Tube rack (9) over the Central spindle (11) and pull the spring loaded Drive sleeve (12) out so the Tube rack comes to rest.

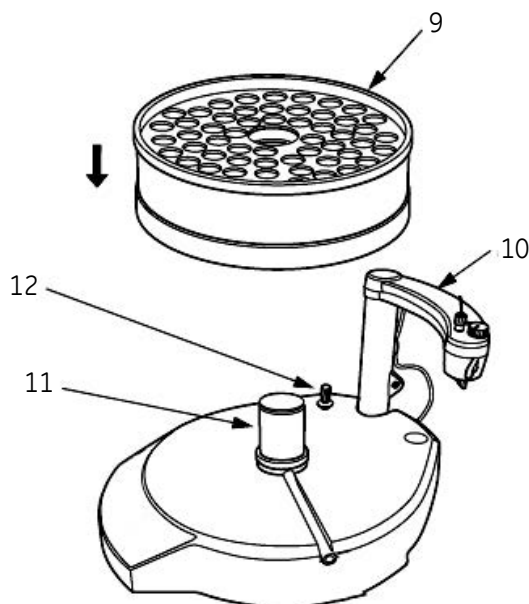


Insert collection tubes

Insert a sufficient number of collection tubes in to the Tube rack, starting at position 1, pushing each one down as far as they will go. All the tubes must be of the same length and diameter and there should be no spaces in the sequence.


Adjust the Delivery arm

Follow the instructions in the table below to adjust the height of the Delivery arm.


Step	Action
1	Lift and then lower the Delivery arm (1), and allow it to move in so the Tube sensor (2) touches the collection tubes of the outer track.

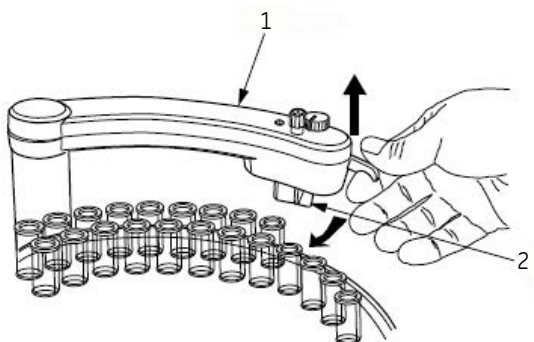


2	Loosen the lock knob (3)
---	--------------------------

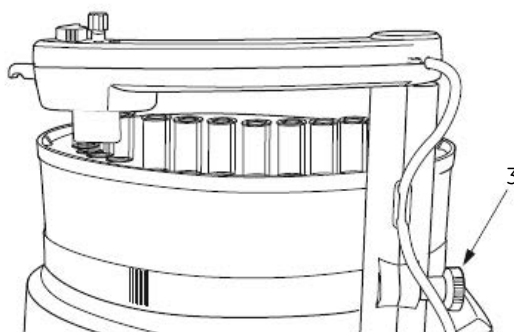

Step	Action
3	Adjust the height so that the horizontal mark (5) on the Tube sensor (6) is at the same level as the top of the flat collection tubes and approximately 2 mm over the top of the flanged collection tubes (4).

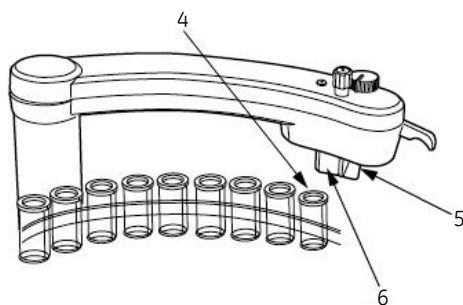

	Lock the Delivery arm at this height with the lock knob.
4	Check that the Tube sensor (9) is in the correct position for the tubes used (10). The eluent tubing (7) should be above the center of the collection tube.

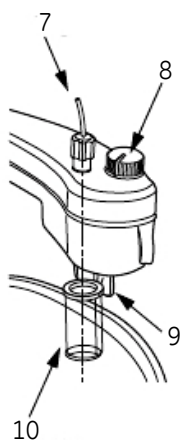

5	Use the Sensor control (8) to position the Tube holder over the center of the collection tube.
---	--

**NOTICE**

Never lift **Fraction collector F9-R** by the Delivery arm. This may damage the Fraction collector.

Sensor control

The sensor control can be switched between the two positions "small tubes" and "large tubes", indicated in the illustration below.



The position for large tubes is used for tubes of approximately 18 mm i.d. and larger. The position for small tubes is used for tubes smaller than 18 mm i.d.

Note that this is a rough approximation. Always check that the eluent tubing is centered above the collection tube.

5.8.3 Fractionation overview

Fractionation types


The table below lists the types of fractionation that the fraction collectors can be used for.

Type	Description
Fixed volume fractionation	During fixed volume fractionation the fraction collector continuously switches tubes according to the set volume throughout the entire fractionation. This type of fractionation is also known as straight fractionation.
Peak fractionation	Peak fractionation can be used to further increase the purity of the collected protein peaks and minimize the number of tubes used. The monitor signal is used to determine when to switch the tubes. See Section 9.8.10 System settings - Watch parameters, on page 461 for information about different watch options.
Combined fixed volume fractionation and peak fractionation	The two fractionation types listed above can be used in combination. Combination of fixed volume and peak fractionation allows fractions collected by fixed volume fractionation and fractions collected by peak fractionation to be directed to different collection tubes.

To be able to analyze different parts of the peak, the fraction size during elution is usually set to a value smaller than the expected peak volume.

Illustration


The illustration below shows examples of fractionation using fixed volume fractionation and fractionation using peak fractionation.

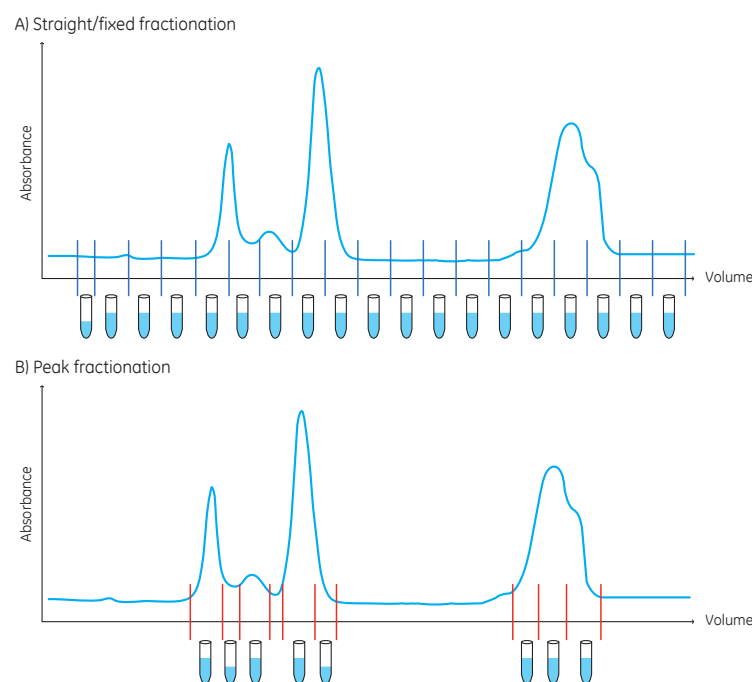

Delay volume

Description


The delay volume settings are used to make sure that the fractions collected during fractionation, using the outlet valve or the fraction collector, correspond to the fractions indicated in the chromatogram. The delay volume is the volume between the UV monitor, and the fraction collector or outlet that is used, see the illustration below.

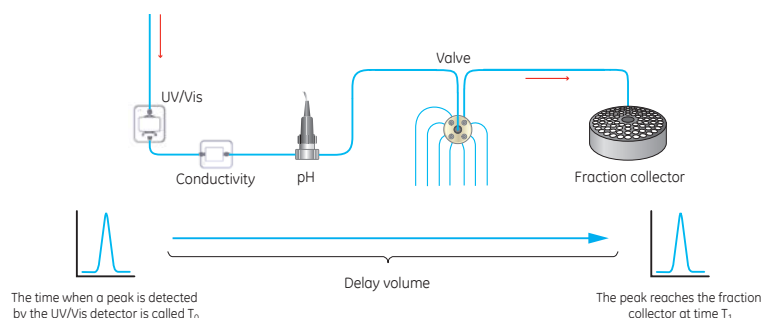

As the delay volume is affected by the length and diameter of the tubing, it should be set according to the tubing and modules used.

Illustration of fraction marking using fixed volume fractionation

The illustration below shows the fractions collected, and the numerical marking of fractions, when fixed volume (straight) fractionation is used with Fraction collector F9-R.

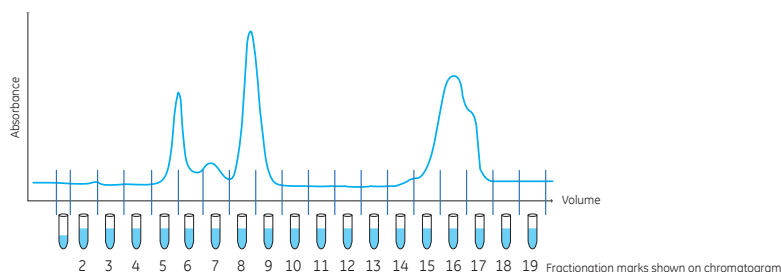


When fixed volume fractionation is used the delay volume is collected at the beginning of fractionation. Fraction collector F9-R saves the delay volume in the first fraction (fraction 1), see the example illustration above. Delay volumes are not indicated with a numerical fraction mark on the chromatogram. Fraction collector F9-C does not save the delay volume as a fraction, instead the delay volume is disposed of in the waste funnel.

Note: If two fraction collectors are used, the fractions collected by Fraction collector F9-R, 2nd are indicated by the prefix 2: (i.e. fractions **2:1**, **2:2**, **2:3** etc.).

Illustration of fractions and fraction marking using peak fractionation

The illustration below shows the fractions collected, and the numerical marking of fractions, when peak fractionation is used with Fraction collector F9-R.

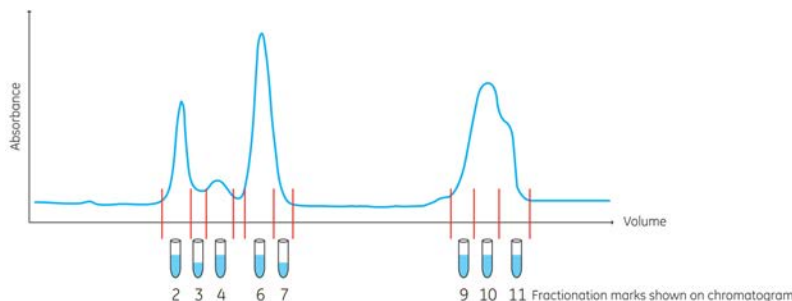

When peak fractionation is used, Fraction collector F9-R collects the delay volumes in the fractions preceeding each peak. In the chromatogram above, delay volumes are collected in fractions 1, 5 and 8. The numerical fraction marks for the delay volume fractions are not indicated on the chromatogram. Fraction collector F9-C does not save the delay volumes as fractions, instead the delay volumes are disposed of in the waste funnel.

Note: If two fraction collectors are used, the fractions collected by the second Fraction collector are indicated by the prefix 2: (i.e. fractions **2:1**, **2:2**, **2:3** etc.).

Fractionation modes for Fraction collector F9-C

There are three fractionation modes for Fraction collector F9-C, **Automatic**, **Accumulator** and **DropSync**. Spillage between collection vessels during a run is avoided with all three fractionation modes.

- **Automatic:** The fraction collector uses the Drop Sync mode for flow rates up to 2 ml/min and automatically switches to Accumulator mode for higher flow rates.
- **Accumulator:** Liquid is collected during movement between tubes or wells. The liquid is then dispensed in the next well or tube. Fractionation with accumulator can be used at all flow rates.
- **DropSync:** When using DropSync, the sensors in the Dispenser head detect when a drop is released from the nozzle. The Dispenser head moves to the next well or tube just after a drop is released. Fractionation with DropSync can be used at flow rates up to 2 ml/min. If only one Cassette is used and it is placed near the waste funnel, DropSync can be used at higher flow rates. Volatile solutions and solutions with low surface tension may require a lower flow.

Fractionation settings for Fraction collector F9-R

There are two fractionation settings for Fraction collector F9-R, **DropSync off** or **DropSync on**.

DropSync off: No synchronization of collection.

DropSync on: When using **DropSync** the sensors in the Tube sensor detect when a drop is released. The Tube rack moves and positions the next tube under the Tube sensor just after a drop is released. Fractionation with **DropSync** can be used at flow rates up to 2 ml/min. For water and solutions with higher surface tension, a higher flow rate can be used. Volatile solutions and solutions with low surface tension may require a lower flow.

Missing tubes in Fraction collector F9-R

If a tube is missing, Fraction collector F9-R will continue the fractionation on the tube row located closer to the center of the fraction collector. The fractionation marks in the chromatogram will then not reflect the tubes in which the sample is collected.

If the fraction collector runs out of tubes, the delivery arm moves to the fraction collector center position while ÄKTA pure pauses and displays an error message.

Missing tubes or plates in Fraction collector F9-C

When automatic cassette configuration is selected in the system settings the fraction collector automatically detects which types of cassettes and plates that are present. The fraction collector will however not detect if tubes or bottles are missing in the cassettes. Make sure that the cassettes to be used are occupied by appropriate types and numbers of tubes or bottles before starting a run.

It is not possible to change the cassette configuration during a run. When the system state is set to **Pause** it is possible to take out cassettes or plates from the fraction collector only if they are replaced by cassettes or plates of the same type and are placed in the same positions.

The action of the system when the last tube in the fraction collector is filled is set in the instruction **Last tube filled** in the system settings. The flow can be directed to waste or to any of the outlets or the run can be paused. If the action is set to **Pause**, the system automatically pauses when the last tube is filled and prompts the user to replace the filled tubes.

Peak broadening

The width of peaks at the fraction collector is influenced by the properties of the column and the dimensions of tubing connecting the components. Initial sample volume affects the peak width in gel filtration (GF) chromatography. A sample zone is broadened during passage through a GF column so that the sample is diluted and the resolution decreases with increasing sample volume. Sample volume does not however affect the resolution in adsorption chromatography techniques such as affinity chromatography (AC), ion exchange chromatography (IEX), and hydrophobic interaction chromatography (HIC). The effect of peak broadening in the system from sample injection to peak detection (including dilution on the column) is apparent in the chromatogram from the UV monitor, but broadening from the UV monitor to fraction collection is not visible in the chromatogram. This "hidden" effect can sometimes be dramatic, especially for high-resolution columns.

To minimize peak broadening, use narrow and short tubing connections as far as possible. Remember that using narrow tubing will increase the back pressure in the system.

5.9 Create a method and perform a run

Introduction

This section provides an overview of how to create a method in UNICORN and how to perform manual and method runs on ÄKTA pure.

It also contains advice on things to be considered during a run.

In this section

This section contains the following sub-sections:

Section	See page
5.9.1 Create a method	209
5.9.2 Prepare and perform a run	214
5.9.3 Monitor a run	216
5.9.4 After run procedures	218

5.9.1 Create a method

Introduction

The predefined methods are built up using phases, where each phase corresponds to a step in a chromatography run with a number of properties associated with that phase.

See UNICORN Method Manual for more information about method structure, definitions and concepts of methods in UNICORN.

Predefined methods

There are several predefined methods to choose from. All the predefined methods are listed below.

The predefined methods available for each system are defined by the Instrument Configuration. Refer to [Section 9.7 Predefined methods and phases, on page 436](#) for more information about each method.

Purification methods

- Affinity Chromatography (AC)
- Affinity Chromatography (AC) with Tag Removal
- Anion Exchange Chromatography (AEX)
- Cation Exchange Chromatography (CEX)
- Chromatofocusing (CF)
- Desalting
- Gel filtration (GF)
- Hydrophobic Interaction Chromatography (HIC)
- Manual Loop Fill
- NHS-coupling
- Reversed Phase Chromatography (RPC)

Maintenance methods

- Column CIP
 - Column Performance Test
 - Column Preparation
 - System CIP
 - System Preparation
-

Main steps when defining a new method

The main steps when defining a method are:

- 1 Create/open a method
 - Create a **Predefined** method (including a set of phases that may be edited)

5 Operation

5.9 Create a method and perform a run

5.9.1 Create a method

or

- Open an existing method that can be edited and saved with a new name or overwritten
- 2 Build/edit the **Method Outline** and/or edit the **Phase Properties** for the appropriate phases
 - 3 Save the method

Create a new method

Follow the instructions below to create a new method.


Step	Action
------	--------

- | | |
|---|---|
| 1 | In the Method Editor : <ul style="list-style-type: none">• click the Create a new method icon in the Toolbar |
|---|---|




or

- select **File:New Method...**



Result: The **New Method** dialog opens.

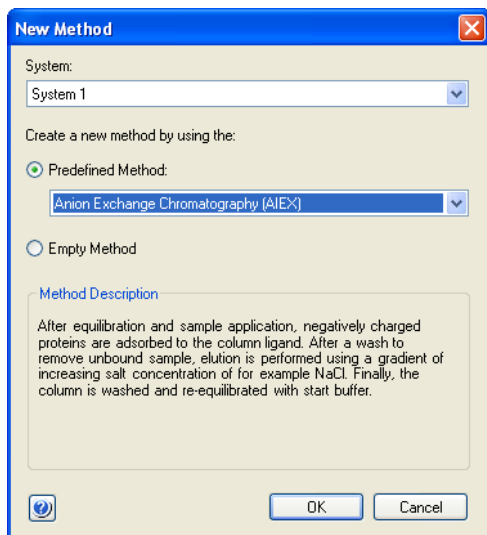


Step	Action
2	In the New Method dialog: - select a System - select a Predefined Method - click OK <i>Result:</i> The Method Outline pane shows the included phases for the chosen method and the Phase Properties pane shows the default settings for the currently highlighted phase.

See UNICORN Method Manual for more information about methods and method creation in UNICORN.

Note: *Sample loop is called capillary loop in UNICORN.*

Text Instruction mode

In most cases methods can be edited using the **Phase Properties** pane in the **Method Editor** module. However, modules without a recommended position are not supported by **Phase Properties** and have to be edited in the **Text Instruction** mode.

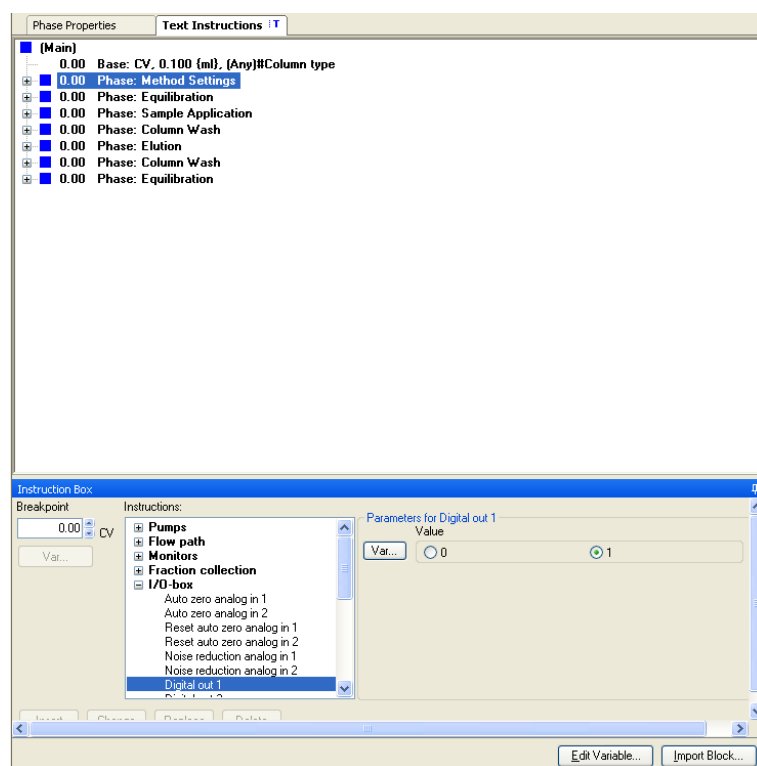

The following modules require that the method is created using the **Text Instruction** mode:

- Inlet valve IX

Note: *When using Inlet valve IX (V9-IX or V9H-IX) connected to another inlet valve in a run, it is necessary to use the instructions for both Inlet valve IX and the other inlet valve, respectively.*

5 Operation

5.9 Create a method and perform a run

5.9.1 Create a method

- Versatile valve
- I/O-box
- UV monitor, 2nd


Note: It is possible to reset the UV monitor **U9-L**, 2nd using **Phase Properties**. All other UV monitor **U9-L**, 2nd instructions need to be edited in the **Text Instruction** mode.


Note: If installing more than one external air sensor, it is necessary to create the methods for the additional air sensors using the **Text Instruction** mode.

Open and save methods for different systems

New ÄKTA pure methods are always created for the set of components of the current system. Methods can be shared between systems, with the restriction that a method created for an ÄKTA pure 150 configured system cannot be used with an ÄKTA pure 25 configured system, and vice versa.

When a method is opened for a system that has been changed or if a method is saved for a system with a different flow configuration, a dialog is opened where the user can choose to either adapt the method or to keep the text method unchanged.

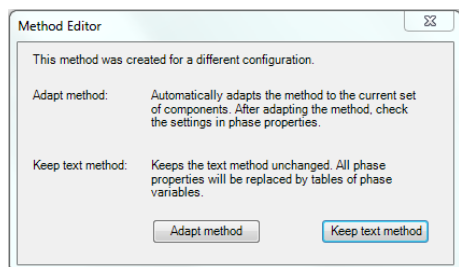

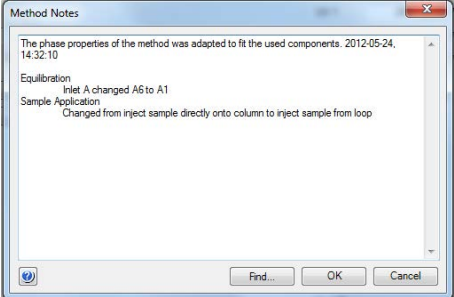If you select..	Then..
Adapt method	the method will be adapted to the new set of components. All functions and positions that are still available will be unchanged. For example, valve positions present on both the original and the new system will be unchanged in the adapted method. Non-compatible settings will be adjusted in order to properly adapt the method for new components. Settings that have been changed are described and saved in Method Notes, which are displayed after the method has been adapted.  Change the settings in Phase Properties if required. Note: <i>Some predefined methods require certain components to be functional. Adapting these methods to systems that do not include the required components is not possible.</i>
Keep text method	the text method will be kept and nothing will be changed. Non-compatible settings will still be present in the method but they will not be functional. All Phase Properties of the method will be replaced by tables of Phase Variables.

5.9.2 Prepare and perform a run

Introduction

This section describes how to start a run using a previously created method and how to perform a manual run. For further information about the capabilities of the **System Control** module, refer to *UNICORN System Control Manual*.

Choose and start a method


The following instruction describes how to open a method and start a run.

Step	Action																				
1	Open the System Control module and click the icon Open Method Navigator. <i>Result:</i> The Method Navigator pane opens. <table> <tr> <th>Folder name</th><th>System</th><th>Last modified</th><th>Created by</th></tr> <tr> <td>DoeMethod</td><td></td><td>2014-10-06 14:3...</td><td>Default</td></tr> <tr> <td>Elvis</td><td></td><td>2012-11-27 14:5...</td><td>Default</td></tr> <tr> <td>AutoTests 2013-05-31</td><td></td><td>2013-05-31 12:0...</td><td>Default</td></tr> <tr> <td>Elvis 1</td><td></td><td>2012-11-27 14:5...</td><td>Default</td></tr> </table>	Folder name	System	Last modified	Created by	DoeMethod		2014-10-06 14:3...	Default	Elvis		2012-11-27 14:5...	Default	AutoTests 2013-05-31		2013-05-31 12:0...	Default	Elvis 1		2012-11-27 14:5...	Default
Folder name	System	Last modified	Created by																		
DoeMethod		2014-10-06 14:3...	Default																		
Elvis		2012-11-27 14:5...	Default																		
AutoTests 2013-05-31		2013-05-31 12:0...	Default																		
Elvis 1		2012-11-27 14:5...	Default																		
2	Select the method to run, and click the Run icon. <i>Result:</i> The Start Protocol dialog opens.																				
3	Step through the displayed pages in the Start Protocol, add requested input and make appropriate changes if necessary. Click Next.																				
4	Click Start on the last page of the Start Protocol. <i>Result:</i> • If column logging was chosen during installation of UNICORN and a column type was selected when the method was created, the Select Columns dialog opens. For further information on column handling, please refer to <i>UNICORN Method Manual</i> and <i>UNICORN System Control Manual</i>. • If column logging was <i>not</i> chosen during installation of UNICORN and/or <i>no</i> column type was selected when the method was created, the run starts directly.																				

Perform a manual run

Manual runs can be convenient for procedures such as filling tubing with buffer or packing a column with media.

Step	Action
1	On the Manual menu, click Execute Manual Instructions .
2	Select instruction group and instruction.
3	Select or enter parameter values.
4	Click Insert to have several instructions performed at the same breakpoint.
	Note: Manual runs are only stored temporarily. However, you can choose to store them permanently in a selected directory. To save results in a chosen directory, click Browse before the run is started. Note: If a method run is started during a manual run, the results from the manual run are not stored.
5	To perform the instructions, click Execute .

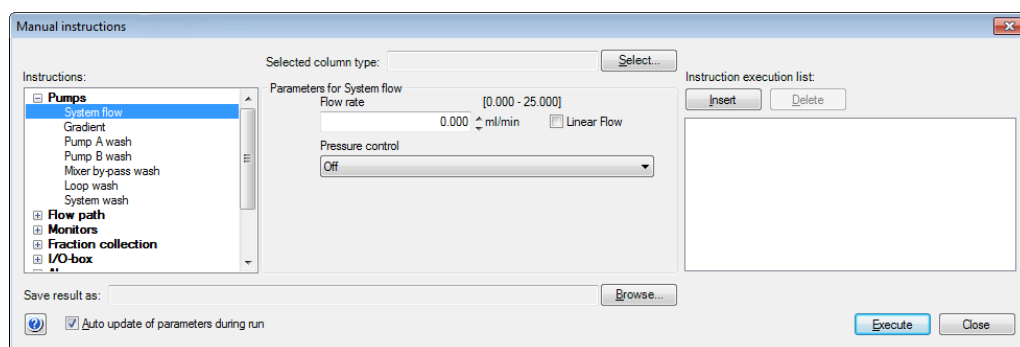

5.9.3 Monitor a run

Introduction

During the run, the **System Control** module will display the run progress of the method being executed. This section describes how to interact with the run from the process picture or by executing manual instructions.

To find an overview of the **System Control** user interface, see UNICORN System Control Manual.

Monitor the run

To interrupt a method during a run you may use the **Hold**, **Pause** or **End** icons in **System Control**. A held or paused method run can be resumed by using the **Continue** icon. See the instructions in the table below.


If you want to...	then...
temporarily hold the method, with current flow rate and valve positions sustained	click the  button.
temporarily pause the method, and stop all pumps	click the  button.
resume, for example, a held or paused method run.	click the  button. Note: <i>An ended method cannot be resumed.</i>
permanently end the run	click the  button.

Note: When ending a method run in advance, it is possible to save the partial result.

More information regarding UNICORN capabilities during the method run is available in the UNICORN System Control Manual.

Actions in the process picture pane

It is possible to manually interact with an ongoing method through the **Process Picture**, see UNICORN System Control Manual.

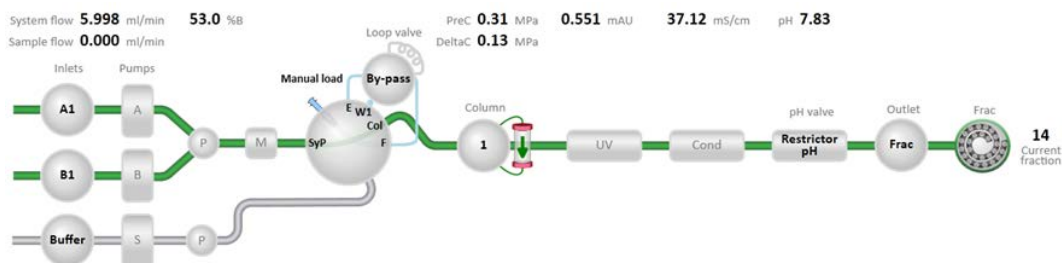

Using UNICORN to control the pressure during a run

The function **Pressure control** allows a method to be run with the set flow rate without the risk of a method stop due to pressure alarm. Pressure control is enabled in the instructions **System flow** and **Sample flow**. Refer to [Section 9.15 Pressure control, on page 499](#) for more information.

The system configuration affects the pressure

Using narrow tubing between components will improve resolution but will lead to increased back pressure in the system. Narrow tubing after the column will increase the pressure in the column at a given flow rate. Make sure that the sensor limits for the pre-column pressure are set so that the maximum pressure for the column in use is not exceeded.

Note: If Column valve **V9-C** or **V9H-C** is mounted, the integrated pressure sensor of the valve allows the system to monitor the post-column pressure. The limit for the pressure sensor in Column valve **V9-C** or **V9H-C** is automatically set so that the UV monitor and the pH monitor are protected from high pressure. If Column valve **V9-C** or **V9H-C** is not mounted, make sure to keep the pressure in the system after the column below the pressure limits for the modules in the flow path.

5.9.4 After run procedures

Introduction

This section describes how to clean the instrument and columns after a chromatographic run, and how to prepare the system for storage.

The instrument and the columns should be cleaned between the runs. This will prevent, for example, sample contamination, protein precipitation and column clogging. If the instrument is not going to be used for a couple of days or longer, the instrument, columns and the pH flow cell should be filled with storage solution. For further information about cleaning and maintenance procedures, see [Chapter 7 Maintenance, on page 248](#).

Tip: To clean and fill the instrument and columns with storage solution, use **System CIP** and **Column CIP** either as separate, predefined methods or as phases included in a chromatographic method.



CAUTION

Hazardous chemicals and biological agents. Before maintenance, service and decommissioning, wash the ÄKTA pure instrument with a neutral solution to make sure that any hazardous solvents and biological agents have been flushed out from the system.

System cleaning

After a method run is completed, perform the following:

- Rinse the instrument with one or several cleaning solution(s) (e.g., NaOH, buffer solution or distilled water) using **System CIP**.

Note: If Column valve **V9-C** or **V9H-C** is mounted, the integrated pressure sensor of the valve allows the system to monitor the post-column pressure. The limit for the pressure sensor in Column valve **V9-C** or **V9H-C** is automatically set so that the UV monitor and the pH monitor are protected from high pressure. If Column valve **V9-C** or **V9H-C** is not mounted, make sure to keep the pressure in the system after the column below the pressure limits for the modules in the flow path.

- If applicable, empty the fraction collector.
- Clean all spills on the instrument and on the bench using a moist tissue.
- Empty the waste vessel.
- Clean the manual injection port of the injection valve, see [Section 7.6.2 Perform System CIP, on page 275](#) for detailed instructions.
- If applicable, clean the pH electrode manually and make sure to leave it in an appropriate buffer. See [Section 7.6.7 Clean the pH electrode, on page 290](#) for detailed instructions.

System storage

If the instrument is not going to be used for a couple of days or longer, also perform the following:

- Fill the system and inlets with storage solution (e.g., 20% ethanol) using **System CIP**.
Note: *If Column valve **V9-C** or **V9H-C** is mounted, the integrated pressure sensor of the valve allows the system to monitor the post-column pressure. The limit for the pressure sensor in Column valve **V9-C** or **V9H-C** is automatically set so that the UV monitor and the pH monitor are protected from high pressure. If Column valve **V9-C** or **V9H-C** is not mounted, make sure to keep the pressure in the system after the column below the pressure limits for the modules in the flow path.*
 - If applicable, prepare the pH electrode for storage as described in [Section 7.6.6 Storage of the pH electrode, on page 288](#).
-

Column cleaning

After a method run is completed, perform the following:

- Clean the column with one or several cleaning solution(s) using **Column CIP**.
-

Column storage

If the column is not going to be used for a couple of days or longer, also perform the following:

- Fill the column with storage solution (e.g., 20% ethanol) using **Column CIP**.
-

pH electrode storage

If pH monitoring will not be used for a week or longer, perform one of the following actions:

- Inject new storage solution into the pH flow cell. Refer to [Section 7.6.6 Storage of the pH electrode, on page 288](#) for instructions.
- Replace the pH electrode with the dummy electrode that is installed in the pH valve on delivery.



In the following situations, in order to increase the lifetime of the pH electrode, use the **By-pass** position and store the electrode in storage solution inside the pH flow cell:

- pH monitoring is not needed during the run.
- Organic solutions are used.
- Extremely acidic or extremely basic solutions are used.

For further information on how to prepare the pH electrode for storage, refer to [Section 7.6.6 Storage of the pH electrode, on page 288](#).

Log off or exit UNICORN

Follow the instructions to log off or exit UNICORN. This can be performed from any of the UNICORN modules.

If you want to...	then...
log off UNICORN	on the File menu, click Log off.  <i>Result:</i> All open UNICORN modules close and the Log On dialog opens.
exit UNICORN	on the File menu, click Exit UNICORN.  <i>Result:</i> All open UNICORN modules close.

Note: If an edited method or result is open and not saved when you try to exit or log off UNICORN, you will see a warning. Click **Yes** to save, **No** to exit without saving, or **Cancel** to stay logged on.

Shut down the instrument

Switch off the instrument by pressing the power switch to the **O** position.



6 Performance tests

About this chapter

This chapter provides information about performance tests.

Performance tests should be run after installation to check the function of the ÄKTA pure system. Different tests are available and the tests to perform depend on the system configuration used.

Performance tests can also be used at any time to check the condition of the system, for example, after a prolonged stop. This chapter describes how to prepare, run, and evaluate the different performance tests available.

In this chapter

This chapter contains the following sections:

Section	See page
6.1 General performance test actions	222
6.2 Air sensor A and Inlet valve A tests	225
6.3 Air sensor B and Inlet valve B tests	227
6.4 Air sensor S and Sample inlet valve tests	229
6.5 Column valve C tests	231
6.6 Fraction collector F9-C test	233
6.7 Fraction Collector F9-R Test	236
6.8 Sample pump tests	238
6.9 System Test UV U9-L (fixed)	240
6.10 System Test UV U9-M (variable)	244

6.1 General performance test actions

Introduction

Some actions are identical for each performance test. These actions are described in this section.


Start the performance tests

Follow the instructions to start a performance test.

Step	Action																				
1	In the System Control module, on the System menu, click Performance Test and Report . <i>Result:</i> The System Performance Test and Report dialog opens.																				
2	In the System Performance Test and Report dialog, click one of the following tests: <table><tr><th>ÄKTA pure 25</th><th>ÄKTA pure 150</th></tr><tr><td>Air sensor A and inlet valve V9-IA test</td><td>Air sensor A and inlet valve V9H-IA test</td></tr><tr><td>Air sensor B and inlet valve V9-IB test</td><td>Air sensor B and inlet valve V9H-IB test</td></tr><tr><td>Air sensor S and Sample inlet valve V9-IS test</td><td>Air sensor S and Sample inlet valve V9H-IS test</td></tr><tr><td>Column valve V9-C test</td><td>Column valve V9H-C test</td></tr><tr><td>Fraction Collector F9-R Test</td><td>Fraction Collector F9-R Test</td></tr><tr><td>Fraction Collector F9-C Test</td><td>Fraction Collector F9-C Test</td></tr><tr><td>Sample pump S9 test</td><td>Sample pump S9H test</td></tr><tr><td>System Test UV U9-L (fixed)</td><td>System Test UV U9-L (fixed)</td></tr><tr><td>System Test UV U9-M (variable)</td><td>System Test UV U9-M (variable)</td></tr></table>	ÄKTA pure 25	ÄKTA pure 150	Air sensor A and inlet valve V9-IA test	Air sensor A and inlet valve V9H-IA test	Air sensor B and inlet valve V9-IB test	Air sensor B and inlet valve V9H-IB test	Air sensor S and Sample inlet valve V9-IS test	Air sensor S and Sample inlet valve V9H-IS test	Column valve V9-C test	Column valve V9H-C test	Fraction Collector F9-R Test	Fraction Collector F9-R Test	Fraction Collector F9-C Test	Fraction Collector F9-C Test	Sample pump S9 test	Sample pump S9H test	System Test UV U9-L (fixed)	System Test UV U9-L (fixed)	System Test UV U9-M (variable)	System Test UV U9-M (variable)
ÄKTA pure 25	ÄKTA pure 150																				
Air sensor A and inlet valve V9-IA test	Air sensor A and inlet valve V9H-IA test																				
Air sensor B and inlet valve V9-IB test	Air sensor B and inlet valve V9H-IB test																				
Air sensor S and Sample inlet valve V9-IS test	Air sensor S and Sample inlet valve V9H-IS test																				
Column valve V9-C test	Column valve V9H-C test																				
Fraction Collector F9-R Test	Fraction Collector F9-R Test																				
Fraction Collector F9-C Test	Fraction Collector F9-C Test																				
Sample pump S9 test	Sample pump S9H test																				
System Test UV U9-L (fixed)	System Test UV U9-L (fixed)																				
System Test UV U9-M (variable)	System Test UV U9-M (variable)																				
3	Click Run Performance Method . <i>Result:</i> The Start Protocol dialog of the selected test opens.																				
4	Click Next in the Start Protocol dialog to open the next page. The pages are described in the table Overview of the Start Protocol dialog, on page 223 .																				
5	In the last page, Result name and location , click Start . <i>Result:</i> The selected test starts.																				

Overview of the Start Protocol dialog

The following table describes the pages of the Start Protocol.

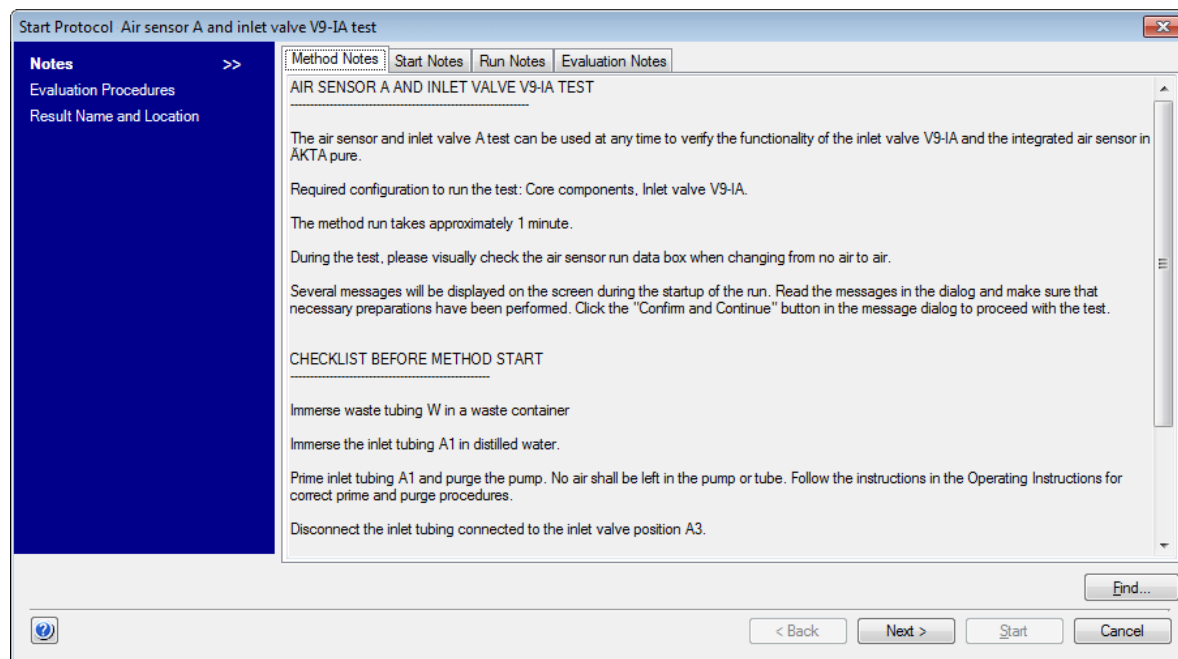

Page	Description
Notes	Displays the Method Notes of the method. The Method Notes contains a method description and instructions on how to run the method. This dialog also allows the user to enter Start Notes .
Evaluation Procedures	Allows the user to select to save the report to file (recommended) and/or to print the report.
Result Name and Location	Allows the user to change result name and result location.

During the run

A **Message** dialog opens during the run. Read the messages in the dialog, and make sure that necessary preparations have been performed.

- Click **Confirm and Continue** in the **Message** dialog to change system state from **System Pause** to **Run** and proceed with the test.
- Alternatively, click **Confirm** in the **Message** dialog and click the **Continue** button on the Instrument display.

Automatic evaluation

The system automatically generates a report when the test is finished. The report can be printed in two ways:

- It is recommended to select **Save the report to file** in the **Evaluation Procedures** page of the **Start Protocol** dialog when starting the test. The report is saved in the folder `Temp` in your UNICORN installation folder. For example `C:\Program Files\GE Healthcare\UNICORN\UNICORN 7.0\Temp`.
- If the option **Print report** was selected in the **Evaluation Procedures** page of the **Start Protocol** dialog when starting the test, the report is also automatically printed on the system printer. Refer to UNICORN Administration and Technical Manual for information on how to install a printer.

Print the report and check the status of the tests. For each of the tests the report states "The test passed" or "The test failed".

Note: *The fraction collector test is evaluated manually and no report is generated.*

6.2 Air sensor A and Inlet valve A tests

Air sensor A and Inlet valve A tests

The following Air sensor A and Inlet valve A tests are available, for ÄKTA pure 25 and ÄKTA pure 150, respectively:

- *Air sensor A and inlet valve V9-IA test*
- *Air sensor A and inlet valve V9H-IA test*

Method description

The Air sensor A and inlet valve A tests switches inlet valve A, labeled **V9-IA** or **V9H-IA**, to an empty position and checks if the air sensor detects air.

The method run takes approximately 1 minute.

Required configuration

A correctly installed Inlet valve A is required to run the test.

Required material

The following materials are required:

- Syringe, 25-30 ml
- Distilled water

Prepare the test

Follow the instructions below to prepare the system before method start.

Step	Action
1	Direct the outlet tubing marked W to a waste container.
2	Place inlet tubing A1 into distilled water.
3	Prime the A1 inlet and purge the pump. See Section 5.4.1 System pumps, on page 159 .
4	Disconnect the inlet tubing connected to the A3 inlet valve position. During the test method air is introduced into the inlet valve through that inlet port to test the function of the air sensor.

Run and evaluate the test

Follow the instructions described in [Section 6.1 General performance test actions, on page 222](#) to start, run and automatically evaluate the performance test.

Possible causes of a failed test

The tables below describe possible causes of a failed test. When possible sources of error have been checked and corrected, repeat the test.

Faulty air sensor A test

Cause	Action
Faulty air sensor	For further information, see Section 8.4 Troubleshooting: Valves, on page 372 .
Incorrect preparation of tubing	Make sure that the tubing was correctly prepared, see Prepare the test, on page 225 .

Faulty inlet valve A test

Cause	Action
The valve did not switch	For further information, see Section 8.4 Troubleshooting: Valves, on page 372 .

6.3 Air sensor B and Inlet valve B tests

Air sensor B and Inlet valve B tests

The following Air sensor B and Inlet valve B tests are available, for ÄKTA pure 25 and ÄKTA pure 150, respectively:

- *Air sensor B and inlet valve V9-IB test*
- *Air sensor B and inlet valve V9H-IB test*

Method description

The Air sensor B and inlet valve B test switches the inlet valve B, labeled **V9-IB** or **V9H-IB**, to an empty position and checks if the air sensor detects air.

The method run takes approximately 1 minute.

Required configuration

A correctly installed Inlet valve B is required to run the test.

Required material

The following materials are required:

- Syringe, 25-30 ml
- Distilled water

Prepare the test

Follow the instructions below to prepare the system before method start.

Step	Action
1	Direct the outlet tubing marked W to a waste container.
2	Place inlet tubing B1 into distilled water.
3	Prime the B1 inlet and purge the pump. See Section 5.4.1 System pumps, on page 159 .
4	Disconnect the inlet tubing connected to inlet valve position B3 . During the test method air is introduced into the inlet valve through that inlet port to test the function of the air sensor.

Run and evaluate the test

Follow the instructions described in [Section 6.1 General performance test actions, on page 222](#) to start, run and automatically evaluate the performance test.

Possible causes of a failed test

The tables below describe possible causes of a failed test. When possible sources of error have been checked and corrected, repeat the test.

Faulty air sensor B test

Cause	Action
Faulty air sensor	For further information, see Section 8.4 Troubleshooting: Valves, on page 372 .
Incorrect preparation of tubing	Make sure that the tubing was correctly prepared, see Prepare the test, on page 227 .

Faulty inlet valve B test

Cause	Action
The valve did not switch	For further information, see Section 8.4 Troubleshooting: Valves, on page 372 .

6.4 Air sensor S and Sample inlet valve tests

Air sensor S and Sample inlet valve tests

The following Air sensor S and Sample inlet valve tests are available, for ÄKTA pure 25 and ÄKTA pure 150, respectively:

- **Air sensor S and Sample inlet valve V9-IS test**
- **Air sensor S and Sample inlet valve V9H-IS test**

Method description

The Air sensor S and Sample inlet valve test checks the functionality of the Sample inlet valve, labeled **V9-IS** or **V9H-IS**, and the integrated air sensor in ÄKTA pure.

The method run takes approximately 1 minute.

Required configuration

Core components of the ÄKTA pure and correctly installed Sample Inlet valve and Sample pump are required to run the test.

Required material

The following materials are required:

- Syringe, 25-30 ml
- Distilled water

Prepare the test

Follow the instructions below to prepare the system before method start.

Step	Action
1	Open System Control and update the system setting Tubing: Sample pump to injection valve (found in System Settings:Tubing and Delay volumes). Note: <i>The system setting Tubing: Sample pump to injection valve is available only if Column valve C is not included in the system.</i>
2	Immerse waste tubing W in a waste container
3	Immerse sample inlet tubing Buffer in distilled water.
4	Prime inlet tubing A1 and sample inlet Buffer and purge the sample pump. See Section 5.4 Prime inlets and purge pump heads, on page 158 . No air shall be left in the pumps or tubings.

Step	Action
5	Disconnect the inlet tubing connected to the sample inlet valve position S3 . During the test method air is introduced into the sample inlet valve through that inlet port to test the function of the air sensor.

Run and evaluate the test

Follow the instructions described in [Section 6.1 General performance test actions, on page 222](#) to start, run and automatically evaluate the performance test.

Possible causes of a failed test

The tables below describe possible causes of a failed test. When possible sources of error have been checked and corrected, repeat the test.

Faulty air sensor S test

Cause	Action
Faulty air sensor	For further information, see Section 8.4 Troubleshooting: Valves, on page 372 .
Incorrect preparation of tubing	Make sure that the tubing was correctly prepared, see Prepare the test, on page 227 .

Faulty Sample inlet valve test

Cause	Action
The valve did not switch	For further information, see Section 8.4 Troubleshooting: Valves, on page 372 .

6.5 Column valve C tests

Column valve C tests

The following Column valve C tests are available, for ÄKTA pure 25 and ÄKTA pure 150, respectively:

- **Column valve V9-C test**
 - **Column valve V9H-C test**
-

Method description

The Column valve C test checks the functionality of Column valve C, labeled **V9-C** or **V9H-C**, and of the integrated pressure sensors that measure pre-column and post-column pressure.

The method run takes approximately 1 minute.

Required configuration

A correctly installed Column valve C is required to run the test.

Required material

The following materials are required:

- Syringe, 25-30 ml
 - Distilled water
 - **Ref 1** tubing, see [Reference capillary, on page 425](#).
-

Prepare the test

Follow the instructions below to prepare the system before method start.

Step	Action
1	Connect the Ref 1 tubing between Column valve C ports 1A and 1B .
2	Make sure the Flow restrictor is inline.
3	Direct outlet tubing W to a waste container.
4	Place inlet tubing A1 into distilled water.
5	Prime the inlet A1 and purge the pump. See Section 5.4.1 System pumps, on page 159 .

Run and evaluate the test

Follow the instructions described in [Section 6.1 General performance test actions, on page 222](#) to start, run and automatically evaluate the performance test.

Possible causes of a failed test

The table below describes possible causes of a failed test. When possible sources of error have been checked and corrected, repeat the test.

Cause	Action
Faulty Column valve	For further information, see Section 8.4 Troubleshooting: Valves, on page 372 .
The integrated pressure monitors are not calibrated	Calibrate the pressure monitors, see Section 7.7.2 Calibrate the pressure monitors, on page 302 .
Incorrect preparation of the system	Make sure that the reference tubing is connected between column ports 1A and 1B and that the flow restrictor is in-line.

6.6 Fraction collector F9-C test

Method description

The Fraction Collector Test checks the functionality of **Fraction collector F9-C**.

The method run takes approximately 6 minutes.

Required configuration

The core components of ÄKTA pure, an outlet valve and a correctly installed **Fraction collector F9-C** are required to run the test.

Required material

The following materials are required:

- Distilled water
 - Syringe, 25-30 ml
 - Two deep well cassettes
 - Two 96 deep well plates for collecting the fractions
-

Prepare the test

Follow the instructions below to prepare the system before method start.

Step	Action
1	Immerse waste tubing W in a waste container
2	Immerse inlet tubing A1 in distilled water.
3	Prime inlet tubing A1 and purge System pump A. See Section 5.4.1 System pumps, on page 159 . No air shall be left in the pump or tubing.
4	Place two 96 deep well plates in positions 1 and 6 in the fraction collector. Make sure that no other cassettes are present in the fraction collector during the run.
5	In the System Control module, select System:Settings . <i>Result:</i> The System Settings dialog opens.
6	In the System Settings dialog: • Select Fraction collection:Fractionation settings. • In the Fraction mode field, select Automatic. • In the Fractionation order field, select Row-Automaticby-Row. • Click OK.

Step	Action
7	In the System Settings dialog: • Select Tubing and Delay volumes. • Select the instruction Delay volume: Monitor to frac • Set the correct delay volume, see Section 9.13 Delay volumes, on page 492 • Click OK.

Run and evaluate the test

Follow the instructions described in [Section 6.1 General performance test actions, on page 222](#) to start and run the performance test.

During the run

- Visually check that the fraction collector wash is performed.
- Several messages will be displayed on the screen during the startup of the run. Read the messages in the dialog and make sure that necessary preparations have been performed. Click the "Confirm and Continue" button in the message dialog to proceed with the test.

Evaluate the result

To evaluate the results, do the following:

- Check that correct volumes, 2 ml/well, are collected in the three first wells in row A (A1-A3) of both plates.
- Check if the fractionation marks in the chromatogram are in accordance with the filled wells. For further information on delay volumes and fractionation marks, see [Delay volume, on page 205](#).

Possible causes of a failed test

The table below describes possible causes of a failed test. When possible sources of error have been checked and corrected, repeat the test.

Cause	Action
Incorrect volumes collected in the tubes, and disturbances of system pressure curves: - Air trapped in System pump A - Faulty System pump A	Air in pumps: Make sure to prime inlet tubing A1 and purge System pump A before method start, see Section 5.4.1 System pumps, on page 159 . Faulty pump: See Section 8.6 Troubleshooting: Pumps, on page 384 .
Incorrect preparation of buffer and tubing	Make sure that the system was correctly prepared, see Prepare the test, on page 233 .

6.7 Fraction Collector F9-R Test

Method description

The Fraction collector F9-R test checks the functionality of **Fraction collector F9-R**.
The method run takes approximately 3 minutes.

Required configuration

A correctly installed Outlet valve, and a correctly installed **Fraction collector F9-R** are required to run the test.

Required material

The following materials are required:

- Distilled water
 - Syringe, 25-30 ml
 - 7 tubes for collecting the fractions.
-

Prepare the test

Follow the instructions below to prepare the system before method start.

Step	Action
1	Direct outlet tubing W to a waste container.
2	Place inlet tubing A1 into distilled water.
3	Prime inlet A1 and purge System pump A. See Section 5.4.1 System pumps, on page 159 .
4	Place 7 tubes in the Fraction collector, in positions 1 to 7.
5	In the System Control module, select System:Settings . <i>Result:</i> The System Settings dialog opens.
6	In the System Settings dialog: • Select Fraction collector:Fractionation settings. • In the Drop sync field, select On. • Click OK.

Run and evaluate the test

Follow the instructions described in [Section 6.1 General performance test actions, on page 222](#) to start and run the performance test.

Evaluate the result

Check that the correct volumes have been collected in the tubes. The tubes should contain the following:

- Tube **1**: The delay volume
- Tube **2-4**: 2 ml
- Tube **5-6**: 1 ml

Also, check that the fractionation marks in the chromatogram correspond to the filled tubes and that spillages are kept to a minimum.

For further information on delay volumes and fractionation marks, see [Delay volume, on page 205](#).

Possible causes of a failed test

The table below describes possible causes of a failed test. When possible sources of error have been checked and corrected, repeat the test.

Cause	Action
Incorrect volumes collected in the tubes, and disturbances of system pressure curves: • Air trapped in System pump A • Faulty System pump A	Air in pumps: Make sure to prime inlet tubing A1 and purge System pump A before method start, see Section 5.4.1 System pumps, on page 159 . Faulty pump: See Section 8.6 Troubleshooting: Pumps, on page 384 .
Liquid collected in wrong tubes:	Make sure the fraction collector delivery arm is positioned above tube number 1 before starting the test.
Incorrect preparation of buffer and tubing	Make sure that the system was correctly prepared, see Prepare the test, on page 236 .

6.8 Sample pump tests

Sample pumps tests

The following Sample pump tests are available, for ÄKTA pure 25 and ÄKTA pure 150, respectively:

- **Sample pump S9 test**
 - **Sample pump S9H test**
-

Method description

The Sample Pump test checks the functionality of the sample pump, labeled **S9** or **S9H**.

The method run takes approximately 12 minutes.

Required configuration

The core components of ÄKTA pure and a correctly installed Sample pump are required to run the test.

Required material

The following materials are required:

- Distilled water
 - 1% Acetone and 1.00 M NaCl in distilled water
 - Syringe, 25-30 ml
 - **Ref 1** tubing, see [Reference capillary, on page 425](#).
-

Prepare the test

Follow the instructions below to prepare the system before method start.

Step	Action
1	Connect a tubing between Injection valve port column and the UV inlet, preferably the Ref 1 tubing included with the system at delivery.
2	Immerse waste tubing W, W1 and W2 in a waste container.
3	Immerse inlet tubing A1 in distilled water.
4	Immerse sample inlet tubing Buffer in 1% Acetone and 1.00 M NaCl in distilled water.
5	Prime inlet tubing A1 and sample inlet Buffer and purge the pumps. See Section 5.4.2 Sample pump, on page 165 and. No air shall be left in the pumps or tubings.

Run and evaluate the test

Follow the instructions described in [Section 6.1 General performance test actions, on page 222](#) to start, run and automatically evaluate the performance test.

Possible causes of a failed test

The table below describes possible causes of a failed test. When possible sources of error have been checked and corrected, repeat the test.

Cause	Action
The two injected peaks of liquid are not delivered as proportional peaks: - Air trapped in Sample pump - Faulty Sample pump	Air in pump: Make sure to prime inlet tubing Buffer and purge sample pump before method start, see Section 5.4.2 Sample pump, on page 165 . Faulty pump: See Section 8.6 Troubleshooting: Pumps, on page 384 .
The delivery of liquid is pulsating (unstable pump pressure)	Air in pump: Make sure to prime inlet tubing Buffer and purge sample pump before method start, see Section 5.4.2 Sample pump, on page 165 . Faulty pump: See Section 8.6 Troubleshooting: Pumps, on page 384 .
The pump pressure is too high (at a flow rate of 25 ml/min or 150 ml/min for ÄKTA pure 25 and ÄKTA pure 150, respectively)	Folded, twisted or blocked tubing: Check the tubing. The Sample pump pressure monitor is not calibrated: Calibrate the pressure monitor, see Section 7.7.2 Calibrate the pressure monitors, on page 302 . Faulty pump: See Section 8.6 Troubleshooting: Pumps, on page 384 .
Incorrect preparation of buffer and tubing	Make sure that the system was correctly prepared, see Prepare the test, on page 238 .

6.9 System Test UV U9-L (fixed)

Method description

The System test with UV monitor **U9-L** checks the functionality of the solvent delivery, the pumps, the System pump pressure sensor, UV monitor **U9-L** and the Conductivity monitor.

The method run takes approximately 35 minutes.

Required configuration

A correctly installed UV monitor **U9-L** and a correctly installed Conductivity monitor are required to run the test.

Required material

The following materials are required:

- Distilled water
 - 1% acetone and 1.00 M NaCl in distilled water
 - **Ref 1** tubing, see [Reference capillary, on page 425](#).
 - Syringe, 25-30 ml
 - Mixer, 1.4 ml
-

Prepare the test

Follow the instructions below to prepare the system before method start.

Step	Action
1	Direct outlet tubing W and W1 to a waste container.
2	Place inlet tubing A1 into distilled water.
3	Place inlet tubing B1 into a solution of 1% acetone and 1.00 M NaCl in distilled water.
4	Connect the Ref 1 tubing between Injection valve port Col and the UV monitor U9-L inlet, to generate a back pressure.
5	Make sure that the Mixer with a chamber volume of 1.4 ml is installed. For further information, see Section 7.8.3 Replace the Mixer, on page 319 .
6	Prime the buffer inlets and purge System pump A and System pump B. See Section 5.4.1 System pumps, on page 159 .


Note: If the test is performed at cold room temperature, select **Conductivity:Cond temp compensation** in the **System Settings** dialog, and set the **Compensation factor** to 2.1.

Run and evaluate the test

Follow the instructions described in [Section 6.1 General performance test actions, on page 222](#) to start, run and automatically evaluate the performance test.

Illustration of chromatogram

The illustration below shows a chromatogram from a System test with UV monitor **U9-L**.

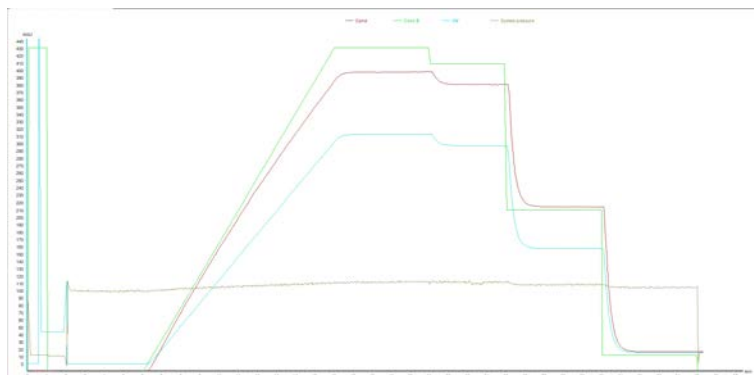

Possible causes of a failed test

The following tables describe possible causes of a failed test. When possible sources of error have been checked and corrected, repeat the test.

Faulty Gradient Test Result

Cause	Action
Disturbances caused by air trapped in any of the pumps	Make sure to prime the buffer inlets and to purge the System pumps before method start. See Section 5.4.1 System pumps, on page 159 .
Disturbances caused by damaged pump piston seals	Replace piston seals. See Chapter 7 Maintenance, on page 248 .
Unstable or incorrect UV signal, or drifting base line: Faulty UV monitor	See Section 8.3 Troubleshooting: Monitors, on page 357 .
Wrong Mixer chamber size or faulty Mixer	Replace the Mixer. See Chapter 7 Maintenance, on page 248 .

Faulty Step Response Result

Cause	Action
If all values are faulty: Air in the pump or a faulty pump	Air in pumps: Make sure to prime the buffer inlets and to purge the System pumps before method start. See Section 5.4.1 System pumps, on page 159 . Faulty pump: See Chapter 7 Maintenance, on page 248 .
Faulty values at 5%: Damaged pump piston seal in System pump B	Replace piston seals. See Chapter 7 Maintenance, on page 248 .
Faulty values at 95%: Damaged pump piston seal in System pump A	Replace piston seals. See Chapter 7 Maintenance, on page 248 .

Faulty UV Absorbance Test

Cause	Action
Incorrectly prepared acetone solution	Make sure that the acetone solution is 1% and that no solution has evaporated.
Wrong UV cell path length set in UNICORN	See, Calibration of the UV monitor U9-L flow cell length, on page 309 .

Faulty Pulsation Test

Cause	Action
Air trapped in the pumps	Make sure to prime and purge the system pumps before starting the test, see Section 5.4.1 System pumps, on page 159 .

Faulty Conductivity Test Result

Cause	Action
Faulty Conductivity monitor	See Conductivity monitor, on page 364 .
Incorrectly prepared NaCl solution	Make sure the NaCl solution is 1.00 M.
The value set for the Cond temp compensation factor is not optimal	If the test is performed at cold room temperature, open the System Settings dialog, select Conductivity:Cond temp compensation and set the Compensation factor to 2.1

Faulty UV Noise Test

Cause	Action
Air or dirt in the UV flow cell	Flush or clean the UV cell, see Section 7.5.1 Clean the UV flow cell, on page 270 .
Impure buffers	Check the buffers.

Faulty Pressure Check Test

Cause	Action
Folded, twisted or blocked tubing	Check the tubing.
The inline filter is dirty	Replace the inline filter, see Section 7.3.2 Replace the inline filter, on page 263 .
The System pressure monitor is not calibrated	Calibrate the pressure monitor, see Section 7.7.2 Calibrate the pressure monitors, on page 302 .

6.10 System Test UV U9-M (variable)

Method description

The System test with UV monitor **U9-M** checks the functionality of the solvent delivery, the pumps, the System pump pressure sensor, UV monitor **U9-M** and the Conductivity monitor.

The method run takes approximately 35 minutes.

Required configuration

A correctly installed UV monitor **U9-M** and a correctly installed Conductivity monitor are required to run the test.

Required material

The following materials are required:

- Distilled water
 - 1% acetone and 1.00 M NaCl in distilled water
 - **Ref 1** tubing, see [Reference capillary, on page 425](#).
 - Syringe, 25-30 ml
 - Mixer, 1.4 ml
-

Prepare the test

Follow the instructions below to prepare the system before method start.

Step	Action
1	Direct outlet tubing W and W1 to a waste container.
2	Place inlet tubing A1 into distilled water.
3	Place inlet tubing B1 into a solution of 1% acetone and 1.00 M NaCl in distilled water.
4	Connect the Ref 1 tubing between Injection valve port Col and the UV monitor U9-M inlet, to generate a back pressure.
5	Make sure that the Mixer with a chamber volume of 1.4 ml is installed. For further information, see Section 7.8.3 Replace the Mixer, on page 319 .
6	Prime the buffer inlets and purge System pump A and System pump B. See Section 5.4.1 System pumps, on page 159 .


Note: If the test is performed at cold room temperature, select **Conductivity:Cond temp compensation** in the **System Settings** dialog, and set the **Compensation factor** to 2.1.

Run and evaluate the test

Follow the instructions described in [Section 6.1 General performance test actions, on page 222](#) to start, run and automatically evaluate the performance test.

Illustration of chromatogram

The illustration below shows a chromatogram from a System test with UV monitor **U9-M**.

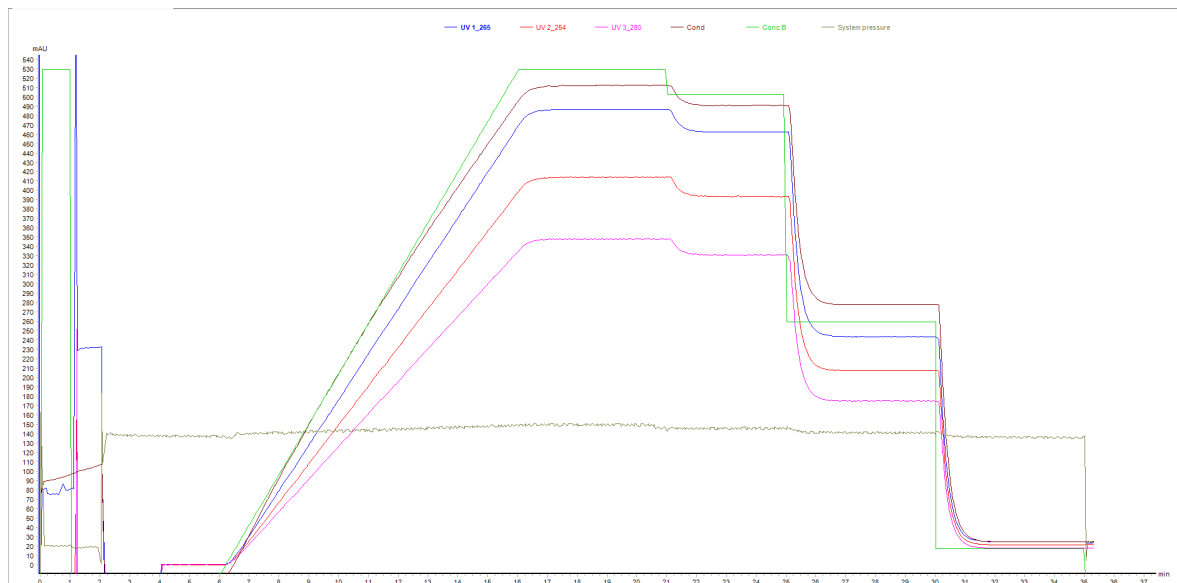

Possible causes of a failed test

The following tables describe possible causes of a failed test. When possible sources of error have been checked and corrected, repeat the test.

Faulty Gradient Test Result

Cause	Action
Disturbances caused by air trapped in any of the pumps	Make sure to prime the buffer inlets and to purge the System pumps before method start. See Section 5.4.1 System pumps, on page 159 .
Disturbances caused by damaged pump piston seals	Replace piston seals. See Chapter 7 Maintenance, on page 248 .
Unstable or incorrect UV signal, or drifting base line: Faulty UV monitor	See Section 8.3 Troubleshooting: Monitors, on page 357 .
Wrong Mixer chamber size or faulty Mixer	Replace the Mixer. See Chapter 7 Maintenance, on page 248 .

Faulty Step Response Result

Cause	Action
If all values are faulty: Air in the pump or a faulty pump	Air in pumps: Make sure to prime the buffer inlets and to purge the System pumps before method start. See Section 5.4.1 System pumps, on page 159 . Faulty pump: See Chapter 7 Maintenance, on page 248
Faulty values at 5%: Damaged pump piston seal in System pump B	Replace piston seals. See Chapter 7 Maintenance, on page 248 .
Faulty values at 95%: Damaged pump piston seal in System pump A	Replace piston seals. See Chapter 7 Maintenance, on page 248 .

Faulty UV Response Test Result

Cause	Action
Faulty UV monitor	Restart the instrument to calibrate the UV monitor. See Section 8.3 Troubleshooting: Monitors, on page 357 .

Faulty UV Absorbance Test

Cause	Action
Incorrectly prepared acetone solution	Make sure that the acetone solution is 1% and that no solution has evaporated.

Faulty Pulsation Test

Cause	Action
Air trapped in the pumps	Make sure to prime and purge the system pumps before starting the test, see Section 5.4.1 System pumps, on page 159 .

Faulty Conductivity Test Result

Cause	Action
Faulty Conductivity monitor	See Conductivity monitor, on page 364 .
Incorrectly prepared NaCl solution	Make sure that the NaCl solution is 1.00 M.
The value set for the Cond temp compensation factor is not optimal	If the test is performed at cold room temperature, open the System Settings dialog, select Conductivity:Cond temp compensation and set the Compensation factor to 2.1

Faulty UV Noise Test

Cause	Action
Air or dirt in the UV flow cell	Flush or clean the UV cell, see Section 7.5.1 Clean the UV flow cell, on page 270 .
Impure buffer	Check buffers for impurities.

Faulty Pressure Check Test

Cause	Action
Folded, twisted or blocked tubing	Check the tubing.
Dirt in inline filter	Replace the inline filter, see Section 7.3.2 Replace the inline filter, on page 263 .
System pressure monitor not calibrated	Calibrate the pressure monitor, see Section 7.7.2 Calibrate the pressure monitors, on page 302 .

7 Maintenance

About this chapter

This chapter describes the maintenance program for ÄKTA pure and provides instructions for maintenance and replacement of spare parts.

In this chapter

This chapter contains the following sections:

Section	See page
7.1 Maintenance Manager	249
7.2 Maintenance program	255
7.3 Weekly maintenance	258
7.4 Monthly maintenance	266
7.5 Semiannual maintenance	269
7.6 Maintenance when required	273
7.7 Calibration procedures	299
7.8 Replacement procedures	313


7.1 Maintenance Manager

Introduction

Maintenance Manager allows the user to display general information about the system and its modules, and also operational statistics of the modules. Notifications for maintenance actions of the system and its modules are predefined. The user can add automated maintenance notifications for the system. Maintenance notifications are based on calendar periods of system use, and for some systems also on operational statistics for the modules.


Open Maintenance Manager

In the **System Control** module, on the **System** menu, click **Maintenance Manager** to open the **Maintenance Manager** dialog.

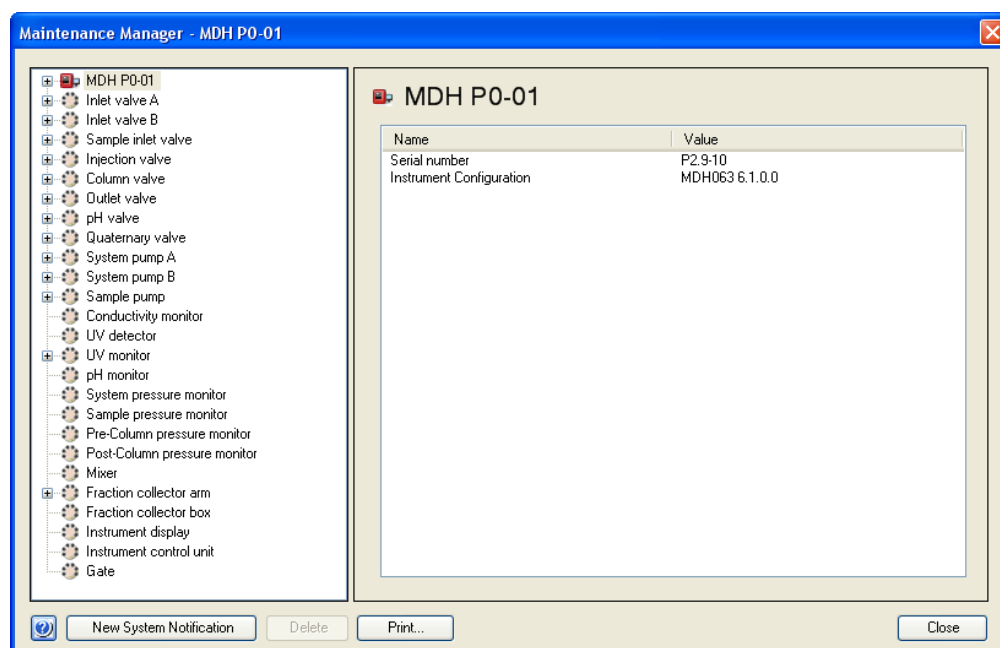


View general information and statistics

In the left pane of the **Maintenance Manager** dialog, select the system of interest to view general information of the selected system. For some systems it is possible to view information for a module of interest. When modules are selected, operational statistics are also displayed.

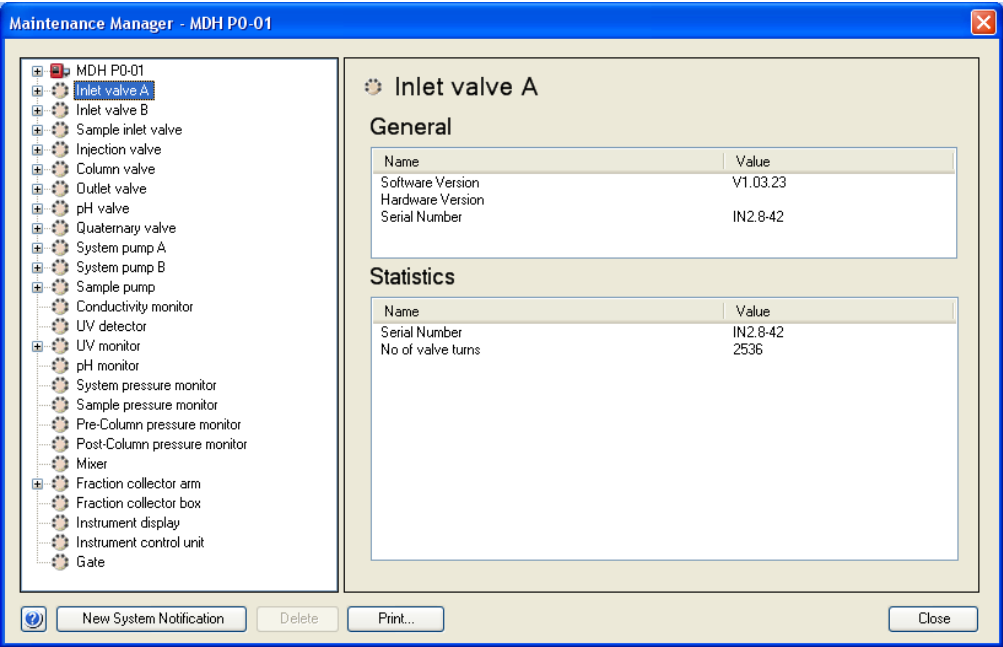

View maintenance notifications

Click the plus symbol (+) of the system of interest to expand the list of related maintenance notifications. For some systems it is possible to view maintenance notifications for a module of interest. Select a notification to view notification details.

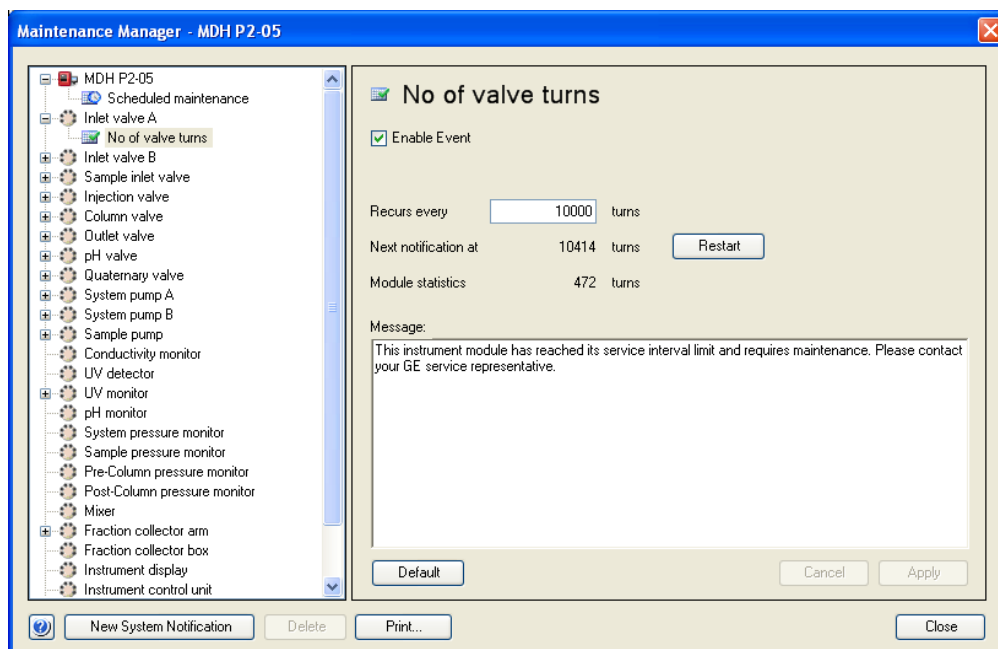


Note: Modules with no plus symbol (+) have no related maintenance notifications.

Edit a maintenance notification

Follow the instruction to edit a maintenance notification.

Step	Action
1	In the left pane of the Maintenance Manager dialog, select a maintenance notification. <i>Result:</i> Details of the selected maintenance notification are displayed in the dialog.

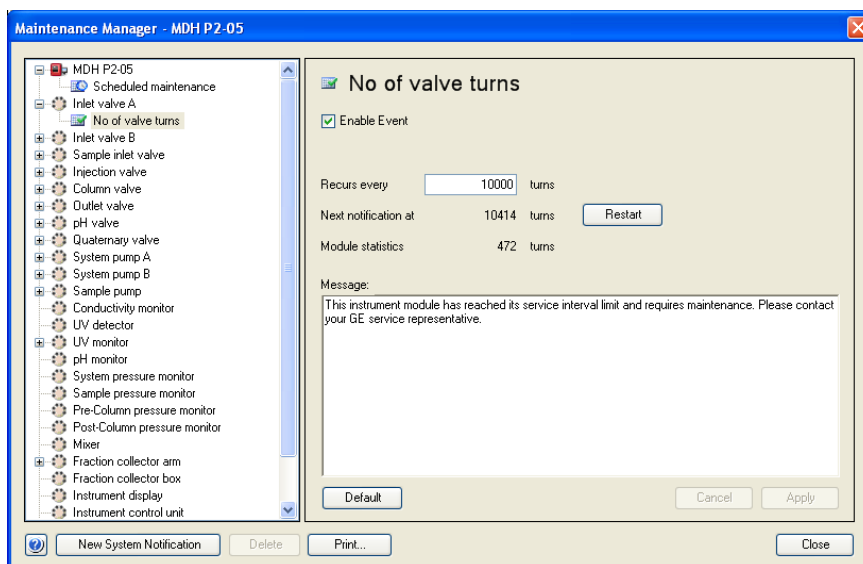

- | | |
|---|---|
| 2 | <p>Edit the maintenance notification as desired:</p> <ul style="list-style-type: none"> • Select the Enable Event checkbox to activate the notification. If the box is unchecked, the notification will not be issued. • Enter a new interval after which the new notification will be issued. • Click Restart to reset the counter and add a complete interval before the next notification. • Edit the message that will be shown in the maintenance notification. • Click Default to restore the default settings for maintenance notifications. |
| 3 | Click Apply to save the changes. |


Add a new system notification

The user can add new system notifications to the list of system events.

Follow the instructions to add a new system notification.

Step	Action
------	--------

- | | |
|---|---|
| 1 | In the Maintenance Manager dialog, click New System Notification .
<i>Result:</i> The NewNotification field appears in the Maintenance Manager dialog. |
|---|---|

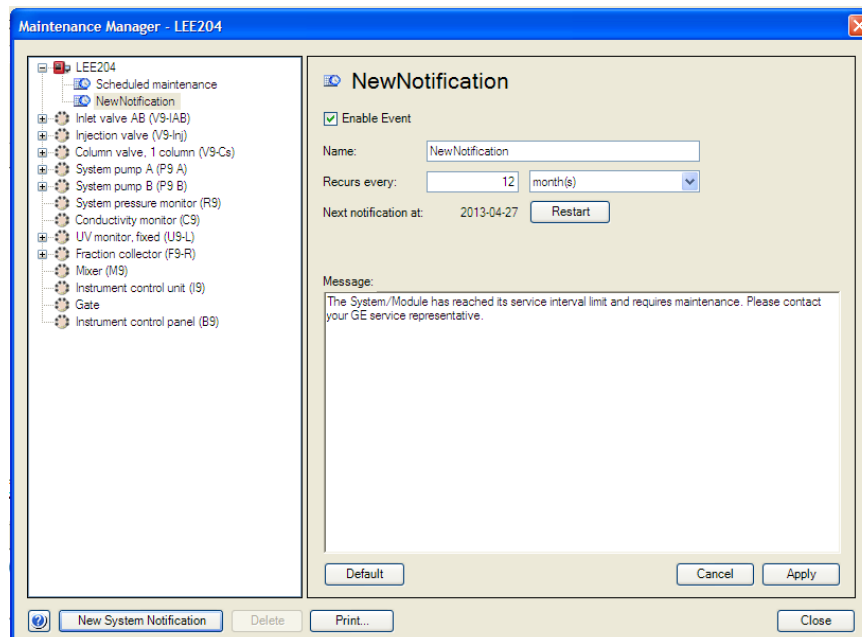

- | | |
|---|--|
| 2 | In the NewNotification field: <ul style="list-style-type: none"> • Enter a name for the new notification. • Select a time interval after which the new notification will be issued. • If desired, write a message that will be shown for the maintenance notification. |
| 3 | Click Apply to save the changes and apply the notification settings. |

Delete a user defined system notification


To delete a user defined system notification, select the notification in the **Maintenance Manager** dialog and press the **Delete** button.

Note: Module notifications are predefined and cannot be deleted. If desired, they can be disabled.


Handle a maintenance notification

Each maintenance notification has a time interval after which the notification is issued. When this time interval has been reached, a **Maintenance Notification** dialog appears.

Note: The possibility to add maintenance notifications for modules is only available for some systems, but all systems can add maintenance notifications for the complete system.

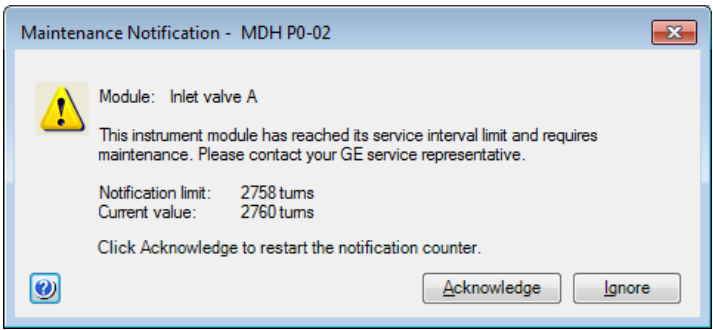

Follow the instruction to handle the notification.

Click...	to...
	reset the counter for a new maintenance notification period. Note: <i>Make sure that the maintenance action is performed as instructed after the notification is acknowledged, otherwise the system performance may deteriorate.</i>
	close the dialog without action. Note: <i>The Maintenance Notification will be displayed each time the System Control module is opened until the notification is acknowledged.</i>

Note: The predefined maintenance notification periods use average values. The actual service interval for a specific module may be shorter or longer.

7.2 Maintenance program

Introduction

This section lists the periodic maintenance activities that should be performed by the user of ÄKTA pure, as well as maintenance activities that should be performed when required.

Maintenance is divided into:

- Daily maintenance
- Weekly maintenance
- Monthly maintenance
- Semiannual maintenance
- Maintenance when required



WARNING

Hazardous biological agents during run. When using hazardous biological agents, run **System CIP** and **Column CIP** to flush the entire system tubing with bacteriostatic solution (e.g., NaOH) followed by a neutral buffer and finally distilled water, before service and maintenance.



CAUTION

Hazardous chemicals during run. When using hazardous chemicals, run **System CIP** and **Column CIP** to flush the entire system tubing with distilled water, before service and maintenance.



CAUTION

Always use appropriate personal protective equipment during operation and maintenance of ÄKTA pure.

Periodic maintenance program

The following periodic maintenance should be performed by the user of ÄKTA pure.

Interval	Maintenance action	See section
Daily	Calibrate the pH monitor	Section 7.7.1 Calibrate the pH monitor, on page 300
Weekly	Calibrate pressure monitors	Section 7.7.2 Calibrate the pressure monitors, on page 302

Interval	Maintenance action	See section
Weekly	Change pump rinsing solution	Section 7.3.1 Change pump rinsing solution, on page 259
Weekly	Clean fraction collector diodes	Section 7.3.3 Clean the Fraction collector F9-C sensors, on page 264
Monthly	Check the Flow restrictor	Check flow restrictor
Semiannually	Clean the UV flow cell	Section 7.5.1 Clean the UV flow cell, on page 270
Semiannually	Replace pH electrode	Section 7.5.2 Replace the pH electrode, on page 272

Maintenance when required

The following maintenance should be performed by the user of ÄKTA pure when required.

Maintenance action	See section
Clean the instrument externally	Section 7.6.1 Clean the instrument externally, on page 274
Perform System CIP	Section 7.6.2 Perform System CIP, on page 275
Perform Column CIP	Section 7.6.3 Perform Column CIP, on page 281
Clean Fraction collector F9-C	Section 7.6.4 Clean Fraction collector F9-C, on page 285
Clean Fraction collector F9-R	Section 7.6.5 Clean Fraction collector F9-R, on page 287
Replace tubing and connectors	Section 7.8.1 Replace tubing and connectors, on page 314
Storage of pH electrode	Section 7.6.6 Storage of the pH electrode, on page 288
Clean the pH electrode	Section 7.6.7 Clean the pH electrode, on page 290
Clean the Conductivity flow cell	Section 7.6.10 Clean the Conductivity flow cell, on page 297
Calibrate the Conductivity monitor	Section 7.7.3 Calibrate the Conductivity monitor, on page 305
Calibrate the UV monitor	Section 7.7.4 Calibrate the UV monitors, on page 309
Replace Mixer	Section 7.8.3 Replace the Mixer, on page 319
Replace inline filter	Section 7.3.2 Replace the inline filter, on page 263
Replace O-ring in Mixer	Section 7.8.4 Replace the O-ring inside the Mixer, on page 320

Maintenance action	See section
Replace UV flow cell	Section 7.8.5 Replace the UV monitor U9-M flow cell, on page 322 and Section 7.8.6 Replace the UV monitor U9-L flow cell, on page 325
Replace the Flow restrictor	Section 7.8.7 Replace Flow restrictor, on page 327
Replace inlet filters	Section 7.8.8 Replace the inlet filters, on page 328
Wipe off excess oil from the pump head	Section 7.6.9 Wipe off excess oil from the pump head, on page 296
Clean the check valves	Section 7.6.8 Clean the pump head check valves, on page 293
Replace check valves	Section 7.8.9 Replace the pump head check valves, on page 329
Replace pump piston seals, pump P9 and P9H	Section 7.8.10 Replace pump piston seals of Pump P9 or P9H, on page 332
Replace pump piston seals, pump P9-S	Section 7.8.11 Replace pump piston seals of Pump P9-S, on page 341
Replace pump pistons	Section 7.8.12 Replace pump pistons, on page 348
Replace pump rinsing system tubing	Section 7.8.13 Replace pump rinsing system tubing, on page 349

7.3 Weekly maintenance

Introduction

This section provides instructions for weekly maintenance activities.

In this section

This section contains the following subsections:

Section	See page
7.3.1 Change pump rinsing solution	259
7.3.2 Replace the inline filter	263
7.3.3 Clean the Fraction collector F9-C sensors	264

7.3.1 Change pump rinsing solution

Maintenance interval

Replace the pump rinsing solution in the system pumps and the sample pump (optional module) every week to prevent bacterial growth.


Required material

The following material are required:

- 20% ethanol
- Syringe, 25-30 ml

Illustration of the system pump piston rinsing system

The illustrations below show the parts and tubing of the system pump piston rinsing system

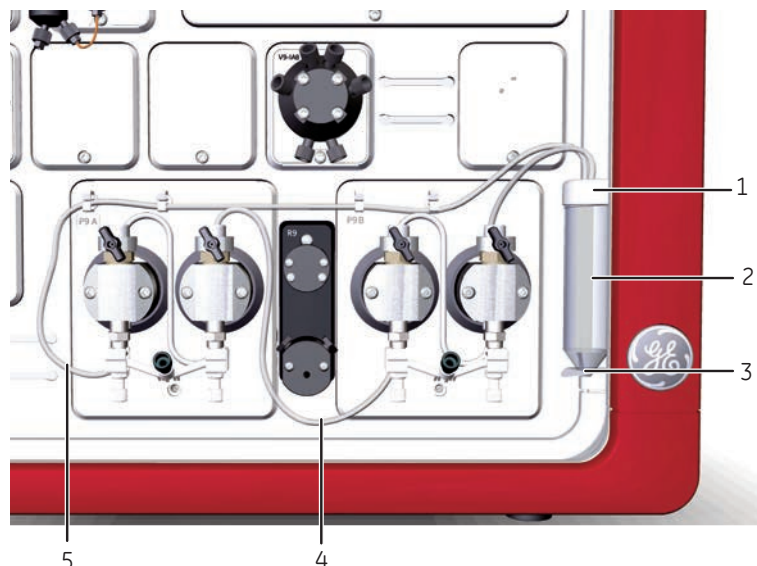


Part	Description
1	Rinsing system tube holder, top
2	Rinsing system tube
3	Rinsing system tube holder, bottom
4	Outlet tubing
5	Inlet tubing

Prime the system pump piston rinsing system

Follow the instructions below to fill the pump piston rinsing system with rinsing solution. See the tubing configuration of the rinsing system in the illustration above.

Step	Action
1	Remove the rinsing system tube from the holder.
2	Fill the rinsing system tube with 50 ml of 20% ethanol.
3	Place the rinsing solution tube back in the holder.
4	Insert the inlet tubing to the System pump piston rinsing system into the fluid in the rinsing solution tube.
Note: <i>Make sure that the inlet tubing reaches close to the bottom of the rinsing solution tube.</i>	
5	Connect a 25 to 30 ml syringe to the outlet tubing of the System pump piston rinsing system. Draw liquid slowly into the syringe.
6	Disconnect the syringe and discard its contents.
7	Insert the outlet tubing into the fluid in the rinsing solution tube.
8	Fill the rinsing solution tube so that the tube contains 50 ml of 20% ethanol.

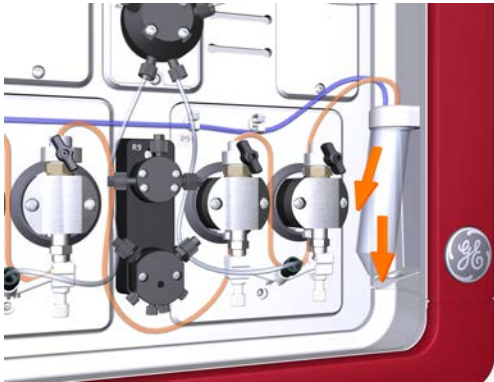


Note:

Make sure that the inlet tubing reaches close to the bottom of the rinsing solution tube.




Illustrations of the sample pump piston rinsing system

The illustrations below show the parts, tubing and flow path of the sample pump piston rinsing system.

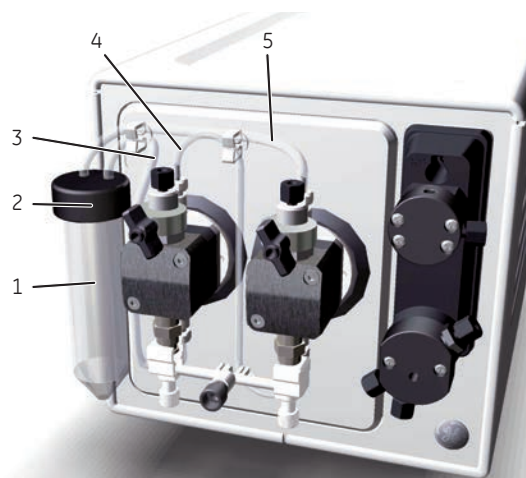

Parts and tubing



Rinsing system flow path


Part	Function
1	Pump rinsing liquid tube
2	Pump rinsing liquid tube holder
3	Inlet tubing, from the rinsing liquid tube to the left pump head (lower rinsing system connection) .
4	Tubing between the left pump head (upper rinsing system connection) and the right pump head (lower rinsing system connection).
5	Outlet tubing, from the right pump head (upper rinsing system connection) to the rinsing liquid tube.

Prime the sample pump piston rinsing system

Follow the instructions below to fill the pump piston rinsing system with rinsing solution. For the tubing configuration of the rinsing system, see the illustration above.

Step	Action
------	--------

- | | |
|---|---|
| 1 | Unscrew and remove the rinsing liquid tube from the holder. |
|---|---|

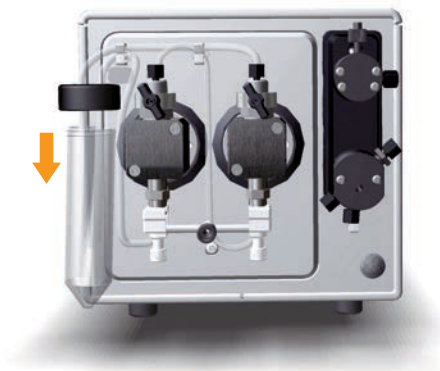


- | | |
|---|---|
| 2 | Fill the rinsing liquid tube with 50 ml of 20% ethanol. |
| 3 | Put the rinsing liquid tube back in the holder and fasten it by screwing it into place. |
| 4 | Insert the inlet tubing to the piston rinsing system into the fluid in the rinsing liquid tube. |

Note:

Make sure that the inlet tubing reaches close to the bottom of the rinsing liquid tube.

- | | |
|---|---|
| 5 | Connect a 25 to 30 ml syringe to the outlet tubing of the System pump piston rinsing system. Draw liquid slowly into the syringe. |
|---|---|

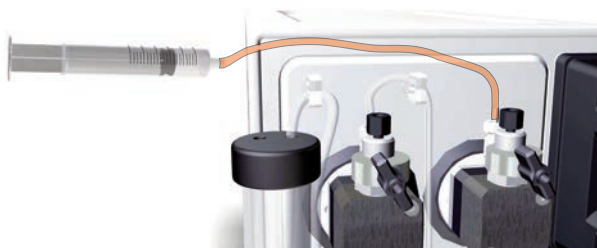

Note:

The outlet tubing is colored orange for clarity in the above illustration.

- | | |
|---|--|
| 6 | Disconnect the syringe and discard its contents. |
| 7 | Insert the outlet tubing into the fluid in the rinsing liquid tube. |
| 8 | Fill the rinsing liquid tube so that the tube contains 50 ml of 20% ethanol. |

7.3.2 Replace the inline filter

Maintenance interval

Replace the inline filter that is located in the top section of the Mixer every week, or when required, for example when the filter becomes clogged.

Required material

The following materials are required:

- Online filter kit
- Forceps
- Gloves

Instruction

Follow the instructions below to replace the inline filter that is located in the top of the Mixer.

Tip: Use forceps and gloves during the replacement procedure to avoid contaminating the Mixer components.

Step	Action
1	Unscrew the top section of the Mixer.
2	Remove the old filter using forceps. Replace the support net if this is damaged. Fit the new filter.
	
3	Check the O-ring of the Mixer. If the O-ring is damaged, replace it according to Section 7.8.4 Replace the O-ring inside the Mixer, on page 320 .
4	While holding the Mixer upright, screw the top section back onto the Mixer.

7.3.3 Clean the Fraction collector F9-C sensors

Maintenance interval

Clean the fraction collector sensors every week, or when required, for example if the fraction collector fails to read the tray ID or do not collect fractions correctly.

Required material


The following material is required:

- Wash bottle
- Water or 20% ethanol
- Cloth


Instructions

Follow the instructions below to clean the fraction collector diodes. See [Section 3.2.2 Fraction collector F9-C illustrations, on page 92](#) for the locations of the components of the fraction collector.

Step	Action
1	In System Control , select Manual:Execute Manual Instructions:Fraction collection:Frac cleaning position . Click Execute .

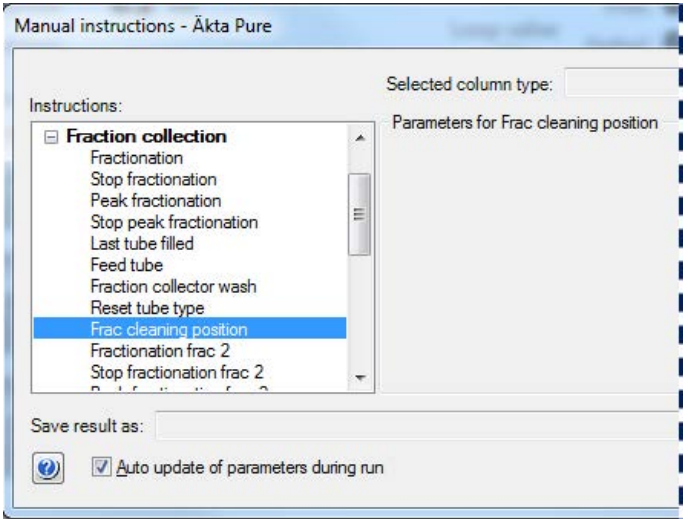

Result: The Dispenser head moves to cleaning position, and the Instrument display states **System pause**.

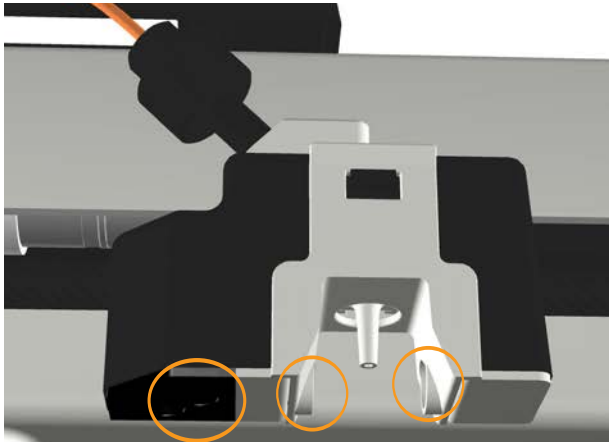Step	Action
2	Wipe off the Dispenser head and the Drop sync and Type code reader sensor windows using a wash bottle with water or 20% ethanol and a cloth. 
3	Let the Dispenser head dry completely before starting a run.
4	Close the fraction collector door. <i>Result:</i> Automatic scanning is performed.
5	In the System Control module, press the End icon in the toolbar.  <i>Result:</i> The Dispenser head moves to home position, and the Instrument display states Ready.

7.4 Monthly maintenance

Introduction

This section provides instructions for monthly maintenance actions.

Maintenance interval

Check the back pressure for the Flow restrictor every month.

Location of the Flow restrictor

The recommended positions for Flow restrictor **FR-902** are:

- Connected between the Conductivity monitor **C9** and the Outlet valve.
or
 - Connected to the **ToR** and **FrR** ports of the pH valve.
-

Check Flow restrictor connected to Conductivity monitor and Outlet valve

Follow the instructions below to check the back pressure of Flow restrictor **FR-902**, when this is connected between the Conductivity monitor and the Outlet valve.

Step	Action
1	Immerse the piece of inlet tubing marked A1 in distilled water, and insert the piece of tubing from Outlet valve port W into a waste container.
2	In the System Control module, select Manual:Execute Manual Instructions . <i>Result:</i> The Manual instructions dialog opens.
3	In the Manual instructions dialog: • Select Flowpath:Injection valve, and select Manual Load. Click Insert. • Select Flowpath:Column valve, and select By-pass. Click Insert. • Select Flowpath:Outlet valve, and select Out-Waste. Click Insert. • Select Pumps:System flow and set the Flow rate to 2.5 ml/min. Click Insert. • Click Execute. <i>Result:</i> A system flow of 2.5 ml/min starts.
4	Note the PreC pressure displayed in the Run Data pane. Tip: <i>If PreC pressure is not displayed, click the Customize icon. In the Customize dialog, under the Run Data Groups tab, select PreC pressure.</i>

Step	Action
5	Click on the Pause icon to stop the flow.
6	Replace the Flow restrictor with a female/female union connector. Tip: <i>The female/female union connector is included in the accessory kit.</i>
7	Click the Continue icon to restart the flow.
8	Note the PreC pressure displayed in the Run Data pane.
9	Calculate the difference between the two pressure values.
10	Check that the pressure difference is within the range 0.2 ± 0.05 MPa. If this is not the case, the Flow restrictor should be replaced, see Section 7.8.7 Replace Flow restrictor, on page 327 .

Check Flow restrictor connected to pH valve

Follow the instructions below to check the back pressure of Flow restrictor **FR-902**.

Step	Action
1	Immerse the piece of inlet tubing marked A1 in distilled water, and insert the piece of tubing from Outlet valve port W into a waste container.
2	In the System Control module, select Manual:Execute Manual Instructions . <i>Result:</i> The Manual instructions dialog opens.
3	In the Manual instructions dialog: • Select Flowpath:Injection valve, and then select Manual Load. Click Insert. • Select Flowpath:Column valve, and then select By-pass. Click Insert. • Select Flowpath:pH valve, and set the pH electrode to Off-line and the Restrictor to In-line. Click Insert. • Select Flowpath:Outlet valve, and then select Out-Waste. Click Insert. • Select Pumps:System flow and set the Flow rate to 2.5 ml/min. Click Insert. • Click Execute. <i>Result:</i> A system flow of 2.5 ml/min starts.
4	Note the PreC pressure displayed in the Run Data pane. Tip: <i>If PreC pressure is not displayed, click the Customize icon. In the Customize dialog, under the Run Data Groups tab, select PreC pressure.</i>

Step	Action
5	In the Manual instructions dialog: • Select Flowpath:pH valve, and set the pH electrode to Off-line and the Restrictor to Off-line. • Click Execute.
6	Note the PreC pressure displayed in the Run Data pane.
7	Calculate the difference between the two pressure values noted in step 4 and step 6.
8	Check that the pressure difference is within the range 0.2 ± 0.05 MPa. If this is not the case, the Flow restrictor should be replaced, see Section 7.8.7 Replace Flow restrictor, on page 327 .

7.5 Semiannual maintenance

Introduction

This section provides instructions for semiannual maintenance activities.

In this section

This section contains the following subsections:

Section	See page
7.5.1 Clean the UV flow cell	270
7.5.2 Replace the pH electrode	272

7.5.1 Clean the UV flow cell

Maintenance interval

Clean the UV flow cell every six months, or when required.



NOTICE

Keep UV flow cell clean. Do not allow solutions containing dissolved salts, proteins or other solid solutes to dry out in the flow cell. Do not allow particles to enter the flow cell, as damage to the flow cell may occur.

Required material

The following materials are required:

- Luer connector
- Waste container
- Syringe, 25-30 ml
- 10% surfactant detergent solution (e.g., Decon™ 90, Deconex 11, or RBS 25)
- Distilled water

Instruction

Follow the instructions below to clean the UV flow cell for UV monitor **U9-M** or UV monitor **U9-L**. The UV flow cell can be mounted or not mounted on the instrument during the cleaning procedure.

The illustrations in the instructions below show UV monitor **U9-M**. UV monitor **U9-L** is cleaned in a corresponding way.

Step	Action
------	--------

- | | |
|---|--|
| 1 | Disconnect the tubing from the top of the UV flow cell, and replace the fingertight connector with a Luer connector. |
|---|--|



- | | |
|---|---|
| 2 | Disconnect the tubing from the bottom of the UV flow cell, and connect a piece of waste tubing to the UV flow cell. Insert the waste tubing into a waste container. |
|---|---|

Step	Action
3	Fill a syringe with distilled water, and connect the syringe to the Luer connector.
	
4	Squirt the distilled water through the UV flow cell in small amounts. Disconnect the syringe.
5	Fill a syringe with a 10% surfactant detergent solution, such as Decon 90, Deconex 11, RBS 25 or equivalent, and connect the syringe to the Luer connector.
	Tip: <i>Heat the 10% surfactant detergent solution to 40°C to increase the cleaning effect.</i>
6	Squirt the detergent solution through the UV flow cell about five times.
7	Leave the detergent solution in the flow cell for at least 20 minutes.
8	Inject the detergent solution remaining in the syringe into the flow cell. Disconnect the syringe.
9	Fill a syringe with distilled water. Connect the syringe to the Luer connector.
10	Inject the distilled water into the UV flow cell to rinse the flow cell. Disconnect the syringe.
11	Disconnect the Luer connector from the top of the UV flow cell. Reconnect the piece of tubing from the Column valve to the top of the UV flow cell.
12	Disconnect the waste tubing from the bottom of the UV flow cell. Reconnect the piece of tubing from the Conductivity monitor to the bottom of the UV flow cell.

7.5.2 Replace the pH electrode

Maintenance interval

Replace the pH electrode every six months, or when required.

Required material

The following materials are required:

- pH electrode
- Deionized water
- Standard buffer pH 4

Instruction



CAUTION

pH-electrode. Handle the pH-electrode with care. The glass tip may break and cause injury.

Follow the instructions below to replace the pH electrode.

Step	Action
1	Disconnect the pH electrode cable of the used pH electrode from the connection on the front of the pH valve.
2	Unscrew the nut of the pH electrode by hand, and pull the used electrode away.
3	Unpack the new pH electrode. Remove the cover from the tip of the new pH electrode. Make sure that the electrode is not broken or dry.
4	Prior to first use of the electrode, immerse the glass bulb in deionized water for 30 minutes and then in a standard buffer, pH 4, for 30 minutes.
5	Carefully insert the new pH electrode into the pH flow cell. Tighten the nut by hand to secure the electrode.
6	Connect the pH electrode cable of the new electrode to the connection on the front of the pH valve.
7	Calibrate the new pH electrode, see Section 7.7.1 Calibrate the pH monitor, on page 300 .

7.6 Maintenance when required

Introduction

This section gives instructions for maintenance activities to be performed when required.

In this section

This section contains the following subsections:

Section	See page
7.6.1 Clean the instrument externally	274
7.6.2 Perform System CIP	275
7.6.3 Perform Column CIP	281
7.6.4 Clean Fraction collector F9-C	285
7.6.5 Clean Fraction collector F9-R	287
7.6.6 Storage of the pH electrode	288
7.6.7 Clean the pH electrode	290
7.6.8 Clean the pump head check valves	293
7.6.9 Wipe off excess oil from the pump head	296
7.6.10 Clean the Conductivity flow cell	297

7.6.1 Clean the instrument externally

Maintenance interval

Clean the the instrument externally when required. Do not allow spilled liquid to dry on the instrument.

Required material

The following materials are required:

- Cloth
 - Mild cleaning agent or 20% ethanol
-

Instruction

Follow the instructions below to clean the instrument externally.

Step	Action
1	Check that no run is in progress.
2	Switch off the instrument.
3	Wipe the surface with a damp cloth. Wipe off stains using a mild cleaning agent or 20% ethanol. Wipe off any excess.
4	Let the instrument dry completely before using it.

7.6.2 Perform System CIP

Maintenance interval

Perform a System cleaning in place (System CIP) when required, for example between runs where different samples and buffers are used. This is important to prevent cross-contamination and bacterial growth in the instrument.

Required material

The following materials are required:

- Appropriate cleaning solutions (e.g., NaOH, buffer solution or distilled water).
- Syringe, 25-30 ml

Introduction

The **System CIP** method is used to fill the instrument and the selected inlets and outlets with cleaning solution.



WARNING

Hazardous biological agents during run. When using hazardous biological agents, run **System CIP** and **Column CIP** to flush the entire system tubing with bacteriostatic solution (e.g., NaOH) followed by a neutral buffer and finally distilled water, before service and maintenance.



CAUTION

Hazardous substances. When using hazardous chemical and biological agents, take all suitable protective measures, such as wearing protective glasses and gloves resistant to the substances used. Follow local and/or national regulations for safe operation, maintenance and decommissioning of the equipment.



CAUTION

Explosion hazard if flammable liquid leaks during cleaning of the flow path. When cleaning the flow path of Fraction collector F9-C with a flammable liquid like ethanol, carefully inspect the flow path, including the waste tubing, to make sure there will be no leakage.

Tip: *If hazardous chemicals are used for system or column cleaning, wash the system or columns with a neutral solution in the last phase or step.*

Create a System CIP method

Follow the instruction below to create a **System CIP** method.

Step	Action
------	--------

- | | |
|---|---|
| 1 | In the Method Editor module,
<ul style="list-style-type: none"> click the New Method icon |
|---|---|




or

- select **File:New Method**.

Result: The **New Method** dialog opens.

- | | |
|---|--|
| 2 | In the New Method dialog, select System and then System CIP in the Predefined Method drop-down list. Click OK . |
|---|--|

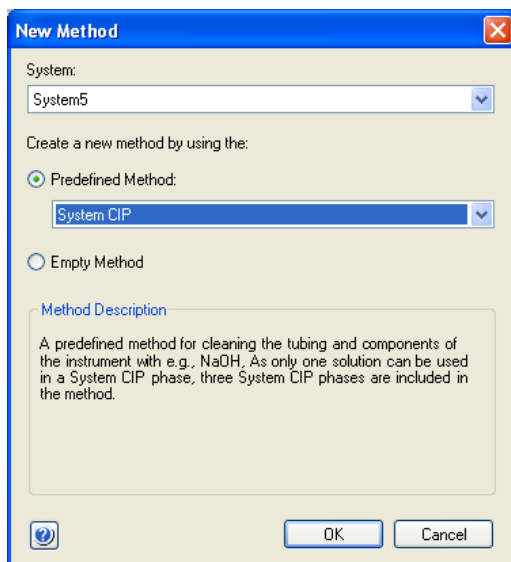

Result: One **Method Settings** phase and three **System CIP** phases show in the **Method Outline** pane. Each **System CIP** phase uses one cleaning solution.



- | | |
|---|--|
| 3 | If desired, add additional System CIP phases to the method using the Phase Library . |
|---|--|

Step	Action
------	--------

4	In the Phase Properties tab of each of the System CIP phases:
---	---

- Enter a note for the first solution (optional).
- Select values for **Flow rate**, **Volume per position** and **Incubation time**.

System CIP

This phase uses one solution

Solution note

☐ Pause to manually move all inlets to the selected solution

Flow rate ml/min [0.000 - 25.000]

Volume per position ml

Incubation time min

- Define the extent of cleaning by checking the check boxes.

Note:

For complete cleaning of the Injection valve, select at least one of the sample inlets and clean the manual injection port using a syringe (see [Clean the manual injection port of the Injection valve, on page 279](#)).

A inlets	B inlets	Sample inlets	Column Position	Outlets
☒ A1	☐ B1	☐ Buffer	☒ By-pass	☒ Waste
☐ A2	☐ B2	☐ S1	☐ 1	☐ Outlet 1
☐ A3	☐ B3	☐ S2	☐ 2	☐ Outlet 2
☐ A4	☐ B4	☐ S3	☐ 3	☐ Outlet 3
☐ A5	☐ B5	☐ S4	☐ 4	☐ Outlet 4
☐ A6	☐ B6	☐ S5	☐ 5	☐ Outlet 5
☐ A7	☐ B7	☐ S6		☐ Outlet 6
		☐ S7		☐ Outlet 7
				☐ Outlet 8
				☐ Outlet 9
				☐ Outlet 10 / Frac 2
☐ All	☐ All	☐ All	☐ All	☐ All

Others

☐ System pump sample flow path

☐ Injection valve with capillary loop

Loop cleaning volume ml


Number of loops

☐ Fraction collector

☐ Second fraction collector

Note:

- The pH electrode and the pH valve are not included in the system CIP. Refer to [Section 7.6.7 Clean the pH electrode, on page 290](#) for instructions on how to clean the pH electrode.
- If the fraction collector is included, a lower flow rate might need to be set in the instruction **Fraction collector wash settings**.
- Make sure not to exceed the pressure limits for any of the modules that are part of the flow path during the CIP.

Step	Action
5	In the Method Editor module, - click the Save the method icon  or - select File:Save As <i>Result:</i> The Save As dialog opens.
6	In the Save As dialog: - Select a target folder to enable the Save button. - Type a Name for the method. - Select a System from the list. - Click . <i>Result:</i> The created method is saved in the selected folder.

Perform a System CIP

Follow the instructions below to run a **System CIP** method.

Step	Action
1	In the Method Editor module, create a System CIP method according to the instructions above.
2	Connect bypass tubing to all selected column positions and loop positions if a loop valve is used.
3	Prepare cleaning solutions and immerse the selected inlet tubing in the solutions. Note: <i>Note that each phase uses one solution. All inlets selected in one phase should be immersed in the same cleaning solution.</i>
4	In the System Control module, select the created method and start the run.
5	For complete cleaning of the flow path, clean the manual injection port of the Injection valve and the pH valve manually, see the instructions below.

Clean the manual injection port of the Injection valve

Follow the instructions below to manually clean the Manual load position of the Injection valve.

- | Step | Action |
|------|--|
| 1 | In the System Control module, select Manual:Execute Manual Instructions .
<i>Result:</i> The Manual instructions dialog opens. |
| 2 | In the Manual instructions dialog, select Flowpath:Injection valve , and select Manual Load . Click Execute . |
| 3 | Connect a suitable sample loop to Injection valve ports LoopF (fill) and LoopE (empty). |

Note:

Do not use a Superloop when cleaning the Injection valve.



- | | |
|---|---|
| 4 | Connect tubing to Injection valve port W1 , and direct this tubing to a waste container. |
| 6 | Fill a syringe with approximately 10 ml of an appropriate cleaning solution (e.g., NaOH or buffer solution). Connect the syringe to Injection valve port Syr , and inject the cleaning solution. |




- | | |
|---|---|
| 6 | Fill a syringe with distilled water. Connect the syringe to Injection valve port Syr , and inject the distilled water. |
|---|---|

Clean the pH valve


Follow the instructions below to clean the pH valve. The calibration function is used to switch the valve position. However, no calibration is performed.

Step	Action
------	--------

- | | |
|---|---|
| 1 | Connect tubing to pH valve port W3 , and direct the other end of this tubing to a waste container. |
| 2 | Unscrew the pH electrode from the pH valve, and replace it with the dummy electrode. |
| 3 | Open the System Control module and select System:Calibrate .
<i>Result:</i> The Calibration dialog opens. |

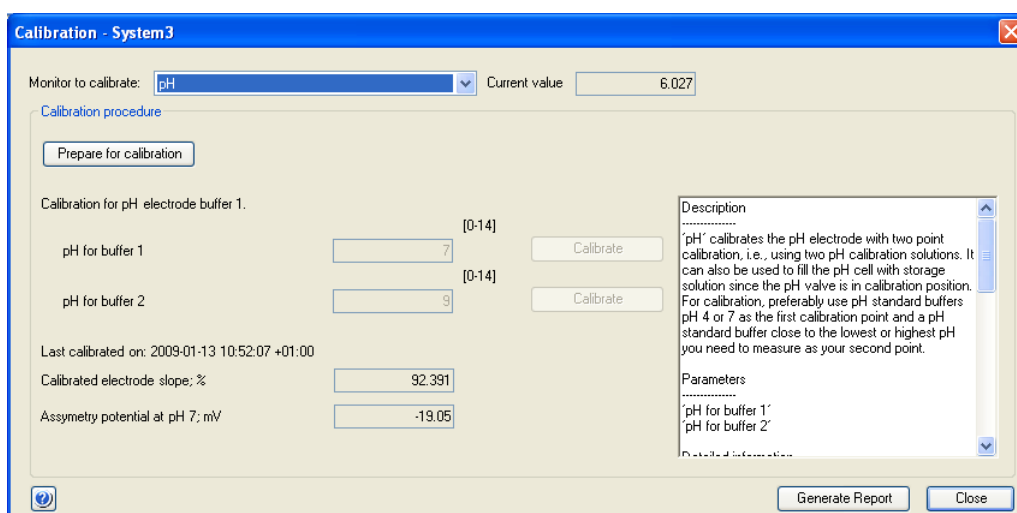


- | | |
|---|---|
| 4 | In the Calibration dialog, select pH from the Monitor to calibrate drop-down list. |
| 5 | Press the Prepare for calibration button. |



Result: The pH valve switches to the calibration position.

- | | |
|---|---|
| 7 | Fill a syringe with approximately 10 ml of 1 M NaOH. Connect the syringe to the pH valve port Cal , and inject the solution. |
| 8 | Fill a syringe with distilled water. Connect the syringe to the pH valve port Cal , and inject the distilled water. |
| 9 | Press the Close button. |



Result: The pH valve switches back to the default position and the **Calibration** dialog closes. No calibration is performed.

7.6.3 Perform Column CIP

Maintenance interval

Perform a Column cleaning in place (Column CIP) when required, for example between runs where different samples are used.

Required material

The following materials are required:

- Appropriate cleaning solutions. Please refer to the instructions for use of the column.
-

Introduction

The **Column CIP** method is used to clean the column after purification runs, to remove non-specifically bound proteins and to minimize the risk for carry-over between different purification runs.



WARNING

Hazardous biological agents during run. When using hazardous biological agents, run **System CIP** and **Column CIP** to flush the entire system tubing with bacteriostatic solution (e.g., NaOH) followed by a neutral buffer and finally distilled water, before service and maintenance.



CAUTION

Hazardous substances. When using hazardous chemical and biological agents, take all suitable protective measures, such as wearing protective glasses and gloves resistant to the substances used. Follow local and/or national regulations for safe operation, maintenance and decommissioning of the equipment.

Tip: *If hazardous chemicals are used for system or column cleaning, wash the system or columns with a neutral solution in the last phase or step.*

Create a Column CIP method

Follow the instruction below to create a **Column CIP** method.

Step	Action
------	--------

- | | |
|---|---|
| 1 | In the Method Editor module,
<ul style="list-style-type: none"> click the New Method icon |
|---|---|




or

- select **File:New Method**.

Result: The **New Method** dialog opens.

- | | |
|---|---|
| 2 | In the New Method dialog, select System and then Predefined Method and Column CIP . Click OK . |
|---|---|

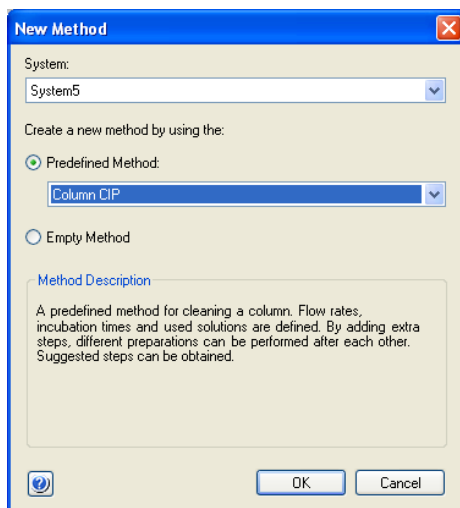

Result: One **Method Settings** phase and one **Column CIP** phase will be displayed in the **Method Outline** pane.

- | | |
|---|--|
| 3 | In the Phase Properties tab of the Method Settings phase, select Column type and Column position . |
|---|--|

Step Action

4 In the **Phase Properties** tab of the **Column CIP** phase:

- Click **Add Step** to add a step.
- Select the step and click **Remove Step** to remove a step.
- To enter a value, select the cell and enter or select a new value.

Column CIP

	CIP solution note	Inlet A	Inlet B	%B (0-100)	Linear gradient	Fill System	Volume (CV)	Flow Rate (0-25) ml/min	Flow direction	Outlet	Incubation time (min)
1		A1	B1	0.00	☐	☒	1.00	1.000	Down flow	Out-Waste	0.00

5 In the **Phase Properties** tab of the **Column CIP** phase, click the **Get Suggested Steps** button to get a suggested procedure for the selected column type. Note that this function is not available for all column types.

Result: Suggested cleaning steps for the selected column type are displayed.

	CIP solution note	Inlet A	Inlet B	%B (0-100)	Linear gradient	Fill System	Volume (CV)	Flow Rate (0-25) ml/min	Flow direction	Outlet	Incubation time (min)
1	2M NaCl	A1	B1	0.00	☐	☒	2.00	2.500	Down flow	Out-Waste	0.00
2	1M NaOH	A1	B1	0.00	☐	☒	4.00	2.500	Down flow	Out-Waste	0.00
3	2M NaCl	A1	B1	0.00	☐	☒	2.00	2.500	Down flow	Out-Waste	0.00
4	Water	A1	B1	0.00	☐	☒	2.00	2.500	Down flow	Out-Waste	0.00
5	Equilibration/storage ...	A1	B1	0.00	☐	☒	4.00	2.500	Down flow	Out-Waste	0.00

6 If several cleaning solutions are used, change settings for **Inlet A** and/or **Inlet B**. Select one inlet for each solution. If Inlet B is used, remember to edit the values in the **%B** column.

	CIP solution note	Inlet A	Inlet B	%B (0-100)	Linear gradient	Fill System	Volume (CV)	Flow Rate (0-25) ml/min	Flow direction	Outlet	Incubation time (min)
1	2M NaCl	A1	B1	0.00	☐	☒	2.00	2.500	Down flow	Out-Waste	0.00
2	1M NaOH	A2	B1	0.00	☐	☒	4.00	2.500	Down flow	Out-Waste	0.00
3	2M NaCl	A1	B1	0.00	☐	☒	2.00	2.500	Down flow	Out-Waste	0.00
4	Water	A3	B1	0.00	☐	☒	2.00	2.500	Down flow	Out-Waste	0.00
5	Equilibration/storage ...	A4	B1	0.00	☐	☒	4.00	2.500	Down flow	Out-Waste	0.00

Step	Action
7	In the Method Editor module, - click the Save the method icon  or - select File:Save As <i>Result:</i> The Save As dialog opens.
8	In the Save As dialog: - Select a target folder to enable the Save button. - Type a Name for the method. - Select a System from the list. - Click the Save button. <i>Result:</i> The created method is saved in the selected folder.

Perform a Column CIP

Follow the instructions below to run a **Column CIP** method.

Step	Action
1	In the Method Editor module, create a Column CIP method according to the instruction above.
2	Prepare cleaning solutions and immerse the selected inlets in the solutions.
3	Connect the column to the selected column position.
4	In the System Control module, select the created method and start the run.

7.6.4 Clean Fraction collector F9-C

Maintenance interval

Clean the Fraction collector when required, for example if liquid has been spilled in the Fraction collector chamber. The internal tubing of the fraction collector may need to be replaced for maintenance or for process purposes. Information on how and when to replace the internal tubing can be found in [Section 7.8.2 Replace internal tubing in Fraction collector F9-C, on page 316](#)

Required material

The following materials are required:

- Wash bottle
- Water or 20% ethanol
- Cloth

Instruction

Follow the instruction below to clean the interior of the Fraction collector. The locations of the components of the fraction collector are shown in [Section 3.2.2 Fraction collector F9-C illustrations, on page 92](#).

Step	Action
1	Perform a fraction collector wash: In System Control, select Manual:Execute Manual Instructions:Fraction collection:Fraction collector wash. Click Execute.  NOTICE • If no column valve is used, make sure to replace any columns in the flow path with tubing before a fraction collector wash is performed. • Lower the flow for the fraction collector wash in the instruction Fraction collector wash settings if the system back pressure is elevated during the wash. • Make sure not to exceed the pressure limits for any of the modules that are part of the flow path.
2	In System Control, select Manual:Execute Manual Instructions:Fraction collection:Fraction cleaning position. Click Execute. Result: The Dispenser head moves to cleaning position, and the Instrument display states System pause.
3	Open the door of the fraction collector and remove the rack

7 Maintenance

7.6 Maintenance when required

7.6.4 Clean Fraction collector F9-C

Step	Action
4	Wash the Cassette tray or rack and the Cassettes (if applicable), with water and a mild cleaning agent.
5	Lift off the Waste funnel and wash it with water and a mild cleaning agent. Refit the Waste funnel.
6	Wipe off the interior of the fraction collector using a damp cloth. Wipe off stains using a mild cleaning agent or 20% ethanol.
7	Wipe off the Dispenser head and its diode windows (the Drop sync sensor and the Type code reader) using a wash bottle with water or 20% ethanol and a cloth.
8	Let the fraction collector dry completely before starting a run.
9	Close the door of the fraction collector. <i>Result:</i> Automatic scanning is performed.
10	In the System Control module, press the End icon in the toolbar. <i>Result:</i> The Dispenser head moves to home position.

7.6.5 Clean Fraction collector F9-R

Maintenance interval

Clean the Fraction collector when required, for example in case of liquid spill.

Required material

The following materials are required:

- Water or 20% ethanol
 - Cloth
-

Clean the instrument

Follow the instructions below to clean the instrument externally.

Step	Action
1	Check that no run is in progress.
2	Switch off the instrument.
3	Wipe the surface with a damp cloth. Wipe off stains using a mild cleaning agent or 20% ethanol. Wipe off any excess.
4	Let the Fraction collector F9-R dry completely before restart.

Clean drop sync sensor

Clean the drop sensor photocell located above the tube sensor (see [Front view illustration, on page 103](#)) with a damp cloth.

7.6.6 Storage of the pH electrode

Maintenance interval

When pH monitoring is not used, the pH electrode can be stored in storage solution inside the pH flow cell. If pH monitoring is not used for a week or longer, inject new storage solution into the pH flow cell or replace the pH electrode with the dummy electrode that was installed in the pH valve on delivery.

Required material

The following materials are required:


- Syringe, 25 to 30 ml
- Storage solution (1:1 mixture of standard buffer, pH 4, and 1 M KNO₃)

Instruction

Follow the instructions below to fill the pH flow cell with storage solution. The calibration function is used to switch the position of the pH valve. However, no calibration is performed.

Step	Action
------	--------

- | | |
|---|---|
| 1 | In the System Control module, on the System menu click Calibrate .
Result: The Calibration dialog opens. |
|---|---|

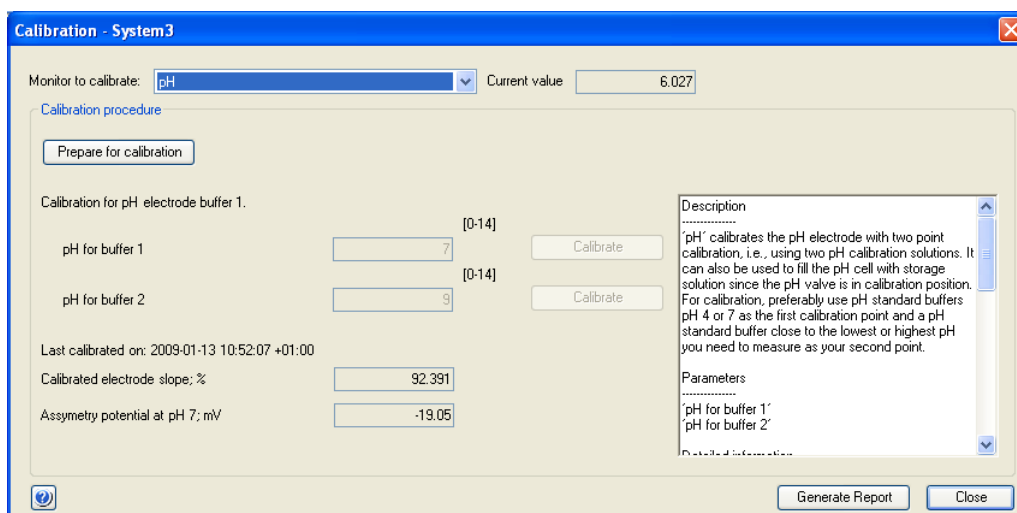

- | | |
|---|---|
| 2 | In the Calibration dialog, click pH on the Monitor to calibrate drop-down list. |
| 3 | Click Prepare for Calculation .
Result: The pH valve switches to the calibration position. |
| 4 | Prepare at least 10 ml storage solution by mixing equal volumes of a standard buffer, pH 4, and a 1 M Potassium Nitrate (KNO ₃) solution. |

Step	Action
5	Fill a syringe with approximately 10 ml of the storage solution. Connect the syringe to the pH valve port Cal, and inject the storage solution.  The diagram illustrates a syringe with a clear barrel and a grey plunger, connected via an orange tube to a black port on a circular valve assembly. The valve assembly is mounted on a white rectangular base. A black cable is also connected to the top of the valve assembly. Below the valve, another black component is connected via an orange tube.
6	Click Close. <i>Result:</i> The pH valve switches back to the default position and the Calibration dialog closes. No calibration is performed.

7.6.7 Clean the pH electrode

Maintenance interval

Clean the pH electrode when required. The pH electrode can be cleaned either when it is installed in the pH valve or when it has been removed. The pH electrode has a limited longevity and should be replaced every six months or when the response time is slow, see [Section 7.5.2 Replace the pH electrode, on page 272](#). After cleaning has been performed, re-calibrate the pH monitor, see [Section 7.7.1 Calibrate the pH monitor, on page 300](#).

Required material

The following materials are required:

- Syringe, 25-30 ml
 - Distilled water
 - 0.1 M HCl and 0.1 M NaOH
or
 - Liquid detergent
or
 - 1% pepsin solution in 0.1 M HCl
or
 - 1 M KNO₃
-

Cleaning agents

Clean the pH electrode using one of the following procedures:

Salt deposits

Dissolve the deposits by immersing the electrode for a five minute period in each of the following solutions:

- 0.1 M HCl
- 0.1 M NaOH
- 0.1 M HCl

Rinse the electrode tip in distilled water between each solution.

Oil or grease films

Wash the electrode tip in liquid detergent and water. If the films are known to be soluble in a particular organic solvent, wash with this solvent. Rinse the electrode tip in distilled water.

Protein deposits

Dissolve the deposit by immersing the electrode in a solution of 1% pepsin in 0.1 M HCl for five minutes, followed by thorough rinsing with distilled water.

If these procedures fail to rejuvenate the electrode, try the following procedure.

Note: This procedure can be performed only when the pH electrode is not installed in the pH valve.

Step	Action
------	--------

- | | |
|---|--|
| 1 | Heat a 1 M KNO ₃ solution to 60°C–80°C. |
| 2 | Place the electrode tip in the heated KNO ₃ solution. |
| 3 | Allow the electrode to cool while immersed in the KNO ₃ solution before re-testing. |


If these steps fail to improve the electrode, replace the electrode, see [Section 7.5.2 Replace the pH electrode, on page 272](#).

Clean a pH electrode installed in the pH valve


Follow the instructions below to clean a pH electrode installed in the pH valve. The calibration function is used to switch the position of the pH valve. However, no calibration is performed.

Step	Action
------	--------

- | | |
|---|---|
| 1 | Open the System Control module and select System:Calibrate .
<i>Result:</i> The Calibration dialog opens. |
|---|---|

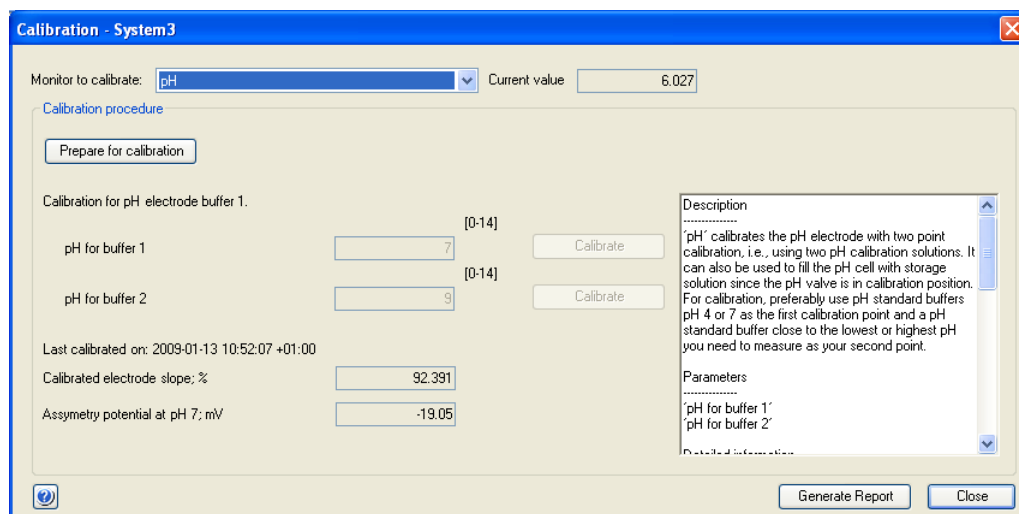

- | | |
|---|---|
| 2 | Set Monitor to calibrate by selecting pH from the list. |
| 3 | Press the Prepare for calibration button. |



Result: The pH valve switches to the calibration position.

7 Maintenance


7.6 Maintenance when required

7.6.7 Clean the pH electrode

Step	Action
4	Fill a syringe with approximately 10 ml of chosen cleaning solution. Connect the syringe to the pH valve port Cal . Inject the liquid and wait for 5 minutes. Disconnect the syringe.



- | | |
|---|---|
| 5 | If several cleaning solutions are to be used, repeat step 4 with distilled water and then with the next solution. |
| 6 | As the last step in the cleaning procedure: <ul style="list-style-type: none">• Fill a syringe with distilled water.• Connect the syringe to the pH valve port Cal.• Inject the water.• Disconnect the syringe. |
| 7 | Press the Close button. |



Result: The pH valve switches back to the default position and the **Calibration** dialog closes. No calibration is performed.

7.6.8 Clean the pump head check valves

Maintenance interval

Clean the check valves when required, for example if solids in the check valve cause irregular or low flow. The cleaning procedure is the same for the system pumps and the sample pump.

Required material


The following materials are required:

- Adjustable wrench
- Methanol
- Distilled water
- Ultrasonic bath

Instruction

Follow the instructions below to remove and clean the pump head check valves.

Step	Action
1	Switch off the instrument.
2	Disconnect the tubing from the pump head and disconnect the pump inlet tubing. Disconnect the tubing of the pump rinsing system.
3	Unscrew the purge valve by turning it counter-clockwise, and lift off the metal ring.

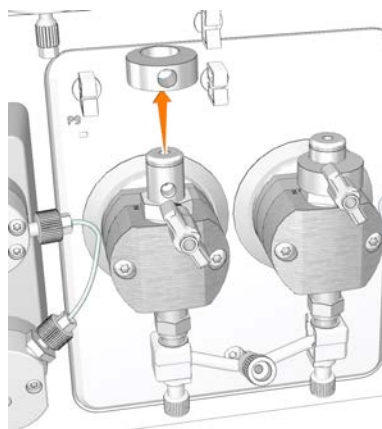


7 Maintenance


7.6 Maintenance when required

7.6.8 Clean the pump head check valves


Step	Action
4	Unscrew the plastic nut of the upper check valve using an adjustable wrench, and gently lift off the upper check valve.

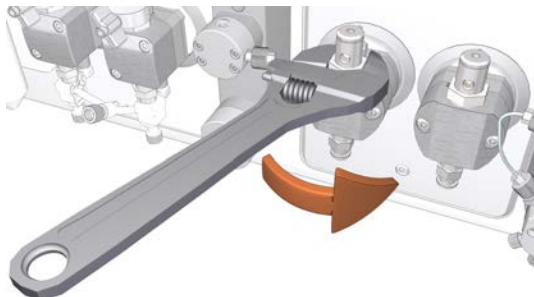

5	Unscrew the two white plastic screws located below each pump head. Pull the plastic connectors to the sides to release the inlet manifold.
---	--

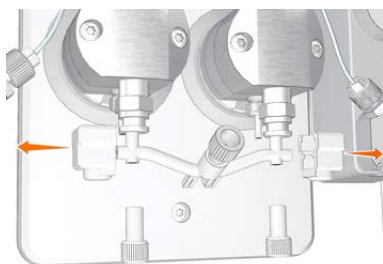

6	Unscrew the lower check valve using an adjustable wrench.
---	---

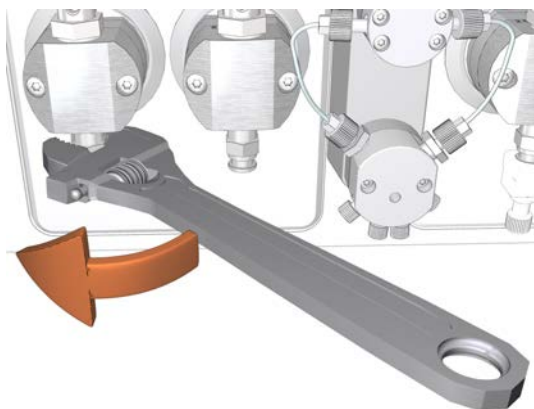

Step	Action
7	CAUTION Hazardous substances. When using hazardous chemical and biological agents, take all suitable protective measures, such as wearing protective glasses and gloves resistant to the substances used. Follow local and/or national regulations for safe operation, maintenance and decommissioning of the equipment. Immerse the valves completely in methanol and place them in an ultrasonic bath for a few minutes. Repeat the ultrasonic bath with deionized water.
8	Refit the check valves.
9	Tighten the nut until fully finger-tight and then use the adjustable wrench to tighten a further 90 degrees.
10	Refit the inlet manifold and reconnect the tubing to the pump head.

7.6.9 Wipe off excess oil from the pump head

Maintenance interval

During the first months of use it is normal that excess oil leaks out of the drain hole below the System pump. The function of the pump is not in any way affected by this.

Required material

The following materials are required:

- Cloth
 - Mild cleaning agent or 20% ethanol
-

Instruction

Follow the instructions below to clean the System pumps externally.

Step	Action
1	Check that no run is in progress.
2	Switch off the instrument.
3	Wipe off the excess oil from the pump head with a damp cloth. Wipe off stains using a mild cleaning agent or 20% ethanol.
4	Let the pump dry completely before using the instrument.

7.6.10 Clean the Conductivity flow cell

Maintenance interval

Clean the Conductivity flow cell when required.


Required material

The following materials are required:

- Luer connector
- Waste container
- Syringe, 25-30 ml
- 1 M NaOH
- Distilled water

Instruction

Follow the instruction below to clean the flow cell of the Conductivity monitor.

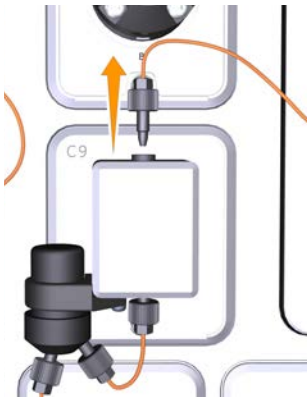Step	Action
1	Disconnect the fingertight connector and the piece of tubing from the top of the Conductivity monitor, and attach a Luer connector. 
2	Disconnect the piece of tubing from the bottom of the Conductivity monitor, and connect a piece of waste tubing to the Conductivity monitor. Place the waste tubing in a waste container.

7 Maintenance

7.6 Maintenance when required

7.6.10 Clean the Conductivity flow cell

Step	Action
3	Fill a syringe with distilled water, and connect the syringe to the Luer connector.
	
4	Squirt distilled water through the Conductivity flow cell in small amounts. Disconnect the syringe.
5	Fill a syringe with 1 M NaOH, and connect the syringe to the Luer connector.
6	Squirt 1 M NaOH through the Conductivity flow cell about five times.
7	Leave the liquid in the flow cell for at least 15 minutes.
8	Fill a syringe with distilled water. Connect the syringe to the Luer connector.
9	Inject the distilled water into the Conductivity flow cell to rinse the flow cell. Disconnect the syringe.
10	Disconnect the Luer connector from the top of the Conductivity flow cell, and reconnect the fingertight connector with tubing.

7.7 Calibration procedures

Introduction

This section provides instructions for calibration procedures that can be performed using the **System Control** module in UNICORN software.

In this section

This section contains the following subsections:

Section	See page
7.7.1 Calibrate the pH monitor	300
7.7.2 Calibrate the pressure monitors	302
7.7.3 Calibrate the Conductivity monitor	305
7.7.4 Calibrate the UV monitors	309

Menu command in UNICORN

Open the **System Control** module and select **System:Calibrate** to open the **Calibration** dialog.

7.7.1 Calibrate the pH monitor

Maintenance interval

Calibrate the pH monitor once a day, when the pH electrode has been replaced, or if the ambient temperature has changed by more than $\pm 5^{\circ}\text{C}$.

Required material

Use two pH calibration buffers with a difference of at least one pH unit. Preferably use a pH standard buffer, pH 4 or pH 7, as the first calibration point, and a pH standard buffer close to the lowest or highest pH you need to measure as your second point. Allow the buffers to equilibrate to ambient temperature before use.


Instruction



CAUTION

pH-electrode. Handle the pH-electrode with care. The glass tip may break and cause injury.

Follow the instructions below to calibrate the pH monitor.

Step	Action
1	In the Calibration dialog, select pH from the Monitor to calibrate drop-down list.
2	Click the Prepare for calibration button.  <i>Result:</i> The pH valve switches to the calibration position.
3	Enter the pH of the first pH standard buffer in the pH for buffer 1 field.

Step	Action
4	Fill a syringe with approximately 10 ml of the first pH standard buffer. Connect the syringe to the Luer connector of pH valve port Cal , and inject the buffer.



5	When the Current value is stable, click the Calibrate button.
---	---



6	Wash the pH flow cell by injecting water into pH valve port Cal using a new syringe.
---	---


7	Enter the pH of the second pH standard buffer in the pH for buffer 2 field.
---	--

8	Repeat steps 4-6 using the second pH standard buffer.
---	---

Result: The calibration date and time are displayed in the dialog, along with values for **Calibrated electrode slope** and **Asymmetry potential at pH 7**.

9	Is the Calibrated electrode slope $\geq 80\%$ and the Asymmetry potential at pH 7 inside the interval ± 60 mV?
---	--

- If Yes: Click the **Close** button to switch the pH valve back to the default position and to close the **Calibration** dialog.



- If No: Clean the pH electrode and repeat the calibration procedure. If this does not help, replace the electrode.

7.7.2 Calibrate the pressure monitors

Maintenance interval

ÄKTA pure can have up to four pressure monitors: System pump pressure monitor, Sample pump pressure monitor, Pre-column pressure monitor and Post-column pressure monitor. Check the pressure monitors every week, or when the ambient temperature has changed by more than $\pm 5^{\circ}\text{C}$. Calibrate the monitor if the zero pressure reading is outside the range $\pm 0.02\text{ MPa}$.

Check the monitors

Follow the instructions below to check the pressure monitors. The procedure is the same for each monitor.

Step	Action
1	Disconnect the relevant tubing from the pressure monitor to obtain zero-pressure, see table Tubing and pressures, on page 303 .
2	Click the Customize icon to open the Customize dialog. In the Customize dialog, under the Run Data Groups tab, select the relevant pressure to display, see table Tubing and pressures, on page 303 . Click OK to close the Customize dialog.
3	In the Run Data pane in the System Control module, check what pressure is displayed.
4	If the zero pressure reading is outside the range $\pm 0.02\text{ MPa}$, calibrate the pressure monitor according to the instruction below.


Calibrate the monitors

Follow the instructions below to calibrate any of the pressure monitors.

Step	Action
1	Disconnect the relevant tubing from the pressure monitor, see table Tubing and pressures, on page 303 .
2	In the Calibration dialog, select the pressure monitor to calibrate from the Monitor to calibrate drop-down list.
3	Click the Reset pressure button. <i>Result:</i> The atmospheric pressure is defined as zero. The date and time of the most recent calibration, and the current pressure value are displayed.
4	Reconnect the tubing to the pressure monitor.

Tubing and pressures

The table below shows the tubing to disconnect when checking and calibrating the pressure monitors. The UNICORN names of the pressures measured by the monitors are also shown.

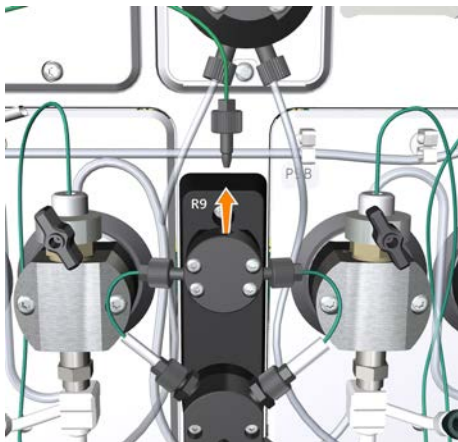Pressure monitor	Tubing to disconnect	Pressure in UNICORN
System pump pressure monitor	Tubing from the System pump pressure monitor 	System pressure
Sample pump pressure monitor	Tubing from the Sample pump pressure monitor 	Sample pressure
Pre-column pressure monitor	Tubing to Column valve V9-C or V9H-C port In 	PreC pressure

Pressure monitor	Tubing to disconnect	Pressure in UNICORN
Post-column pressure monitor	Tubing to Column valve V9-C or V9H-C port Out 	PostC pressure

7.7.3 Calibrate the Conductivity monitor

Introduction

Two types of calibrations can be performed:

- **Conductivity monitor - factory calibration:** Restores the conductivity cell constant to the factory default value.
- **Conductivity monitor - user calibration:** Calibrates the conductivity cell constant.

Maintenance interval

Recommended maintenance intervals for the two types of calibrations:

- **Conductivity monitor - factory calibration:** Perform calibration to override an incorrect user calibration.
- **Conductivity monitor - user calibration:** The conductivity cell is factory calibrated, and should not require recalibration under normal usage. Perform calibration when the signal is unstable or you suspect that it is incorrect. It is also recommended to recalibrate the Conductivity monitor after cleaning.

Conductivity monitor - factory calibration

Follow the instruction below to restore the conductivity cell constant to the factory default value.

Step	Action
1	In the Calibration dialog, select Conductivity monitor - factory calibration from the Monitor to calibrate drop-down list. <i>Result:</i> The time for the new calibration and the current value are displayed.
2	Click Restore . <i>Result:</i> The conductivity cell constant is restored to the factory default value. The conductivity cell constant is written on the packaging of the Conductivity monitor.


Conductivity monitor - user calibration

Follow the instruction below to calibrate the Conductivity flow cell constant.


Step	Action
1	Make sure that the instrument has been switched on for at least one hour.
2	In the System Control module, select System:Settings . <i>Result:</i> The System Settings dialog opens.

Step	Action
------	--------

- | | |
|---|--|
| 3 | In the System Settings dialog, select Conductivity and Cond temp compensation . Set the Compensation factor to 0%, and click OK . |
|---|--|

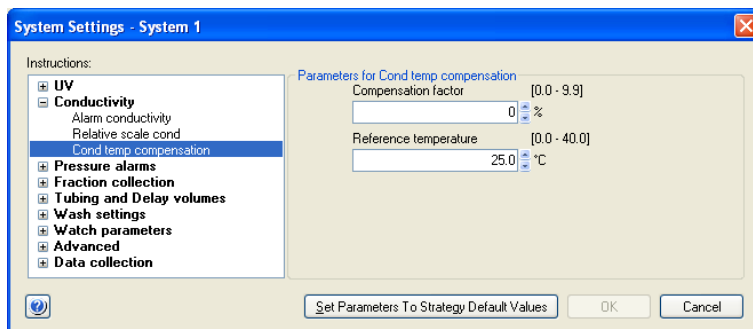

- | | |
|---|--|
| 4 | Wash the whole flow path and fill it with deionized water using a suitable inlet and the System pump, until the conductivity value reaches 0.00 mS/cm. |
| 5 | Connect the tubing (labelled 3) from the system pump pressure monitor directly to the conductivity cell inlet, by-passing the Mixer, Injection valve, Column valve and UV-monitor, see image below. Ensure that the Flow restrictor is inline. |

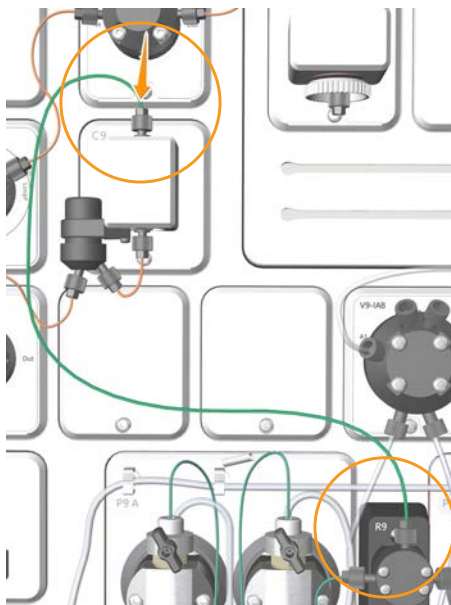


- | | |
|---|--|
| 6 | Prime and purge the inlet used in step 4 with the 1.00 M NaCl calibration solution. Fill the conductivity cell with the calibration solution at 1 ml/min. Pump in at least 15 ml of the calibration solution and wait until the conductivity signal and the temperature have stabilized before continuing the calibration. See Section 5.4.1 System pumps, on page 159 . |
| 7 | Under continuous flow, read the current Conductivity temperature from Run Data with an accuracy of one decimal place. |
| 8 | In the Calibration dialog, select Conductivity monitor - user calibration from the Monitor to calibrate drop-down list. |

Step	Action
9	In the Run Data pane of System Control, read the current Cond temp. Tip: <i>If Cond temp is not showing, click the Customize icon. In the Customize dialog, under the Run Data Groups tab, select to view Cond temp.</i>
10	In the Calibration dialog, enter the theoretical conductivity value at the current conductivity temperature in the Enter theoretical conductivity value input field. • If a certified conductivity standard solution is used, use the supplied theoretical conductivity value. • If a manually prepared 1.00 M NaCl calibration solution is used, see the graph for conductivity value at the current temperature on page 308.
11	In the Calibration dialog, click Calibrate. Result: The new conductivity cell constant is displayed in the Conductivity cell 1 constant/cm box. The new constant should normally be $40 \pm 10 \text{ cm}^{-1}$. The date and time for the calibration are also displayed.
12	In the System Control toolbar, click the End icon to end the run.
13	In the System Settings dialog, select Conductivity:Cond temp compensation and set the Compensation factor back to desired value, default 2.0%. Click OK. Note: <i>When using NaCl, the optimal compensation factor is 2.1%.</i>

Graph for conductivity value

The graph below shows the conductivity value at the current temperature when 1.00 M NaCl calibration solution is used.

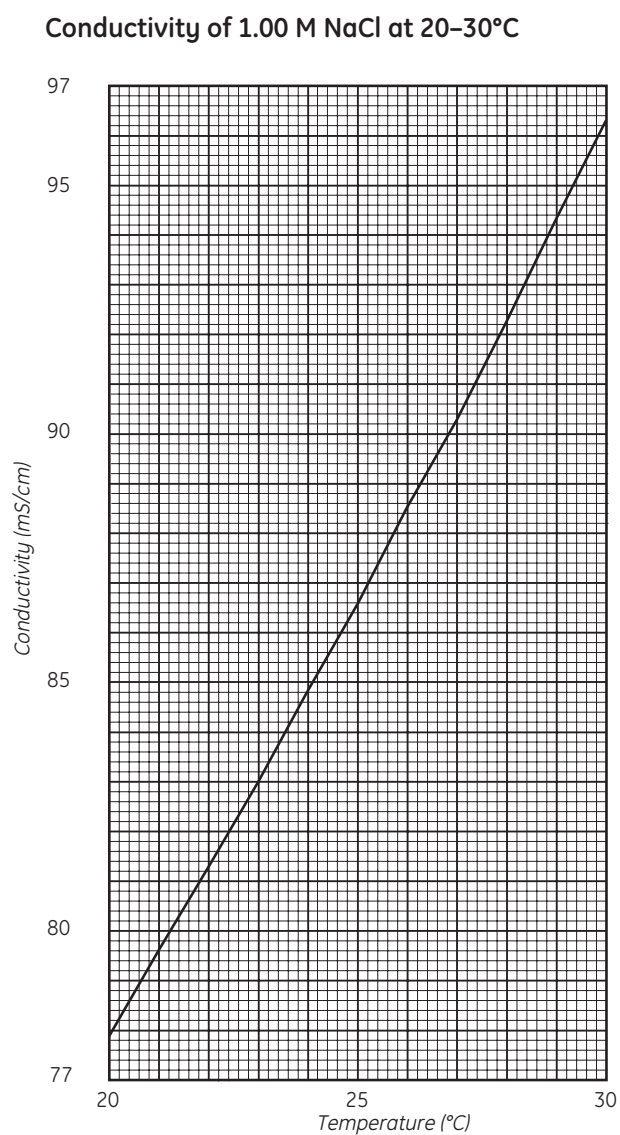

7.7.4 Calibrate the UV monitors

Automatic calibration of the UV monitor U9-M

The wavelength is automatically calibrated every time the instrument is switched on. If the instrument has been switched on for a couple of days, and the ambient temperature and/or the humidity has changed, restart the instrument using the power switch to calibrate the UV monitor.

Calibration of the UV monitor U9-L flow cell length

The path length in the UV flow cell or the UV 2nd flow cell might differ from the nominal length, which leads to incorrect results in the calculation of protein concentration in the eluate. To achieve normalized absorbance, the path length in the UV flow cell or the UV 2nd flow cell must be calibrated. The calibration procedure that is described below is the same for both UV flow cell and the UV 2nd flow cell, unless otherwise stated.

Note: *The flow cell path length must be registered or updated in UNICORN, when the flow cell is replaced.*

Equipment needed

To perform the calibration, a calibration kit containing test solutions, syringes and accessories is needed. A specified kit is available for each cell length.

If using a UV flow cell with the theoretical path length...	Then use calibration kit...
2 mm	UV-900 2 mm calibration kit (Product Code 18-6324-02)
5 mm	UV-900 5 mm calibration kit (Product Code 18-6324-04)

To calculate the real path length of the UV flow cell, use the following software:

- UV-900 cell calibration Excel-file (Product Code 18-6324-06)

Prepare for calibration

Follow the instructions below to prepare for the calibration of the UV monitor U9-L.


Step	Action
1	Ensure that the flow restrictor is inline in the flow path after the UV flow cell.
2	Mount the union Luer female/1/16" male, included in the test kit, in the upper inlet of the UV flow cell.
3	Open the software UV-900 cell calibration Excel-file.

Step	Action
4	The solution bottles are labelled with the concentration value and the reference absorbance value for each solution. Enter the concentrations of the solutions in ascending order into the column UV Test kit Concentration (mg/l) . Enter the corresponding absorbance values into the column UV Test kit Absorbance (AU/cm) .

Perform the calibration

Follow the instructions below to calibrate UV monitor U9-L and UV monitor U9-L, 2nd.

Step	Action
1	In the System Control module, select Manual:Execute Manual Instructions. In the Manual Instructions dialog: • Select Pumps:System flow and set the Flow rate to 0.0 ml/min. • Click Execute. <i>Result:</i> The absorbance can now be monitored.
2	Fill one of the supplied syringes with 1.5-2 ml of the first solution (0 mg/l). Ensure that there are no air bubbles in the syringe.
3	Fit the syringe in the union Luer connector and inject the solution. DO NOT remove the syringe.

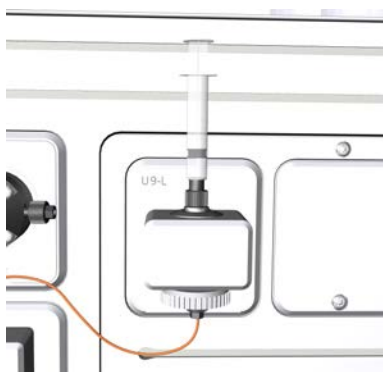

Note:

Air trapped in the UV cell causes inaccurate measurements. To avoid introducing air into the UV cell, gently fill the union Luer up to the edge with test solution that is to be introduced, using the syringe. Then insert the syringe into the union Luer.

4	Wait until the monitored absorbance value has stabilized.
---	---

Step	Action
5	In the Manual Instructions dialog: For UV monitor U9-L: • Select Monitors:Auto zero UV • Click Execute. For UV monitor U9-L, 2nd: • Select Monitors:Auto zero UV 2nd • Click Execute. <i>Result:</i> The UV absorbance is set to zero.
6	Remove the syringe.
7	Repeat the injections with the remaining four test solutions in increasing concentration order. Use a new syringe for each solution.
8	After each injection, wait for a stable absorbance value. Note the measured absorbance values for each solution.
9	Enter the measured absorbance values into the table in the column UV-900 Absorbance (AU). Note: <i>The values should be converted from mAU to AU.</i>
10	When all absorbance values have been entered into the table, the real UV flow cell path length is shown at the bottom of the table. Note: <i>The regression coefficient R2 should be larger than 0.999. If this is not the case, one or more measured values are faulty.</i>

Update the cell path length

Follow the instructions below to define the **UV cell path length** or the **UV 2nd cell path length**. The flow cell path length should be updated when the flow cell has been replaced or calibrated.

Step	Action
1	In the System Control module, select System:Calibration .
2	In the Calibration dialog, select • UV cell path length or • UV 2nd cell path length from the Monitor to calibrate drop-down list.
3	Enter the nominal flow cell path length in the Nominal length input field and click Set .

7 Maintenance

7.7 Calibration procedures

7.7.4 Calibrate the UV monitors

Step	Action
4	• If a calibration has been performed: enter the calculated flow cell path length, obtained in the calibration procedure, in the Real length input field and click Set. • If no calibration has been performed: enter the nominal flow cell path length in the Real length input field and click Set. <i>Result:</i> The UV flow cell path length is updated.

7.8 Replacement procedures

Introduction

This section gives instructions for the replacement procedures to be performed by the user of ÄKTA pure.



WARNING

Disconnect power. Always disconnect power from the instrument before replacing any component on the instrument, unless stated otherwise in the user documentation.

In this section

This section contains the following subsections:

Section	See page
7.8.1 Replace tubing and connectors	314
7.8.2 Replace internal tubing in Fraction collector F9-C	316
7.8.3 Replace the Mixer	319
7.8.4 Replace the O-ring inside the Mixer	320
7.8.5 Replace the UV monitor U9-M flow cell	322
7.8.6 Replace the UV monitor U9-L flow cell	325
7.8.7 Replace Flow restrictor	327
7.8.8 Replace the inlet filters	328
7.8.9 Replace the pump head check valves	329
7.8.10 Replace pump piston seals of Pump P9 or P9H	332
7.8.11 Replace pump piston seals of Pump P9-S	341
7.8.12 Replace pump pistons	348
7.8.13 Replace pump rinsing system tubing	349

7.8.1 Replace tubing and connectors

Maintenance interval

Replace tubing and connectors when required, for example when a tubing has clogged or has been bent so that the flow is stopped.

Required material


The following material are required:

- Tubing and connectors
 - Tubing cutter
 - Fingertight wrench
-

Instruction

Follow the instruction below to replace tubing and connectors.

Step	Action
1	Make sure that no run is in progress on the instrument.
2	Unscrew the connectors, and disconnect the tubing.
3	If the tubing has labels, remove the labels to be used with the new tubing later. Discard the tubing and connectors.

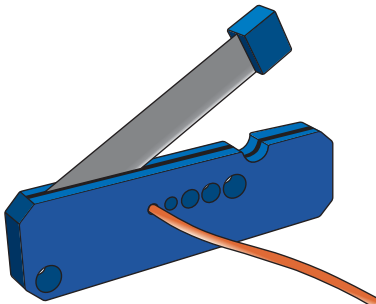Step	Action
4	Cut the new tubing to the same length as the old tubing. Use a tubing cutter to get a straight angle cut.  CAUTION Cut injuries. The tubing cutter is very sharp and must be handled with care to avoid injuries. Note: <i>When replacing system tubing, use the original inner diameter and length to ensure that the correct delay volumes are maintained. Inlet and outlet tubing may be shortened if required.</i>
5	Put the old labels on the new tubing.
6	Mount the connectors on the tubing. For fingertight connectors: • Slide the connector onto the tubing. For tubing connectors 1/8": • Slide the connector onto the tubing. • Slide the ferrule onto the tubing with the thick end towards the end of the tubing.
7	Insert the tubing with connector into the port. Make sure to insert the tubing all the way into the bottom of the port.
8	Tighten the connector fully. For areas difficult to access, use the fingertight wrench included in the accessory kit.

7.8.2 Replace internal tubing in Fraction collector F9-C

Maintenance interval

Replace tubing and connectors when required, for example when the tubing has clogged or has been bent so that the flow is stopped.

Required material


The following material are required:

- Tubing and connectors
- Tubing cutter
- Fingertight wrench

Instructions

Follow the instructions below to replace tubing and connectors. See [Section 3.2.2 Fraction collector F9-C illustrations, on page 92](#) for the locations of the components of the fraction collector.

Step	Action
1	Switch off the power to the fraction collector by switching off power to the ÄKTA pure instrument.
2	Remove the connector for the internal tubing that is attached to the inlet port: • Unscrew the connector from the inlet port.

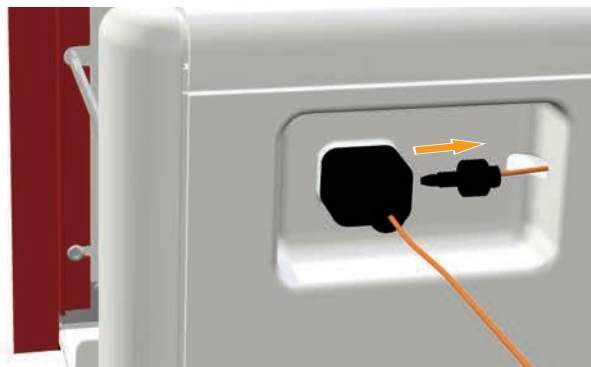


- Remove the connector from the tubing.

Step	Action
------	--------


3	Remove the tubing connector from the dispenser head:
---	--

- Open the fraction collector and gently move the fractionation arm forward.
- Unscrew the connector from the dispenser head and remove the tubing.

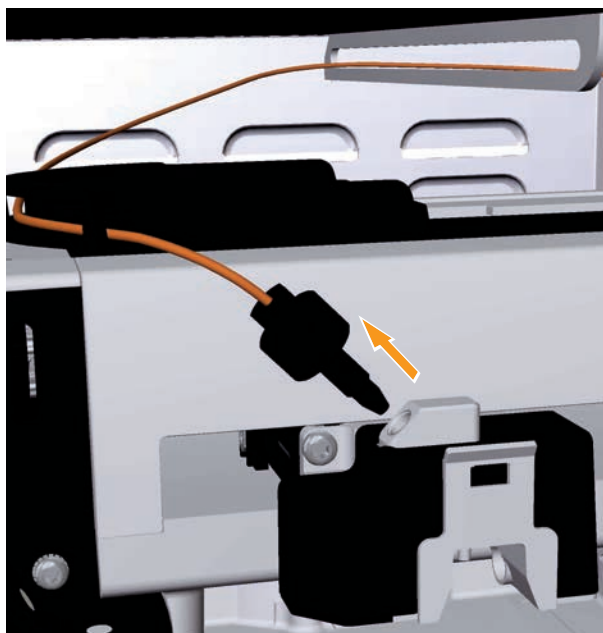

- Gently move the fractionation arm all the way back.

4	Cut the new tubing to the same length as the old tubing. Use a tubing cutter to get a straight angle cut.
---	---

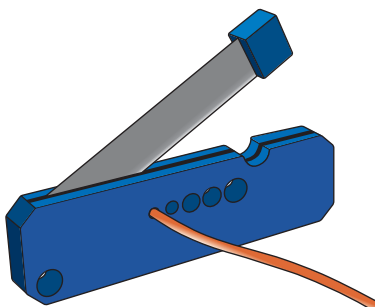

CAUTION

Cut injuries. The tubing cutter is very sharp and must be handled with care to avoid injuries.

Note:

Use tubing with the original inner diameter and length to ensure that the correct delay volume is maintained.

Step	Action
5	Attach the new tubing to the inlet port: • Thread the tubing from the interior of the fraction collector to the inlet port. • Slide the fingertight connector onto the tubing. • Insert the tubing with connector into the port. Make sure to insert the tubing all the way into the bottom of the port. • Tighten the connector fully.
6	Thread the tubing into the fraction collector and through the tubing guide in the ceiling of the fractionation chamber.
7	Position the new tubing: • Gently move the fractionation arm forward while holding the tubing. • Thread the tubing through the second tubing guide.
	
8	Attach the new tubing to the dispenser head: • Slide the fingertight connector onto the tubing. • Insert the tubing with connector into the port. Make sure to insert the tubing all the way into the bottom of the port. • Tighten the connector fully.
9	Make sure that the tubing not is twisted or bent and that it does not dip downwards.

7.8.3 Replace the Mixer

Maintenance interval

Replace the Mixer when a different Mixer chamber is desired, or when the Mixer is damaged.

Required material

The following is required:

- Mixer

Instruction

Follow the instruction below to change the Mixer.

Step	Action
1	Disconnect the tubing from the top and bottom of the Mixer.



2	Pull the Mixer away from the instrument.
---	--



3	Attach the new Mixer.
4	Reconnect the tubing to the top and bottom of the new Mixer.

7.8.4 Replace the O-ring inside the Mixer

Maintenance interval

Replace the O-ring inside the Mixer if it is damaged.

Required material

One of the following O-rings are required:

- O-ring 13.1 x 1.6 mm (for Mixer chambers 0.6, 1.4, and 5 ml)
- O-ring 13.1 x 1.6 mm (highly resistant, for use when the system is exposed to organic solvents or high concentrations of organic acids such as acetic acid or formic acid for longer periods of time).
- O-ring 22.1 x 1.6 mm (for Mixer chamber 15 ml)

Instruction

Follow the instruction below to replace the O-ring inside the Mixer.

Tip: Use a forceps and gloves during the replacement procedure to avoid contaminating the Mixer components.

Step	Action
1	Loosen the top section of the Mixer.
2	Unscrew the top section of the Mixer and pull apart the Mixer in two halves.



- 3 Remove the outer locking O-ring from the top section.



Step	Action
4	Lift up the top section of the Mixer and pull away the old O-ring inside. 
5	Wet the new O-ring with 20% ethanol and fit it in position. Make sure that the inline filter is still in position.
6	Reassemble the Mixer components and, while holding the Mixer upright, screw the top section back onto the Mixer.

7.8.5 Replace the UV monitor U9-M flow cell

Maintenance interval

Replace the UV flow cell when it is desired to use a flow cell with a different path length, or if the cell is damaged. Clean the optical fiber connectors if they have accidentally been touched.

Required material

The following materials are required:

For replacement of flow cell

- UV flow cell

For cleaning of the optical fiber connectors

- Lens paper
- Isopropanol

Replace the flow cell



CAUTION

Hazardous chemicals or biological agents in UV flow cell. Make sure that the entire flow cell has been flushed thoroughly with bacteriostatic solution (e.g., NaOH) and distilled water, before service and maintenance.

Follow the instruction to replace the UV flow cell.

Step	Action
1	Switch off the instrument.
2	Disconnect the tubing from the UV flow cell.
3	Push the latch on the UV detector to disconnect the detector.



Note:

While the UV detector is disconnected, the UV lamp becomes inoperable so no UV light can be emitted from the instrument.

Step	Action
4	Pull off the detector and the flow cell from the monochromator. Be careful not to damage the UV flow cell.  Note: <i>Make sure that the flow cell does not come into contact with any liquid, and that no liquid enters the UV detector or monochromator.</i> Note: <i>While the UV detector is disconnected, protect the fiber connectors from dust or other impurities by mounting the rubber protective caps onto them.</i> Note: <i>Do not touch the optical fiber connectors as this will result in poor monitor performance. If you accidentally touch the optical fiber connectors, clean them according to Clean the optical fiber connectors, on page 324.</i>
5	Pull off the UV flow cell from the detector.
6	Pull off the black protective caps from the new UV flow cell, and connect the new UV flow cell to the detector.
7	Connect the detector, with the new flow cell connected, to the monochromator. Pull the latch upwards to fasten the detector.
8	Connect the tubing to the new flow cell.
9	Switch on the instrument. <i>Result:</i> The flow cell path length is automatically recognized by the monitor when a new flow cell is connected.

Clean the optical fiber connectors

Follow the instruction to clean the optical fiber connectors.



WARNING

Hazardous substances. When using hazardous chemicals, take all suitable protective measures, such as wearing protective glasses and gloves resistant to the substances used. Follow local and/or national regulations for safe operation and maintenance of the product.

Step

Action

- | Step | Action |
|------|---|
| 1 | Wipe the optical fiber connectors with isopropanol on lens paper. |
| 2 | Wipe the optical fiber connectors dry with lens paper. |

7.8.6 Replace the UV monitor U9-L flow cell

Maintenance interval

Replace the UV flow cell when it is desired to use a flow cell with a different path length, or if the cell is damaged.

Required material

- UV flow cell

Replace the flow cell



CAUTION

Hazardous chemicals or biological agents in UV flow cell. Make sure that the entire flow cell has been flushed thoroughly with bacteriostatic solution (e.g., NaOH) and distilled water, before service and maintenance.

Follow the instruction below to replace the UV flow cell.

Step	Action
1	Switch off the instrument.
2	Disconnect the tubing from the UV flow cell.
3	Unscrew the knurled wheel at the bottom of the UV monitor (1). Press the wheel upwards to release the flow cell (2).



7 Maintenance

7.8 Replacement procedures

7.8.6 Replace the UV monitor U9-L flow cell

Step	Action
4	Pull the flow cell upwards out of the monitor. Hold the flow cell by the top part with the O-ring; do not touch the optical surfaces of the flow cell.



Note:

Make sure that the flow cell does not come into contact with any liquid, and that no liquid enters the monitor.

- 5 Insert a new flow cell into the monitor.
- 6 Tighten the knurled wheel firmly.
- 7 Connect the tubing to the new flow cell.
- 8 Switch on the instrument and log on to UNICORN.
- 9 Update the UV flow cell path length in the **Calibrate** dialog, in **System Control**.

Note:

The flow path cell length can be:

- updated with the nominal value, see [Update the cell path length , on page 311](#) to set the nominal flow cell path length
or
- calibrated and updated with the calculated value, see [Calibration of the UV monitor U9-L flow cell length, on page 309](#) to calibrate the flow cell path length and to update the software with the calculated value.

7.8.7 Replace Flow restrictor

Maintenance interval

Replace the Flow restrictor when required, for example when the back pressure of the Flow restrictor is outside the range 0.2 ± 0.05 MPa.

Required material

The following material is required:

- Flow restrictor **FR-902**
-

Instruction

Follow the instruction to replace the Flow restrictor.

Step	Action
1	Disconnect the tubing connected from the used Flow restrictor, and discard the used Flow restrictor.
2	Connect the tubing to the new Flow restrictor. Make sure that the Flow restrictor connector marked IN is connected to the pH valve port ToR (To Restrictor), and that the Flow restrictor connector marked OUT is connected to the pH valve port FrR (From Restrictor).
3	Check the back-pressure of the new Flow restrictor, see Section 7.4 Monthly maintenance, on page 266 .

7.8.8 Replace the inlet filters

Maintenance interval

Replace the inlet filter when required, for example when the filters are clogged.

Required material

The following material is required:


- Inlet filter set
-

Instruction

Follow the instruction to replace an inlet filter and a support net.

Step	Action
------	--------

- | | |
|---|---|
| 1 | Pull off the inlet filter and the support net from the inlet filter holder. |
|---|---|

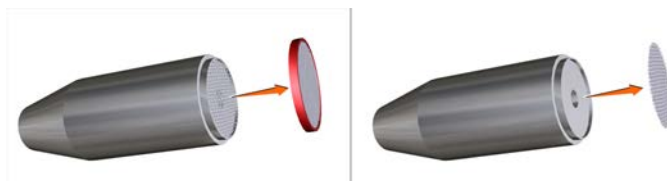

- | | |
|---|---|
| 2 | Fit the new support net and inlet filter, and press the filter into position. |
|---|---|
-

7.8.9 Replace the pump head check valves

Maintenance interval

Replace a check valve when required, for example if the check valve is damaged or clogged. The following instructions are valid for the system pumps and the sample pump.

Required material

The following materials are required:

- Check valve kit
- Adjustable wrench

Instruction




NOTICE

Handle the check valves with care when they have been removed from the pump heads, to prevent loss of any internal components.

Follow the instruction to replace the check valves of a pump.

Step	Action
1	Disconnect the tubing from the pump head and disconnect the pump inlet tubing.
2	Unscrew the purge valve by turning it counter-clockwise, and lift off the metal ring.

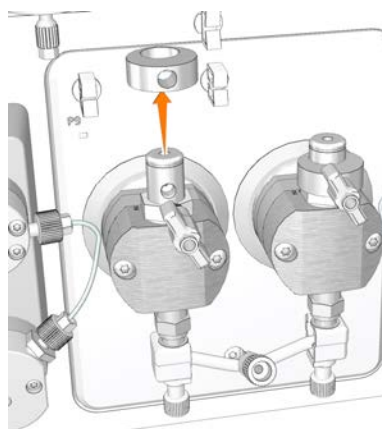


7 Maintenance


7.8 Replacement procedures

7.8.9 Replace the pump head check valves


Step	Action
3	Unscrew the plastic nut of the upper check valve using an adjustable wrench, and gently lift off the upper check valve.

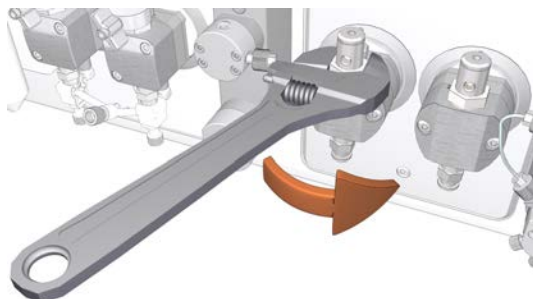

- | | |
|---|--|
| 4 | Replace the upper check valve with a new one. |
| 5 | Tighten the nut until fully finger-tight and then use the adjustable wrench to tighten a further 180 degrees. |
| 6 | Place the new metal ring onto the new upper check valve, and screw the new purge valve. |
| 7 | Unscrew the two white plastic screws located below each pump head. Pull the plastic connectors to the sides to release the inlet manifold. |

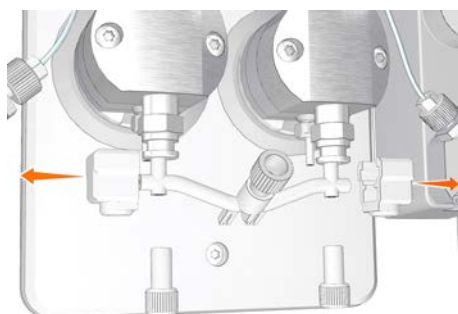

- | | |
|---|---|
| 8 | Unscrew the lower check valve using an adjustable wrench. |
|---|---|

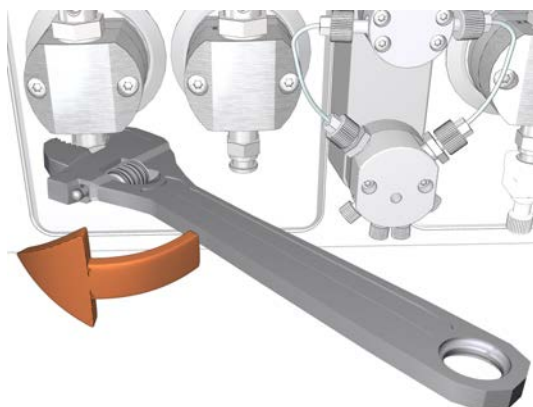

Step	Action
9	Replace the lower check valve with a new one.
10	Tighten the nut until fully finger-tight and then use the adjustable wrench to tighten a further 180 degrees.
11	Refit the inlet manifold and reconnect the tubing to the pump head.

7.8.10 Replace pump piston seals of Pump P9 or P9H

Maintenance interval

Replace the O-rings and piston seals and rinse the membranes of the pumps if they are damaged. After replacement, perform a run to break in the new piston seals.

The instructions in this section apply to the following pumps.

Configuration	Label	Pump type
System pump A, ÄKTA pure 25	P9 A	P9
System pump B, ÄKTA pure 25	P9 B	P9
System pump A, ÄKTA pure 150	P9H A	P9H
System pump B, ÄKTA pure 150	P9H B	P9H
Sample pump S9H , ÄKTA pure 150	P9H S	P9H



NOTICE

Advanced maintenance. Read the instruction carefully before disassembly of the pump head.


Required material

The following materials are required:


- Adjustable wrench
- For pump P9: Torx screwdriver, T20
- For pump P9H: Torx screwdriver, T10 and T20
- Ultrasonic bath
- Ethanol, 20%
- For pump P9: Tubing giving a back pressure of 6 to 8 MPa.
- For pump P9H: Tubing giving a back pressure of 2 to 3 MPa
- For pump P9: P9 Seal kit 25 ml
- For pump P9H: P9H Seal kit 150 ml

Illustrations

The illustrations below show the parts of the pump heads of the pumps P9 and P9H.

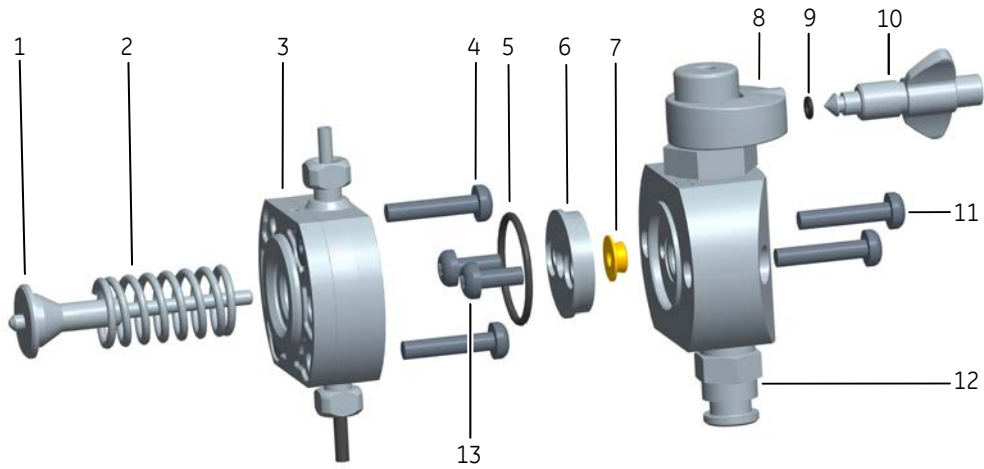

Pump P9

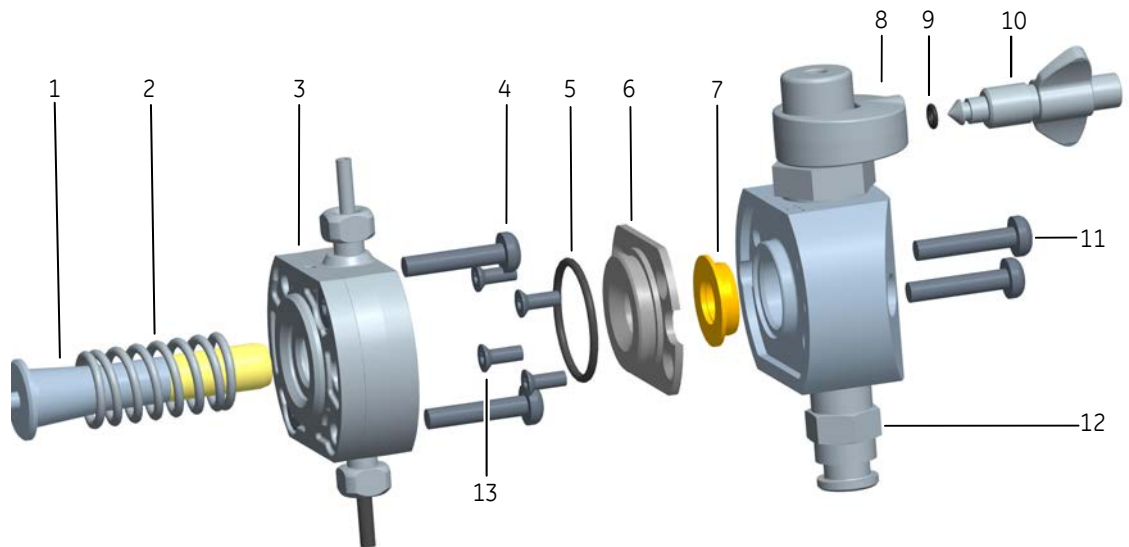

Pump P9H

7 Maintenance

7.8 Replacement procedures

7.8.10 Replace pump piston seals of Pump P9 or P9H

Part	Description	Part	Description
1	Piston	7	Piston seal
2	Return spring	8	Outlet check valve
3	Pump membrane housing	9	O-ring
4	Torx screws	10	Purge valve
5	O-ring	11	Torx screws
6	Support washer	12	Inlet check valve
13	Torx screws		


Introduction

Follow the instructions below to replace the O-rings, piston seal, and pump membrane housing of pumps **P9** and **P9H**.

Note: Always replace the O-rings, piston seals, and pump membrane housing of both pump heads of a pump at the same time.


Disassemble the pump head

Step	Action
1	Make sure that no run is in progress on the instrument.
2	Disconnect the tubing from the pump head, and disconnect the pump inlet tubing.
3	Unscrew the two white plastic screws located below each pump head by hand. Pull the plastic connectors to the sides to release the inlet manifold.

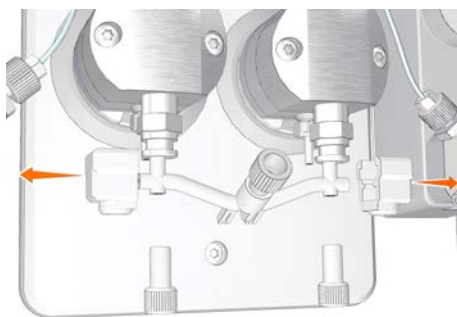

4	Disconnect the tubing of the pump piston rinsing system.
---	--

Step	Action
5	Unscrew the two screws of the front section of the pump head using a Torx screwdriver T20, and pull off the front section.

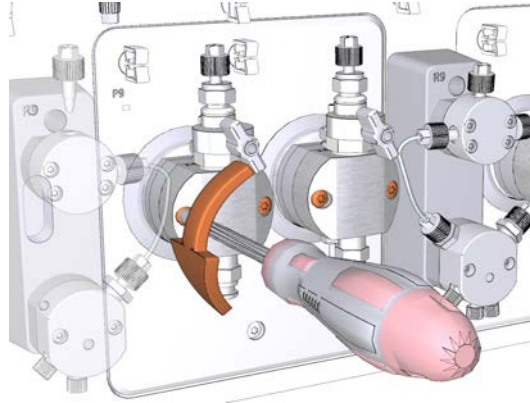


6	Place the front section of the pump head face down on the bench. For Pump P9, unscrew the two screws of the support washer using a Torx screwdriver, T20. For Pump P9H, unscrew the four screws of the support washer using a Torx screwdriver, T10. Discard the O-ring (1) on the support washer, and discard the piston seal (2) located in the front section of the pump head.
---	---

Note:

Be careful not to scratch the metal surfaces.



Pump P9


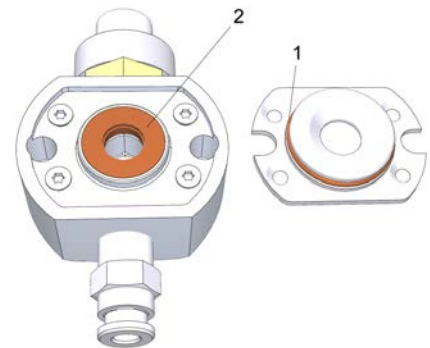


Pump P9H

7 Maintenance


7.8 Replacement procedures

7.8.10 Replace pump piston seals of Pump P9 or P9H

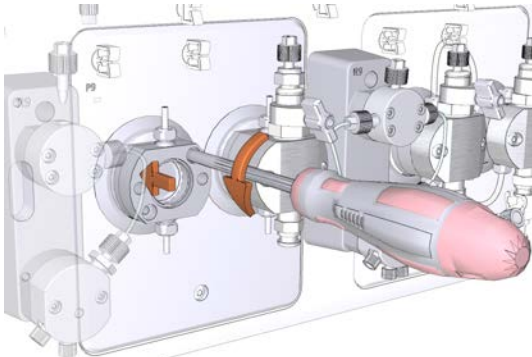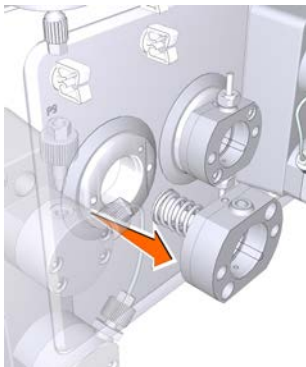Step	Action
7	Unscrew <i>one</i> of the two screws securing the pump membrane housing using a Torx screwdriver, T20. Unscrew the second screw, and at the same time push firmly on the front of the pump membrane housing to compensate for the pressure of the piston return spring.
	
8	Carefully pull off the pump membrane housing together with the piston and return spring.
	
9	Inspect the piston and return spring for signs of damage. If damaged, discard the piston and return spring and use a new piston and return spring when assembling the pump head.
10	Clean the pump head and pump membrane housing in an ultrasonic bath. If there are solids on any surfaces, the check valves should be removed and cleaned separately, see Section 7.6.8 Clean the pump head check valves, on page 293 .

Replace O-rings, piston seal and pump membrane housing


Step	Action
1	Unscrew the purge valve of the pump head. Replace the O-ring on the purge valve with a new O-ring, , and screw the purge valve back into the pump head.

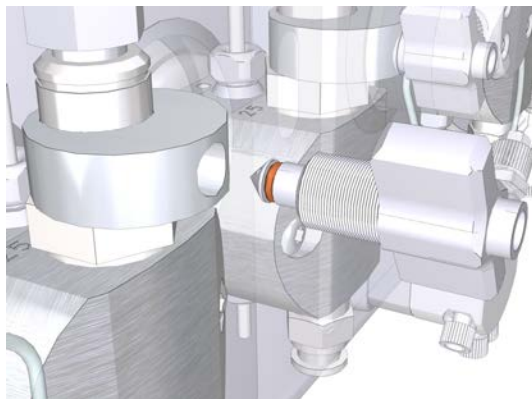


Note:

Always use Lubricant 56686700 when exchanging the O-ring 3 x 1 mm.

2	Wet a new seal with 20% ethanol. Place the new seal in the hole in the front section of the pump head and press it into position.
---	---

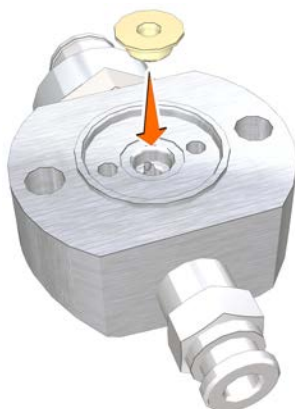

Pump P9

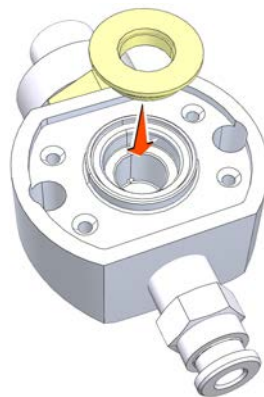

Pump P9H

7 Maintenance


7.8 Replacement procedures

7.8.10 Replace pump piston seals of Pump P9 or P9H

Step	Action
3	Place the support washer on top of the new seal in the front section of the pump head. Screw the two or four screws of the support washer. Make sure to tighten the screws fully.



Pump P9

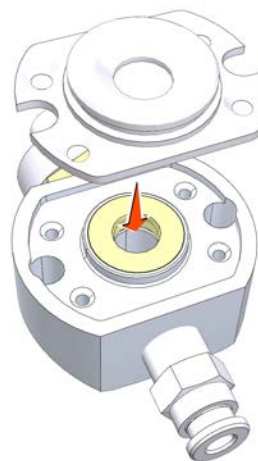

Pump P9H

4	Wet a new O-ring, 21.4 x 1.6 mm, with 20% ethanol. Fit the O-ring around the support washer.
---	--



Pump P9



Pump P9H

Assemble the pump head

Make sure to assemble the pump head correctly. Refer to the illustration [on page 333](#).

Step	Action
1	Insert the piston into the return spring. Insert piston and return spring into hole in the pump module. Note: <i>Do no touch the ceramic or glass part of the pump piston.</i>
2	Wet the membrane in the hole with 20% ethanol before mounting.
3	Place the pump membrane housing onto the locating pins on the front of the pump module.
4	Screw one of the two screws securing the pump membrane housing using a Torx screwdriver, T20. Push firmly on the front of the Pump Membrane Housing to compensate for the pressure of the piston and then screw the second screw.
5	Make sure that the new seal is wetted with 20% ethanol and then tighten both screws fully.
6	Reconnect the tubing of the pump piston rinsing system.
7	Reconnect the inlet manifold.
8	Reconnect the tubing to the pump head, and reconnect the pump inlet tubing.

Break in the new pump piston seal

Follow the instruction below to run in the new pump piston seal of pumps P9 and P9H.

Step	Action
1	Fill a buffer vessel with 20% ethanol in water. Immerse the inlet tubing, for example A1 for System pump A, or B1 for System pump B, in the buffer vessel. Place the buffer vessel on the Buffer tray.
2	Prime the inlets and purge the pump, see Section 5.4.1 System pumps, on page 159 .
3	- For pump P9: Connect tubing that gives a back pressure of 6 to 8 MPa to one of the column positions of the Column valve or between the Injection valve and the UV monitor. - For pump P9H: Connect tubing that gives a back pressure of 2 to 3 MPa to one of the column positions of the Column valve or between the Injection valve and the UV monitor.
3	Immerse the waste tubing in the buffer vessel to recirculate the liquid.

Step	Action
4	- For a system pump, in the Manual instructions dialog: - Select Flow path:Column valve, and select the position of the tubing connected to the Column valve, in this example Position 1. Click Insert. - Select Flow path:Inlet A (for System pump A) or Flow path:Inlet B (for System pump B) and select a Position, in this example A1 or B1. Click Insert. - Select Pumps:Gradient and set Target to 0% B (for System pump A) or 100% B (for System pump B). - For pump P9: Select Pumps:System flow and set the Flow rate to 5.0 ml/min. Click Insert. - For pump P9H: Select Pumps:System flow and set the Flow rate to 25.0 ml/min. Click Insert. - Click Execute. <i>Result:</i> A system flow starts. - For a sample pump, in the Manual instructions dialog: - Select Flow path:Column valve, and select the position of the tubing connected to the Column valve, in this example Position 1. Click Insert. - Select Flow path:Sample inlet and select a Position, in this example S1. Click Insert. - Select Flow path:Injection valve and select Direct inject from the Position drop-down list. Click Insert. - Select Pumps and Pressures:Sample flow and set the Flow rate to 25.0 ml/min. Click Insert. - Click Execute. <i>Result:</i> A sample flow starts.
5	Run the flow for 2 hours.
6	Discard the used buffer.

7.8.11 Replace pump piston seals of Pump P9-S

Maintenance interval

Replace the O-ring and the piston seal, and rinse the membrane of the pump if they are damaged. After replacement, perform a run to break in the new piston seals.

The instructions in this section apply to the following pump.

Configuration	Label	Pump type
Sample pump S9 , ÄKTA pure 150	P9-S	P9-S



NOTICE

Advanced maintenance. Read the instruction carefully before disassembly of the pump head.


Required material

The following material is required:

- Adjustable wrench
- Torx screwdriver, T20
- Cross-headed screwdriver
- Allen key
- Ultrasonic bath
- Ethanol, 20%
- Reference capillary **Ref 1**
- P9-S Seal kit 65 ml

Illustration

The illustration below shows the parts of the pump heads of pump P9-S.

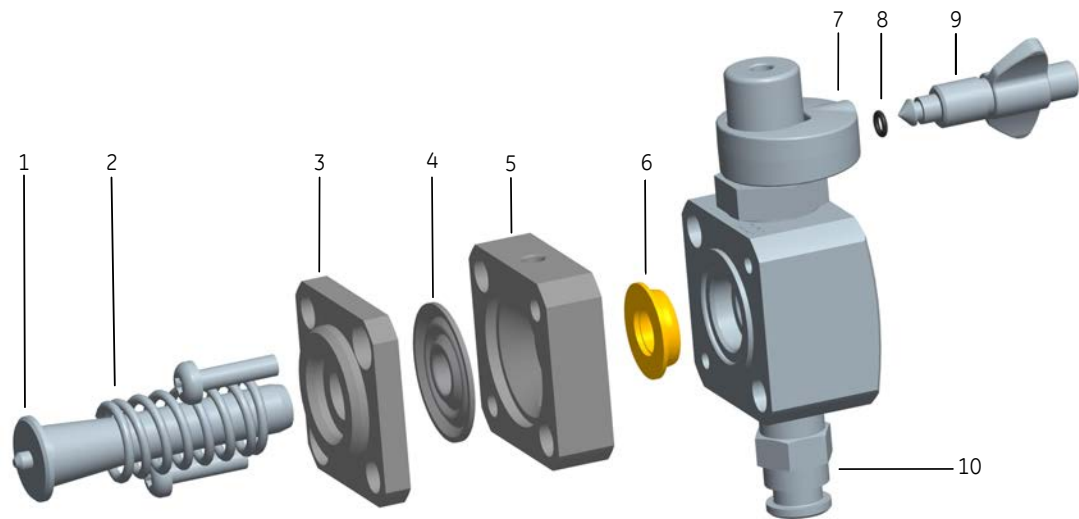

Part	Description	Part	Description
1	Piston	6	Piston seal
2	Return spring	7	Outlet check valve
3	Drain plate	8	O-ring
4	Rinse membrane	9	Purge valve
5	Rinse chamber	10	Inlet check valve

Introduction


Follow the instructions below to replace the o-ring, piston seal, and rinse membrane of pump P9-S.

Note: Always replace the o-rings, piston seals, and rinse membranes of both pump heads of a pump at the same time.


Disassemble the pump head

Step	Action
1	Make sure that no run is in progress on the instrument.
2	Disconnect the tubing from the pump head, and disconnect the pump inlet tubing.


Step	Action
3	Unscrew the two white plastic screws located below each pump head by hand. Pull the plastic connectors to the sides to release the inlet manifold.

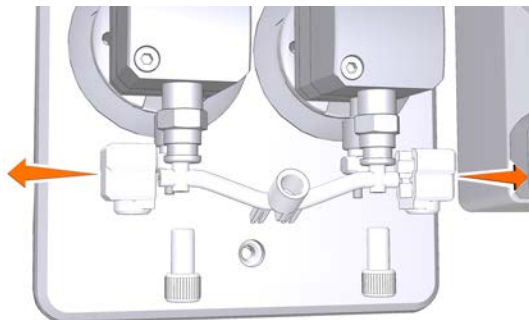


- 4 Disconnect the tubing of the pump piston rinsing system.
- 5 Unscrew *one* of the two screws of the pump head using an Allen key. Unscrew the second screw, and at the same time push firmly on the front of the rinse chamber to compensate for the pressure of the piston return spring.

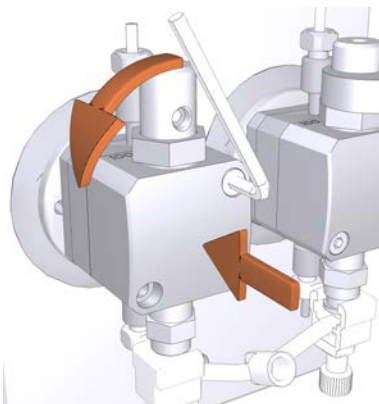


- 6 Place the pump head face down on the bench. Pull out the piston together with the return spring.

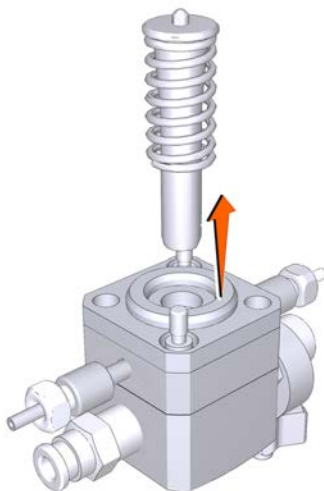

Step	Action
7	Inspect the piston and return spring for sign of damage. If damaged, discard the piston and return spring and use a new piston and return spring when assembling the pump head.
9	Unscrew the two screws securing the drain plate and the rinse chamber. Lift off the drain plate, and discard the membrane located between the drain plate and the rinse chamber.

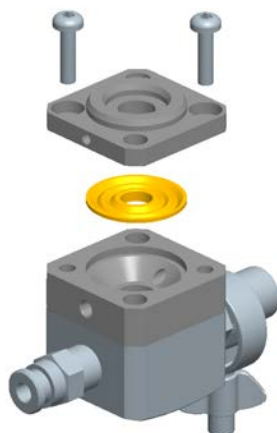


10	Lift off the rinse chamber. Gently pull off the piston seal. Discard the used seal.
----	---

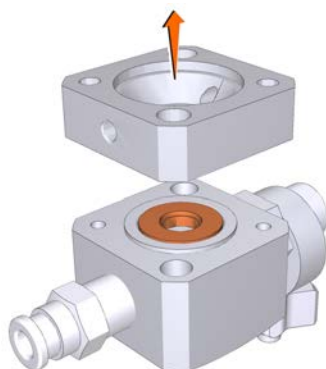

11	Clean the pump head, rinse chamber and drain plate in an ultrasonic bath. If there are solids on any surfaces, the check valves should be removed and cleaned separately, see Section 7.6.8 Clean the pump head check valves, on page 293 .
----	---

Replace O-ring, piston seal, and rinse membrane


Step	Action
1	Unscrew the purge valve of the pump head. Replace the O-ring on the purge valve with a new O-ring, 3x1 mm, and screw the purge valve back into the pump head.

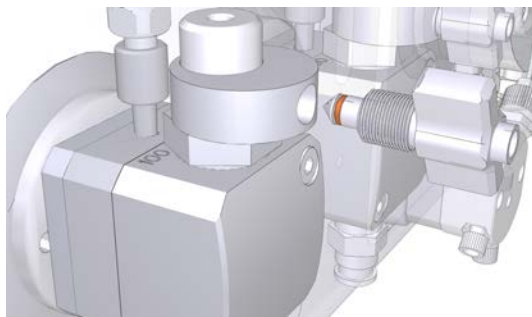

Note:

Always use Lubricant 56686700 when exchanging the O-ring 3 x 1 mm.

2	Wet a new seal with 20% ethanol. Place the new seal in the hole in the front section of the pump head and press it into position.
---	---

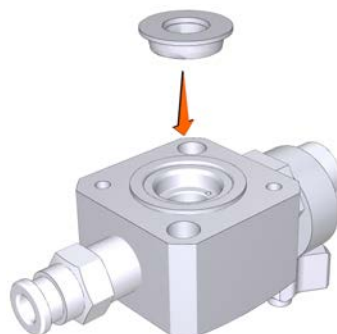

3	With the pump head facing downwards on the bench, place the rinse chamber onto the front section of the pump head with the rinse ports in line with the check valves. The conical depression in the rinse chamber shall be facing upwards. Wet a new membrane with 20% ethanol, and place the membrane into the rinse chamber with the conical face upwards.
---	--



Assemble the pump head

Make sure to assemble the pump head correctly. Refer to the illustration [on page 342](#).

Step	Action
1	Place the drain plate on top of the assembly. Screw the two screws through the drain plate and the rinse chamber using a cross-headed screwdriver.
2	Wipe clean the piston and remove all finger prints. Wet the piston with 20% ethanol, and insert the piston into the return spring. With the pump head facing downwards on the bench, insert the piston into the pump head by pushing it gently but firmly vertically downwards into the seal.
3	Place the complete pump head over the locating pins on the front panel of the Sample pump module. Turn the pump head so that the text UP on the drain plate is facing upwards. Push firmly on the front of the pump head, and at the same time screw one of the screws to fasten the pump head onto the front of the module using an Allen key. Screw the second screw of the pump head. Make sure to tighten both screws fully.
4	Reconnect the tubing of the pump piston rinsing system.
5	Reconnect the inlet manifold.
6	Reconnect the tubing to the pump head, and reconnect the pump inlet tubing.
7	Break in the new pump piston seal, see instruction below.

Break in the new pump piston seal

Follow the instruction below to break in the new pump piston seal of pump P9-S.

Step	Action
1	Fill a buffer vessel with 20% ethanol in water. Immerse a piece of sample inlet tubing, for example S1 , in the buffer vessel. Place the buffer vessel on the Buffer tray.
2	Prime the inlets and purge the pump, see Section 5.4.2 Sample pump, on page 165
3	Connect the reference capillary Ref 1 (or equivalent tubing that gives a backpressure of 2-3 MPa) to one of the column positions of the Column valve (e.g., ports 1A and 1B).
4	Immerse the waste tubing in the buffer vessel to recirculate the liquid.

Step	Action
5	In the Manual instructions dialog: • Select Flow path:Column position, and select the Position of the tubing connected to the Column valve, in this example 1. Click Insert. • Select Flow path:Sample inlet and select a Position, in this example S1. Click Insert. • Select Flow path:Injection valve and select Direct inject from the Position drop-down list. Click Insert. • Select Pumps:Sample flow and set the Flow rate to 25.0 ml/min. Click Insert. • Click Execute. <i>Result:</i> A sample flow of 25 ml/min starts.
6	Run the flow for 2 hours.
7	Discard the used buffer.

7.8.12 Replace pump pistons

Maintenance interval

Replace the pump pistons if they are damaged.

Required material

The following materials are required:

- Adjustable wrench
 - Torx screwdriver, T20
 - Piston kit
-

Replace pump pistons of Pump P9 and P9H

If a damaged piston has been in operation, the piston seal will be destroyed and should also be replaced. To replace the piston and the seal of a system pump, see [Section 7.8.10 Replace pump piston seals of Pump P9 or P9H, on page 332](#).

Replace pump pistons of Pump P9-S

If a damaged piston has been in operation, the piston seal will be destroyed and should also be replaced. To replace the piston and the seal of the sample pump, see [Section 7.8.11 Replace pump piston seals of Pump P9-S, on page 341](#)

7.8.13 Replace pump rinsing system tubing

Maintenance interval

Replace the pump rinsing system tubing when required, for example if the tubing is clogged or damaged. Replacement instructions for the system pumps and the sample pump (external module) are given below.


Required material

The following material is required:

- Rinsing system tubing

System pump piston rinsing system


The illustrations below show the parts and tubing of the system pump piston rinsing system

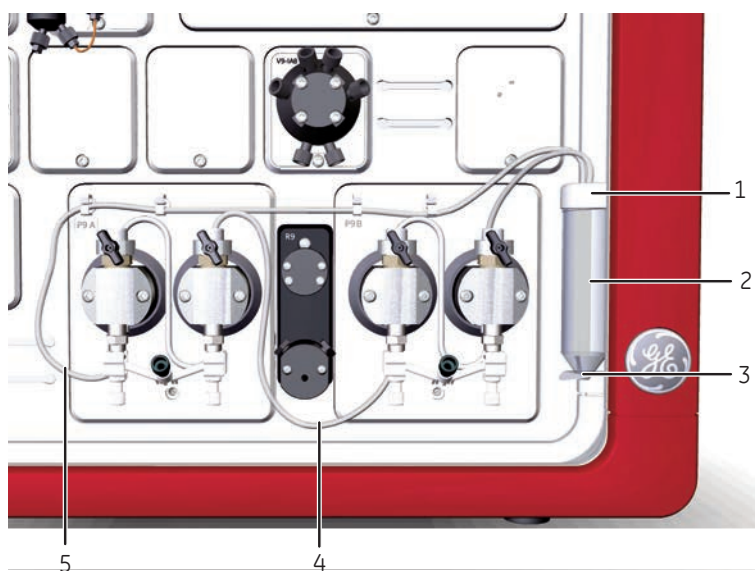


Part	Description
1	Rinsing system tube holder, top
2	Rinsing system tube
3	Rinsing system tube holder, bottom
4	Outlet tubing
5	Inlet tubing

Sample pump piston rinsing system

The illustrations below show the parts, tubing and flow path of the sample pump piston rinsing system.

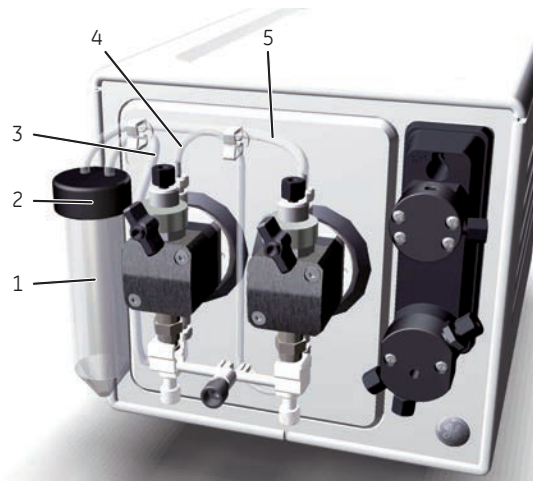

Parts and tubing



Rinsing system flow path

Part	Function
1	Pump rinsing liquid tube
2	Pump rinsing liquid tube holder
3	Inlet tubing, from the rinsing liquid tube to the left pump head (lower rinsing system connection) .
4	Tubing between the left pump head (upper rinsing system connection) and the right pump head (lower rinsing system connection).
5	Outlet tubing, from the right pump head (upper rinsing system connection) to the rinsing liquid tube.

Connect new tubing

Step	Action
1	Disconnect the used tubing.
2	Cut the new tubing to desired length.
3	Connect the new tubing according to the illustrations above.
4	Fit all pieces of tubing into the tubing holders on the pump modules.

Prime the rinsing systems

Before usage, prime the pump rinsing system tubing. Refer to [Section 7.3.1 Change pump rinsing solution, on page 259](#) for detailed instructions.

8 Troubleshooting

About this chapter

This chapter describes troubleshooting and corrective actions for ÄKTA pure.

In this chapter

This chapter contains the following sections:

Section	See page
8.1 Introduction to troubleshooting	353
8.2 Troubleshooting: General Checklist	355
8.3 Troubleshooting: Monitors	357
8.4 Troubleshooting: Valves	372
8.5 Troubleshooting: Fraction collector	374
8.6 Troubleshooting: Pumps	384
8.7 Troubleshooting: Other components	391
8.8 Troubleshooting: Instrument communication	398
8.9 Troubleshooting: Method development	400
8.10 Error codes	401

8.1 Introduction to troubleshooting

Introduction

This section describes troubleshooting procedures for ÄKTA pure and how to generate a System error report for service purposes. Subsequent sections in this chapter present general troubleshooting checklists, module-specific problems and corrective actions.

Troubleshoot the software

For software related troubleshooting, see the following table and the list of literature below:

Problem	Possible cause and action
Text in the <i>Process Picture</i> pane in the <i>System control</i> module looks strange	The operating system of the computer does not have the text font Calibri True Type installed. For example, Windows XP does not include this font by default. Install the font Calibri True Type or switch to an operating system that includes the font.

- *UNICORN Method Manual*,
- *UNICORN Evaluation Manual* and
- *UNICORN Administration and Technical Manual*

Troubleshooting procedure

To troubleshoot ÄKTA pure:

Step	Action
1	Always start by checking the General checklist. See Section 8.2 Troubleshooting: General Checklist, on page 355 .
2	In this document, search for solutions in the section corresponding to the problem.
3	Make the recommended corrective actions.
4	If problems remain after corrective actions, generate a System error report and contact your local GE representative.

Generate a System error report

A System error report can be generated during a troubleshooting case with information about the problem and can also include methods, logs, and results. The report can then be sent to Service for action.

To generate a System error report for information to Service:

Step	Action
1	In the System Control module, on the System menu, click Create System Error Report . <i>Result:</i> The first page of a wizard is displayed.
2	- Click Next and start to enter information about the problem, click Next. - Choose to enclose methods, logs or result files. - Select location for the report and click Finish to generate the report. The filename of the zip file will be <code>Report_YYYYMMDD.zip</code> and the default folder location is: <code>C:\Program Files\GE Healthcare\UNICORN</code>.
3	E-mail the report to GE Service department.

8.2 Troubleshooting: General Checklist

Introduction

Check the items in the following topics before starting more in-depth troubleshooting work.

System checks

- Is the correct system selected in UNICORN **System Control**? For more details, see [Section 5.3 Start UNICORN and connect to system, on page 155](#).
 - Are the fans blowing at the back and at the right side of the system?
-

Monitor checks

- Is the UV monitor set to the correct wavelength? Check the wavelengths that are used in the method. For the predefined methods the wavelengths are set in the **Method Settings** phase. For more details, see UNICORN Method Manual.
 - Is the air sensor sensitivity set to normal in UNICORN **System Control: System Settings** to avoid unnecessary stops due to minor air bubbles?
-

Instrument communication

- Have Node IDs been set correctly for all instrument modules? To check and change Node IDs, see [Node ID, on page 76](#).
-

Flow path checks

- Is all tubing connected correctly? See [Section 9.3 Tubing and connectors, on page 419](#) and [Section 5.2 Prepare the flow path, on page 148](#).
- Is there leakage at any of the connections?
- Is any tubing folded or twisted?
- Is the inlet tubing correctly immersed in the buffer solution, beneath the liquid surface but not too close to the flask bottom?
- Have Fraction collector F9-R and Fraction collector F9-C been correctly prepared? For more details, see relevant sections in [Chapter 3 ÄKTA pure external modules, on page 86](#) and [Chapter 4 System configuration, on page 121](#).
- Are the inlet and inline filters clean or are they generating a back pressure higher than normal? If this is the case, change the inline and inlet filters. For more details, see [Section 7.3.2 Replace the inline filter, on page 263](#) and [Section 7.8.8 Replace the inlet filters, on page 328](#).

- Does the positioning of the columns correspond to the selections made in the method? For more details, see [Section 5.5 Connect a column, on page 170](#).
-

Purification checks

- Have all columns been cleaned and prepared according to the column recommendations?
 - Have the samples been adjusted to binding buffer conditions?
 - Have the samples been clarified by centrifugation and/or filtration prior to sample loading?
 - Are the correct buffers used for the chosen columns and proteins?
 - Check buffers for precipitations. Adjust to room temperature.
 - Are the chosen columns suitable for the chosen target proteins?
 - Do the buffers have correct pH? The pH of some buffers changes with the temperature.
 - Are the UV-wavelengths used by the method appropriate with respect to used buffers and proteins? For more details see the method handbooks available from GE.
-

8.3 Troubleshooting: Monitors

In this section

- UV monitor and UV detector
- Conductivity monitor
- pH monitor and pH valve
- Pressure monitors

UV monitor U9-M and UV detector unit

Problem	Possible cause and action
The UV module is not found by the instrument	• Communication problem Contact Service. • The cable between the UV module and the ICU is not connected Remove the UV module and make sure that the cable is connected. • Wrong Node ID Check the module's Node ID. If necessary, change the Node ID. See Node ID, on page 76.
Too low UV lamp intensity	• The detector is not correctly fitted Contact Service. • Unclean optical fiber connectors Clean the connectors. See Section 7.8.5 Replace the UV monitor U9-M flow cell, on page 322. • Dirt on optical sensors in detector Remove visible dirt on detector photo diodes. Use lint free lens paper winded around a thin wood splinter (e.g a match or toothpick). Clean the sensors with Isopropanol through the small hole of the metal plate which covers the sensors. Dry the sensors with clean and dry lint free lens paper. • Worn-out or broken lamp Contact Service.

Problem	Possible cause and action
No light transmission through the UV cell	• Wrong wavelength for current buffer Change wavelength or buffer. • Dirt in the UV flow cell Clean the UV cell. See Section 7.5.1 Clean the UV flow cell, on page 270. • Unclean optical fiber connectors Clean the connectors. See Section 7.8.5 Replace the UV monitor U9-M flow cell, on page 322. • Broken UV flow cell Replace UV flow cell. See Section 7.8.5 Replace the UV monitor U9-M flow cell, on page 322.
Autozero out of accepted range	• Wrong wavelength for current buffer Change wavelength or buffer. • Unclean optical fiber connectors Clean the connectors. See Section 7.8.5 Replace the UV monitor U9-M flow cell, on page 322.
The internal temperature of the UV monitor is too high	• The air intake on the rear or on the left side of the instrument is covered Make sure that none of the air intakes on the instrument are covered. • Hot surroundings Decrease the room temperature. Maximum operating temperature is 35°C. • Hardware error Switch off the instrument and wait until the temperature has decreased. Restart the instrument. If this error is recurrent, generate a System error report and contact Service.
UV cell path length unreadable	• No UV flow cell is attached Attach UV cell. See Section 7.8.5 Replace the UV monitor U9-M flow cell, on page 322. • UV flow cell is not correctly installed. Verify that the UV cell is correctly installed. See Section 7.8.5 Replace the UV monitor U9-M flow cell, on page 322. • The UV flow cell is broken Replace the cell. See Section 7.8.5 Replace the UV monitor U9-M flow cell, on page 322.

Problem	Possible cause and action
Ghost peaks	Air in the UV flow cell Use the Flow restrictor. Use the pH valve instruction to manually set the Flow restrictor inline (Flow path:pH valve:Restrictor in-line), or select the Flow restrictor in the Method Settings phase of a method. Remove the air by flushing the cell with water or buffer. If persistent, clean the UV cell. See Section 7.5.1 Clean the UV flow cell, on page 270. Air in buffers De-gas if necessary. Dirt in the UV flow cell Clean the UV cell. See Section 7.5.1 Clean the UV flow cell, on page 270. Dirt in the flow path Clean the system in accordance to Section 7.6.2 Perform System CIP, on page 275. Clean the column in accordance to Section 7.6.3 Perform Column CIP, on page 281.

Problem	Possible cause and action
Baseline drift or noisy signal	Flow restrictor in off-line position Use the Flow restrictor. Use the pH valve instruction to manually set the Flow restrictor inline (Flow path:pH valve:Restrictor in-line), or select the Flow restrictor in the Method Settings phase of a method. Air in the UV flow cell Use the Flow restrictor. Remove the air by flushing the cell with water or buffer. If persistent, clean the UV cell. See Section 7.5.1 Clean the UV flow cell, on page 270. Air in buffers De-gas if necessary. - Make sure that both the instrument and the buffers have reached the ambient temperature. Impure buffers Check if the signal is noisy with water. Unclean optical fiber connectors Clean the connectors. See Section 7.8.5 Replace the UV monitor U9-M flow cell, on page 322. Dirt in the UV flow cell Perform a System CIP. See Section 7.6.2 Perform System CIP, on page 275. If necessary, manually clean the UV cell. See Section 7.5.1 Clean the UV flow cell, on page 270. Wrong type of UV cell is used If a UV cell with 2 mm path length is to be used, use only cells marked U9-2.

Problem	Possible cause and action
Unstable signal	• Bad pump function Check that the pump is operating properly. See Select Mixer chamber, on page 149 for example of pump pressure curves. • Poor mixing function Check the mixer chamber size and change the chamber if necessary. See Select Mixer chamber, on page 149. Check the function of the mixer. Place a stirrer bar in the palm of your hand. Hold the hand above the mixer. The stirrer should move when the mixer is activated. Check that the mixer chamber is free from solids. To open the mixer, see Section 7.3.2 Replace the inline filter, on page 263.
The UV curve shows a gradient that is inverted compared to the expected gradient	• Large difference in refractive index between buffer A and buffer B Due to light spreading effects in the UV cell, the buffer with the highest UV absorption shows the lowest UV absorption in the chromatogram, and the buffer with the lowest UV absorption shows the highest UV absorption. This can occur if there is a large difference in refractive index between buffer A and buffer B and the UV is run at high sensitivity.

UV monitor U9-L

Problem	Possible cause and action
Autozero out of accepted range	• Wrong UV flow cell for current buffer Change to a shorter UV flow cell or change buffer. • The UV flow cell is not correctly installed Check that the UV flow cell is fitted correctly, see Section 7.8.6 Replace the UV monitor U9-L flow cell, on page 325. • Broken UV flow cell Replace the cell, see Section 7.8.6 Replace the UV monitor U9-L flow cell, on page 325.

Problem	Possible cause and action
The internal temperature of the UV monitor is too high	• The air intake on the rear or on the right side of the instrument is covered Make sure that none of the air intakes on the instrument are covered. • Hot surroundings Decrease the room temperature. Maximum operating temperature is 35°C. • Hardware error Switch off the instrument and wait until the temperature has decreased. Restart the instrument. If this error is recurrent, generate a System error report and contact Service.
Maximum absorbance that can be measured by the detector is reached	• Wrong UV flow cell for current buffer Change to a shorter UV flow cell or change buffer. • The UV flow cell is not correctly installed Check that the UV flow cell is fitted correctly, see Section 7.8.6 Replace the UV monitor U9-L flow cell, on page 325. • Dirt in the UV flow cell Clean the UV flow cell, see Section 7.5.1 Clean the UV flow cell, on page 270. • Broken UV flow cell Replace the cell, see Section 7.8.6 Replace the UV monitor U9-L flow cell, on page 325.
The UV cell is not correctly installed	• Check that the UV flow cell is fitted correctly, see Section 7.8.6 Replace the UV monitor U9-L flow cell, on page 325.

Problem	Possible cause and action
Ghost peaks	Air in the UV flow cell Use the Flow restrictor. Use the pH valve instruction to manually set the Flow restrictor inline (Flow path:pH valve:Restrictor in-line), or select the Flow restrictor in the Method Settings phase of a method. Remove the air by flushing the cell with water or buffer. If persistent, clean the UV cell. See Section 7.5.1 Clean the UV flow cell, on page 270. Air in buffers De-gas if necessary. Dirt in the UV flow cell Clean the UV cell. See Section 7.5.1 Clean the UV flow cell, on page 270. Dirt in the flow path Clean the system in accordance to Section 7.6.2 Perform System CIP, on page 275. Clean the column in accordance to Section 7.6.3 Perform Column CIP, on page 281.
The UV lamp is broken or worn out	Contact Service

Problem	Possible cause and action
Distorted protein peaks in IEX gradients (for example step gradients).	Rapid changes of the refractive index The refractive index of the buffer changes rapidly in quick IEX gradients. The rapid change may cause light spreading effects and disturb the shape of the protein peaks in the U9-L 2 mm flow cell. Run with reversed flow direction through the 2 mm cell: connect the inlet tubing at the bottom and the outlet tubing at the top of the flow cell. Note: The standard tubing (7) between the UV monitor and the conductivity monitor is too short (170 mm) for mounting the monitor for reversed flow direction. Perform the following actions: 1 Replace the standard tubing with a tubing that is 210 mm long. 2 Update the total delay volume. The increase in volume depends on the inner diameter (i.d.) of the tubing: - i.d. 0.25 mm : 2 µl - i.d. 0.50 mm : 8 µl - i.d. 0.75 mm: 18 µl - i.d. 1.0 mm: 32 µl

Conductivity monitor

Problem	Possible cause and action
The conductivity part of the system performance test failed	Test was performed at cold room temperature and the conductivity temperature compensation factor was not optimized. In the System Settings dialog, select Conductivity:Cond temp compensation and set the Compensation factor to 2.1%.
The cell constant measurement has been aborted	Internal errors See error log. Restart instrument and retry. If this problem recurs, generate a System error report and contact Service.
Unstable conductivity	Air in the Conductivity flow cell Flush the Conductivity flow cell with water. Solids in the Conductivity flow cell Clean the Conductivity cell. See Section 7.6.10 Clean the Conductivity flow cell, on page 297.

Problem	Possible cause and action
Temperature out of range for calibration	• This error can only occur when the temperature compensation is turned on. The error will occur when the temperature is outside the range 2°C to 40°C. Make sure the temperature of the calibration solution is within 2°C and 40°C.
Baseline drift of noisy signal	• Air in the Conductivity flow cell Use the Flow restrictor. Remove the air by flushing the flow cell with water or buffer. • Leaking tubing connections Tighten the connectors. If necessary, replace the connectors. • Unclean Conductivity flow cell Clean the Conductivity flow cell. See Section 7.6.10 Clean the Conductivity flow cell, on page 297. • Poor mixing function Check the Mixer chamber size and change chamber if necessary, see Select Mixer chamber, on page 149. Check the motor operation of the Mixer. Place a magnet close to the Mixer chamber during run. The magnet should vibrate. Check that the Mixer chamber is free from solids. To replace the inline filter, see Section 7.3.2 Replace the inline filter, on page 263.
Conductivity measurement with the same buffer appears to decrease/increase over time.	• Unclean conductivity flow cell Clean the Conductivity cell, see Section 7.6.10 Clean the Conductivity flow cell, on page 297. • The ambient temperature may have decreased/increased Use a temperature compensation factor. The temperature compensation factor is found in System Control: System Settings: Conductivity. Instruction regarding the factor is also found in Section 7.7.3 Calibrate the Conductivity monitor, on page 305. • The Conductivity monitor needs to be calibrated Check calibration with a solution with known conductivity. Calibrate the Conductivity monitor, see Section 7.7.3 Calibrate the Conductivity monitor, on page 305.

Problem	Possible cause and action
Waves on the gradient	• Bad pump function Check that the pump is operating properly. See Examples of pump pressure curves, on page 387 for example of pump pressure curves. • Air in the flow path Purge the pumps. See Section 5.4.1 System pumps, on page 159. • Poor mixing function Check that the correct Mixer chamber size is used. See Select Mixer chamber, on page 149 for recommendations. To change the Mixer, see Section 7.8.3 Replace the Mixer, on page 319. Check the motor operation of the Mixer. Place a magnet close to the mixer chamber during run. The magnet should vibrate. Check that the Mixer chamber is free from solids. To open the mixer, see Section 7.3.2 Replace the inline filter, on page 263.
Ghost peaks appear in the gradient profile	• A charged particle has been detected Prepare the sample so that charged particles are eliminated. • Air bubbles are passing through the flow cell Check for loose tubing connections. Use the Flow restrictor.
Non-linear gradients or slow response to %B changes	• Dirt in the tubing Make sure that the tubing has been washed properly. • Bad pump function Make sure that the pump operates properly. See Examples of pump pressure curves, on page 387 for example of pump pressure curves. • The Mixer chamber is too large Change to a Mixer chamber with a smaller volume. See Select Mixer chamber, on page 149 for recommendations. To change the Mixer, see Section 7.8.3 Replace the Mixer, on page 319.

Problem	Possible cause and action
Incorrect or unstable reading	• The temperature compensation factor is not properly set Use a temperature compensation factor. The temperature compensation factor is found in System Control: System Settings: Conductivity. Instruction regarding the factor is also found in Section 7.7.3 Calibrate the Conductivity monitor, on page 305. • The column is not equilibrated Equilibrate the column. Use the method phase Equilibration. If necessary, clean the column. Use the predefined method Column CIP. See Section 7.6.3 Perform Column CIP, on page 281. • Poor mixing function Check that the correct Mixer chamber size is used. See Select Mixer chamber, on page 149 for recommendations. To change the Mixer, see Section 7.8.3 Replace the Mixer, on page 319. Check the motor operation of the mixer. Place a magnet close to the Mixer chamber during run. The magnet should vibrate. Check that the Mixer chamber is free from solids. To open the mixer, see Section 7.3.2 Replace the inline filter, on page 263.

pH monitor and pH valve

Problem	Possible cause and action
The pH module is not found by the instrument	• The cable between the pH valve and the ICU is not connected Remove the pH valve and make sure that the cable is connected. See Hardware installation of a module, on page 76.
The internal valve temperature is too high	• The air intake on the rear or on the left side of the instrument is covered Make sure that none of the air intakes on the instrument are covered. • Hot surroundings Decrease the room temperature. Maximum operating temperature is 35°C. • Hardware error Switch off the instrument and wait until the temperature has decreased. Restart the instrument. If this error is recurrent, generate a System error report and contact Service.

Problem	Possible cause and action
Unstable pH signal	Calibration time out Check the connections between pH electrode and pH monitor. Regenerate the pH electrode. Place the electrode in deionized water for 30 minutes followed by 30 minutes in a buffer with pH 4. If persistent, replace the pH electrode. See Section 7.5.2 Replace the pH electrode, on page 272. Bad pH electrode Regenerate the pH electrode. Place the electrode in deionized water for 30 minutes followed by 30 minutes in a buffer with pH 4. Clean the pH electrode. See Section 7.6.7 Clean the pH electrode, on page 290. If persistent, replace the pH electrode. See Section 7.5.2 Replace the pH electrode, on page 272. Wrong mixer size for the used flow rate Use the recommended mixer size for the used flow rate. See
Drift of pH signal when the pH electrode has been removed from storage solution	Decreasing salt concentration in the electrode membrane due to osmosis to buffer Regenerate the pH electrode. Place the electrode in deionized water for 30 minutes followed by 30 minutes in a buffer with pH 4.
Temperature reading error	The temperature compensation of the pH monitor is turned off Contact Service.
It is not possible to inject calibration solution	Waste tubing is twisted or blocked Untwist the tubing. Perform System CIP to clean waste tubing. See Section 7.6.2 Perform System CIP, on page 275. Change the tubing.

Problem	Possible cause and action
Alarm in UNICORN: (Alarm) The pH cell can only be run at pressures below 0.8 MPa. Please check the tubing or lower the flow through the pH cell. Note: The pressure limit 0.8 MPa is for the post column pressure.	• High pressure in the pH cell Decrease the flow rate. Bypass the pH electrode (see Ports and flow paths of the pH valve, on page 61) and measure pH in fractions manually.

Pressure monitors

Problem	Possible cause and action
Pressure offset	• The monitors have lost their calibration Calibrate the pressure monitors. See Section 7.7.2 Calibrate the pressure monitors, on page 302. • The temperature has changed Wait until the temperature has stabilized and calibrate the pressure monitors.
Excessively high pressure values	• Unclean inline filter in the Mixer Replace the inline filter in the Mixer. See Section 7.3.2 Replace the inline filter, on page 263. • Solids in the flow path To use the predefined method System CIP to clean the flow path, see Section 7.6.2 Perform System CIP, on page 275. To clean the column, see Section 7.6.3 Perform Column CIP, on page 281. If persistent, replace the column. • 0.25 mm i.d. tubing kit is mounted A smaller tubing inner diameter gives higher back pressure. The back pressure for the 0.25 mm i.d. tubing kit is normally 16 times higher than for the 0.50 mm i.d. tubing kit used at the same running conditions. Maximum system flow rate for 0.25 mm i.d. tubing is 10 ml/min
The pressure monitors are not found by the instrument	• The cable between the Pressure monitors and the ICU is not connected. Remove the monitor and make sure that the cable is connected.

Problem	Possible cause and action
The internal temperature of the pressure monitor is too high	The air intake on the rear or on the left side of the chromatography instrument or the sample pump is covered Make sure that none of the air intakes on the instrument are covered. Hot surroundings Decrease the room temperature. Maximum operating temperature is 35°C. Hardware error Switch off the instrument and wait until the temperature has decreased. Restart the instrument. If this error is recurrent, generate a System error report and contact Service.

Problem	Possible cause and action
Irregular pressure curves	Air bubbles are passing through or are trapped in the pump Check that there is a sufficient volume of buffer present in the flasks. Check all connections for leaks. Check pump pressure curves. See Examples of pump pressure curves, on page 387 for examples of pump pressure curves. Purge the pumps, see Section 5.4.1 System pumps, on page 159 or Section 5.4.2 Sample pump, on page 165 The check valve does not function correctly Remove any solids in the valves by cleaning the check valves according to the instructions in Section 7.6.8 Clean the pump head check valves, on page 293. Piston seal is leaking Replace the piston seal of a system pump according to the instructions in Section 7.8.10 Replace pump piston seals of Pump P9 or P9H, on page 332. Replace the piston seal of the sample pump according to the instructions in Section 7.8.11 Replace pump piston seals of Pump P9-S, on page 341 Blockage of flow path Use the predefined method Prepare System to flush through to clear blockage. If necessary, replace tubing. See Section 7.8.1 Replace tubing and connectors, on page 314. Check the mixer inline filter. It can be clogged if unfiltered buffers or samples are applied. See Section 7.3.2 Replace the inline filter, on page 263 for instructions how to replace the mixer inline filter. Check the inlet filters. They can be clogged if unfiltered buffers or samples are applied. To replace the filters, see Section 7.8.8 Replace the inlet filters, on page 328. Check the column. It can be clogged if unfiltered buffers or samples are applied. To clean a column, see Section 7.6.3 Perform Column CIP, on page 281.

8.4 Troubleshooting: Valves

General

The following table lists the general problems that may occur for the different valves.

Problem	Possible cause and action
The valve is not found by the instrument	• The cable between the valve and the ICU is not connected Remove the valve and make sure that the cable is connected. See Hardware installation of a module, on page 76. • Wrong Node ID Check the valve Node ID. If necessary, change the Node ID. See Node ID, on page 76.
The internal valve temperature is too high	• The air intake on the rear or on the left side of the instrument is covered Make sure that none of the air intakes on the instrument are covered. • Hot surroundings Decrease the room temperature. Maximum operating temperature is 35°C. • Hardware error Switch off the instrument and wait until the temperature has decreased. Restart the instrument. If this error is recurrent, generate a System error report and contact Service.
The valve is not switching or is switching to wrong position	• Hardware error Generate a System error report and contact Service.
External leakage	• Hardware error Generate a System error report and contact Service.
Internal leakage	• Broken valve Replace the valve. See Section 2.5 Installation of internal modules, on page 76.

Inlet valves

The Inlet valves include Inlet valve V9-IA, V9H-IA, V9-IB, V9H-IB, V9-IAB, V9H-IAB, V9-IX and V9H-IX, as well as Sample inlet valve V9-IS and V9H-IS.

Problem	Possible cause and action
Faulty air sensor in the valve	• Hardware error Restart the instrument with the power switch. If this error is recurrent, generate a System error report and contact Service.

pH valve

Problem	Possible cause and action
Leaking pH valve	• The dummy electrode was dry when it was installed in the valve. 1 Remove the dummy electrode. 2 Wet the dummy electrode properly with distilled water. 3 Insert the dummy electrode into the pH valve. 4 Rotate the dummy electrode before securing it with the nut.

Module Panel

Problem	Possible cause and action
The instrument is unable to find some of the modules	• A Module Panel is missing and the position is left empty Install the missing Module panel. • The cable between the Module Panel and the ICU is not connected Remove the Module Panel and make sure that the cable is connected.

8.5 Troubleshooting: Fraction collector

In this section

- Fraction collector F9-C
- Fraction collector F9-R

Fraction collector F9-C

Problem	Possible cause and action
The fraction collector cannot be found by the instrument	• The cable between the fraction collector and the ÄKTA pure instrument is not connected Generate a System error report and contact Service. • A fuse in the instrument ICU is broken The ICU needs to be changed. Generate a System error report and contact Service.
Fraction collector arm is blocked or internal fault in the fraction collector	• Obstruction inside the fraction collector Switch off the instrument and check for obstruction inside the fraction collector. Try to move the fractionation arm by hand. Switch on the instrument. If this error is recurrent, generate a System error report and contact Service.
The accumulator is jammed or there is an internal error in the instrument	• Salt crystals or protein residuals block the accumulator Restart the instrument and perform an accumulator wash. • Mechanical error If this error is recurrent, generate a System error report and contact Service.
Fraction collection tube or well is overfilled and fractionation movements are lost.	• Too many commands are pending in the fraction collector The reason could be that too many fraction collector instructions have been sent. Wait for a while and try again.

Problem	Possible cause and action
The fraction collector failed to detect the code on the Cassette	• Cassette tray or tube rack is inserted in the wrong direction Take it out and insert it in the correct direction. • Unclean Cassette type code reader Clean the dispenser head and its four diode windows using a cloth and a mild cleaning agent or 20% ethanol. See Section 7.6.4 Clean Fraction collector F9-C, on page 285 for more information. • Unclean Cassette type codes Clean the Cassette type codes. See Section 7.6.4 Clean Fraction collector F9-C, on page 285 for more information. If this error is recurrent, set the Fraction collector configuration manually in UNICORN. In System Control, select System:Settings. Navigate to Fraction collector:Cassette configuration and select Manual.
The Cassette tray is loose in the fraction collector	• The Tray guides in the fractionation chamber are missing Replace the Tray guides. See Section 7.6.4 Clean Fraction collector F9-C, on page 285. • The Tray catch is broken Contact service.
Calibration of the Drop sync sensor failed	• Unclean Drop sync sensor diode windows Clean the Drop sync sensor diode windows. See Section 7.6.4 Clean Fraction collector F9-C, on page 285 for location of the Drop sync sensor diode windows and cleaning instructions. If this error is recurrent, generate a System error report and contact Service.
Drop sync does not work	• Liquid spatter in the fraction collector Change to another type of tubes or deepwell plates or collect fraction volumes of maximum two thirds of the volume of the tubes. Clean the diode windows of the drop sync sensor more frequently than once a week, using a cloth and a mild cleaning agent or 20% ethanol.

Problem	Possible cause and action
The Dispenser head failed to detect a drop	Air in the flow path If this error is recurrent, generate a System error report and contact Service. Check the flow path for air. Fill system and purge pumps according to Section 5.4.1 System pumps, on page 159. Unclean Drop sync sensor diode windows Clean the diode windows of the Drop sync sensor. See Section 7.6.4 Clean Fraction collector F9-C, on page 285. If this error is recurrent, generate a System error report and contact Service. Too high flow rate Decrease the flow rate.
The Dispenser head failed to detect the flow properly and has switched to tube change with reduced accumulator functionality	Air in the flow path Check the flow path for air. Fill system and purge pumps according to Section 5.4.1 System pumps, on page 159. If this error is recurrent, generate a System error report and contact Service. Unclean diode windows in the Drop sync sensor Clean the diode windows of the Drop sync sensor. See Section 7.6.4 Clean Fraction collector F9-C, on page 285. If this error is recurrent, generate a System error report and contact Service.
The Dispenser head failed to detect a drop and has switched to tube change without Drop sync	Too high flow rate Decrease the flow rate. Air in the flow path Check the flow path for air. Fill system and purge pumps according to Section 5.4.1 System pumps, on page 159. If this error is recurrent, generate a System error report and contact Service. Unclean diode windows in the Drop sync sensor Clean the diode windows of the Drop sync sensor. See Section 7.6.4 Clean Fraction collector F9-C, on page 285. If this error is recurrent, generate a System error report and contact Service.
Tubes do not fit in the Cassette	Wrong tube dimensions are used Check that the used tubes have the right dimensions. See Fraction collector tubes and bottles, on page 99 for information about tubes and Cassettes. QuickRelease function is worn out Order a new Cassette. See Chapter 10 for ordering information.

Problem	Possible cause and action
Deep well plate does not fit in the Cassette	• Unsupported deep well plate model Check that the deep well plates are supported. See Deep well plates, on page 100.
The Cassette does not fit the Cassette tray	• The Cassette is turned in the wrong direction See Prepare and insert the Cassette tray, on page 192 for information of how to place the Cassettes. • Objects or dirt under the Cassette Remove the object or dirt.
Cassette tray in wrong position	• The Tray guides in the fractionation chamber are missing Replace the Tray guides. See Section 7.6.4 Clean Fraction collector F9-C, on page 285. • The Cassette tray is facing the wrong direction Make sure that the front of the tray (marked with the GE-logotype) is facing outwards. See Prepare and insert the Cassette tray, on page 192. • Dirt under the Cassette tray Remove the dirt.
The loaded Cassette tray cannot be inserted into the fractionation collector	• The Cassette tray is facing the wrong direction Check that the GE-logotype is facing outwards when the tray is inserted into the fraction collector. • Some of the tubes or plates are incorrectly placed in the Cassettes Check that all tubes and plates are correctly inserted in the Cassettes. See Prepare and insert the Cassette tray, on page 192. • Some of the tubes or plates have the wrong dimensions Check that the deep well plates and the tubes used are of the right type. See Fraction collector tubes and bottles, on page 99 and Deep well plates, on page 100 for information about supported tubes and plates.

Problem	Possible cause and action
Quick scan or Full scan does not work	• The Tray guides in the fractionation chamber are missing Replace the Tray guides. See Section 7.6.4 Clean Fraction collector F9-C, on page 285. • The Cassette tray is facing the wrong direction Check that the GE-logotype is facing outwards. • The Cassette type codes are unclean Clean the the Cassette type codes. • The QuickRelease of a Cassette is in open position Close the Cassette. See Prepare and insert the Cassette tray , on page 192. • The Cassette code reader diode window is unclean Clean the Cassette code reader diode window. See Section 7.6.4 Clean Fraction collector F9-C, on page 285. • The automatic scanning is turned off in UNICORN Make sure that the automatic scanning is turned on in UNICORN software. In System Control, select System:Settings. Navigate to Fraction collector:Cassette configuration and select Automatic. • Wells in deep well plates are prefilled to a volume above 25% of the total well volume Full scan will not work with prefilled wells during these conditions. • Hardware error Generate a System error report and contact Service.
The interior of the fraction collector is dark	• The light has been turned off in UNICORN Turn on the light in UNICORN. In System Control, select System:Settings. Navigate to Fraction collector:Fraction collector lamp and select Lamps On. • The lamp is broken Contact Service.

Problem	Possible cause and action
The waste or the interior of the fraction collector is flooded	• The waste tubing is positioned so that the flow is obstructed Untwist the waste tubing. • The waste container is placed in a position higher than the waste outlet Place the waste container in a position lower than the waste outlet. • The waste tubing is blocked. Clean or replace the waste tubing.
The liquid leaving the nozzle does not strike the waste funnel	• Check the position of the waste funnel Refit the waste funnel.
The tubing in the fraction collector is blocked	• Salt residuals in the tubing Perform a <i>Fraction collector wash</i>, see Section 7.6.4 Clean Fraction collector F9-C, on page 285. If persistent, contact Service.
The fraction volume found in the tubes or wells are smaller than expected	• Leakage on the wet side of the instrument Localize the leakage and take care of the leakage, for example by tightening connectors. • Air in pumps Purge pumps. See Section 5.4.1 System pumps, on page 159. • Bad pump function See troubleshooting of pumps in Section 8.6. • Leakage inside the Frac chamber Contact Service.
Liquid on the floor of the fraction collector	• The fingertight connector on the Dispenser head is not tight enough Tighten the connector. Replace the connector if the leakage is persistent. • The waste tubing or the waste funnel is blocked. Make sure that there is no blockage or clogging and that the waste tubing not is bent. • Leakage in the Frac arm Contact service.

Problem	Possible cause and action
Spillage by the fraction collector during fractionation	• Unclean diode windows in the Drop sync sensor or unclean nozzle Clean the Drop sync diode windows and the nozzle. See Section 7.6.4 Clean Fraction collector F9-C, on page 285. Use the Fraction collector cleaning position. • Too high flow rate during usage of Drop sync Use a flow rate below 2 ml/min. • One or more Cassettes have empty positions Make sure that all Cassette positions contain tubes or plates. • The tubes are flooded Make sure that the fraction volume is adapted to the tube volume. Fraction tubes have not been replaced by empty tubes when the Fraction collector was opened.
It is not possible to fractionate	• The door of the fraction collector is not properly closed Close the door.
The fraction collector fractionates in the wrong well or tube	• Quick scan has not detected the correct Cassette Clean the Cassette type code of the Cassette. See Section 7.6.4 Clean Fraction collector F9-C, on page 285. • Unsupported deep well plate is used. Make sure that approved deep well plates are used. See Deep well plates, on page 100. • Wells in deep well plates are prefilled to a volume above 25% of the total well volume Full scan will not work with prefilled wells during these conditions. • The deep well plate is not correctly positioned in the Cassette See Prepare and insert the Cassette tray, on page 192 for information of how to place the deep well plate. • Dirt on the nozzle or Drop sync sensor diode windows. Dirt may effect where the drops fall. Clean nozzle and Drop sync sensor diode windows. See Section 7.6.4 Clean Fraction collector F9-C, on page 285.
Error message when the door of the fraction collector is opened during a run	• Some parts in a method require that the door of the fraction collector is closed. Do not open the door when the Fractionation indicator is lit.

Problem	Possible cause and action
Fraction collector wash is reported as Completed when it has been aborted.	The Fraction collector wash instruction is aborted when the fraction collector door is opened during state pause. When selecting to continue the run the instruction is reported as Completed, it should state Cancelled. Action: Do not open the door during the Fraction collector wash instruction. If the door has been opened, restart the Fraction collector wash instruction to make sure that the Fraction collector wash has been performed as recommended.
The instrument does not fractionate via the Outlet valve ports	• The Detector - Outlet valve delay volume has been set to zero. 1 In System Control, select System:Settings:Fraction collections:Delay volumes. 2 Correct the Detector - Outlet valve delay volume.
When starting a method run during a manual run, the fraction collector generates an error message indicating that the wrong Cassettes are in place, even though the correct Cassettes are present in the Fraction collector.	Action: End a manual run before starting a method run.
High pressure alarm when collecting fractions with the fraction collector	Action: • Decrease the flow rate or use Outlet valve fractionation, or • replace the following tubing with tubing of larger inner diameter (i.d.) - the tubing between the outlet valve and the fraction collector and - the internal tubing of the fraction collector. Note: Update the delay volume. In the System Control software module, select System:Settings:Tubing and Delay volumes and update the value for Delay volume: Monitor to frac.
Spillage in Fraction collector when the Frac arm is moving from Cassette placed in position 1 and 2 to waste	Action: If possible, place the Cassettes close to waste, i.e., position 5 or 6 during fractionation.

Problem	Possible cause and action
The fractionation starts in the first row again	• The door of the fraction collector has been opened between two runs. When the instrument is in state <i>Ready</i> and the door is opened and closed, the Fraction collector content is reset. If fractionation will continue after the last fraction of the first run, do not open the door of the fraction collector between two runs.
Spillage between fractions	• The combination of high flow rates and liquids with low surface tension might lead to spillage in the Fraction collector. If possible use Cassette positions 5 and 6. Lower the flow rate when using liquids with low surface tension.

Fraction collector F9-R

Problem	Possible cause and action
The fraction collector cannot be found by the instrument	• The cable between the fraction collector and the ÄKTA pure instrument is not connected Make sure that the cable is connected. • Wrong node ID Check the Node ID of the fraction collector. If necessary, change the Node ID. See Section 9.16 Node IDs, on page 501.
The internal temperature of the fraction collector is too high	• Hot surroundings Decrease the room temperature. Maximum operating temperature is 35°C. • Hardware error Switch off the instrument and wait until the temperature has decreased. Restart the instrument. If this error is recurrent, generate a System error report and contact service.

Problem	Possible cause and action
The fraction collector failed to detect a drop and has changed tube without drop sync.	• To high flow rate for drop sync Decrease the flow rate or disable drop sync. • Air in the flow path Check the flow path for air. Fill system and purge pumps. If this error is recurrent, generate a System error report and contact service. • Unclean drop sync sensor Clean the drop sensor photocell located above the tube sensor with a damp cloth. • The tubing is not correctly mounted in the tubing holder nut Check that the tubing is correctly mounted, see Connect tubing to the ÄKTA pure instrument, on page 106.
The tube sensor has not detected a new tube.	• The fraction collector movement is blocked Make sure that the fraction collector can move and is free from obstructions.
The delay queue is full or there is a tube change overload.	• The flow rate is too high Reduce the flow rate. • The fraction volume is too small Collect larger fractions. • Too many fraction collector instructions have been sent Wait for a while and try again.
Fraction numbering does not start at 1 when the fractionation is restarted after a <i>No tube</i> error	Fraction numbering continues from where it was at the time of the <i>No tube</i> error Manually reset the fraction number in the System settings menu.

8.6 Troubleshooting: Pumps

In this section

- Troubleshooting for System pumps and Sample pumps
- Example of pump pressure curves
- Remove persistent air bubbles

Pumps

Problem	Possible cause and action
Liquid is leaking between the pump head and the side panel	• Piston seal or rinsing membrane incorrectly fitted or worn Replace or reinstall the seal or the membrane. For System pumps and Sample pump S9H, see Section 7.8.10 Replace pump piston seals of Pump P9 or P9H, on page 332. For Sample pump S9, see Section 7.8.11 Replace pump piston seals of Pump P9-S, on page 341
Low eluent flow and noise	• Air in pumps Purge the pumps. See Section 5.4 Prime inlets and purge pump heads, on page 158 or Section 5.4.2 Sample pump, on page 165. • Bad piston spring Disassemble the pump head and examine the piston spring. If the spring is corroded, check piston seal and rinse membrane. Make sure that the pump piston rinsing system is always used when working with aqueous buffers containing salt. • Bad pump piston If the piston is damaged, replace it according to Section 7.8.12 Replace pump pistons, on page 348. • Bad pump piston seal Replace the piston seal and rinse membrane according to Section 7.8.10 Replace pump piston seals of Pump P9 or P9H, on page 332 or Section 7.8.11 Replace pump piston seals of Pump P9-S, on page 341.
Leakage around a connector	• Leaking connection and/or crystallized material around a connector Unscrew the connector and check if it is worn or incorrectly fitted. If so, replace the connector. Gently finger tighten the connector.

Problem	Possible cause and action
Erratic pump pressure	• Air trapped in the pump heads • Partially blocked solvent filters • Leaking connections • Piston seal leakage • Check valve malfunction • Piston damaged See Examples of pump pressure curves, on page 387 for examples of pump pressure curves.
The pump is not found by the instrument	• The cable between the system pump and the ICU is not connected. Contact Service. • The cable between the sample pump and the ÄKTA pure instrument is not connected. Connect the cable. • A fuse in the instrument ICU is broken. Contact Service.
The internal temperature of the pump is too high	• The air intake on the rear or on the left side of the instrument is covered Make sure that none of the air intakes on the instrument are covered. • Hot surroundings Decrease the room temperature. Maximum operating temperature is 35°C. • Hardware error Switch off the instrument and wait until the temperature has decreased. Restart the instrument. If this error is recurrent, generate a System error report and contact Service.
High pressure alarm	• The pressure has increased due to increased viscosity The viscosity increases in cold room. Lower the flow when performing runs in a cold room.


Problem	Possible cause and action
High pressure alarm when pressure control is activated	• The parameter selected for pressure control is not the most appropriate one The pressure control is based on either the Pre column pressure or the Delta column pressure. To change the parameter for pressure control, select Pre column pressure or Delta column pressure from the Pressure control drop-down list in the Instruction box of the instruction of interest. • The flow is too high Lower the flow.
Abnormal difference in system pressure compared to pre column pressure	• Clogged inline filter Replace the inline filter, see Section 7.3.2 Replace the inline filter, on page 263.
Internal pump error combined with high pressure	• The flow path is blocked Remove obstructions in the flow path. For example, remove stop plugs and replace constricted tubing.
Internal pump error at normal pressure	• Blocked pump restrictor Contact Service.
Too slow pressure build up when pressure control is active	• Too low I factor in the Pressure control parameters instruction In the Manual Instructions dialog, increase the I factor of the Pressure control parameters instruction.
Too slow pressure build up when using constant pressure flow	• Too low I factor in the Constant pressure flow parameters instruction In the Manual Instructions dialog, increase the I factor of the Constant pressure flow parameters instruction.
Pressure overshoot or oscillating pressure when pressure control is active	• Too high I factor in the Pressure control parameters instruction In the Manual Instructions dialog, decrease the I factor of the Pressure control parameters instruction.
Pressure overshoot or oscillating pressure when using constant pressure flow	• Too high I factor in the Constant pressure flow parameters instruction In the Manual Instructions dialog, decrease the I factor of the Constant pressure flow parameters instruction.

Examples of pump pressure curves

The table below shows some examples of pump system pressure curves obtained when errors have occurred. The examples can be useful in troubleshooting of the system pumps and the sample pump. The system pressure monitor R9 has higher resolution than the other pressure monitors, and is therefore recommended for troubleshooting purposes.


Incident: 30 μ l of air enters pump.

Action: Purge pump. See [Section 5.4 Prime inlets and purge pump heads, on page 158](#). If the problem is persistent, see [Remove persistent air bubbles, on page 389](#).

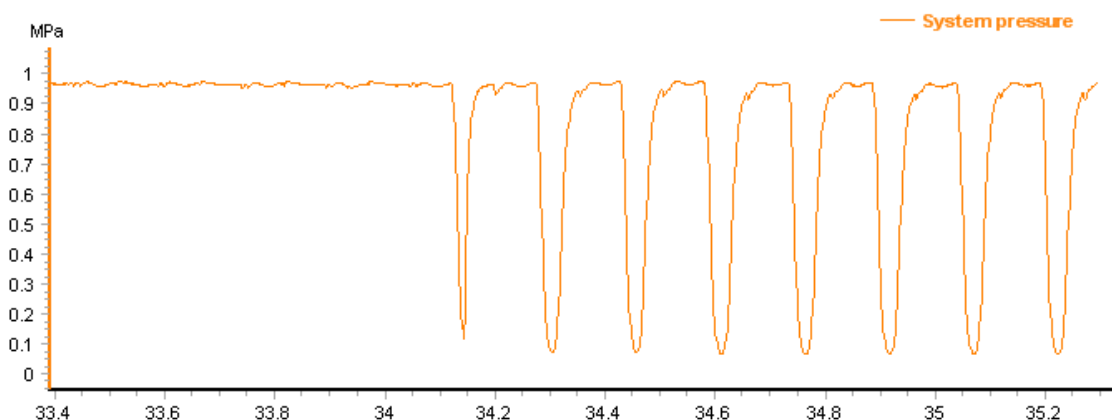


Incident: A large volume of air enters pump.

Action: Purge pump. See [Section 5.4 Prime inlets and purge pump heads, on page 158](#).

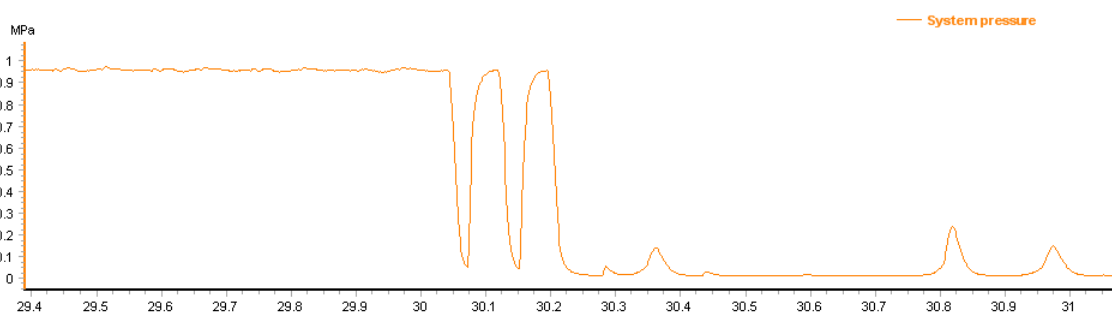


Incident: Blocked outlet check valve

Action: Clean the check valve, See [Section 7.6.8 Clean the pump head check valves, on page 293](#).

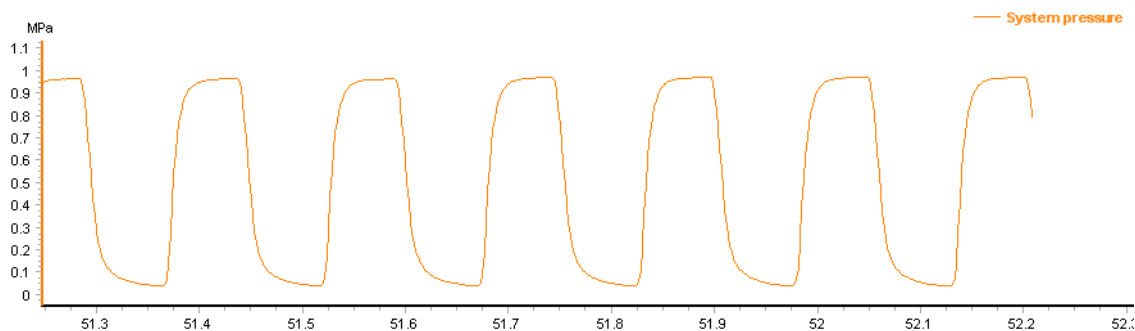


Incident: Inlet check valve is loose.

Action: Tighten the check valve. See [Section 7.8.9 Replace the pump head check valves, on page 329](#).

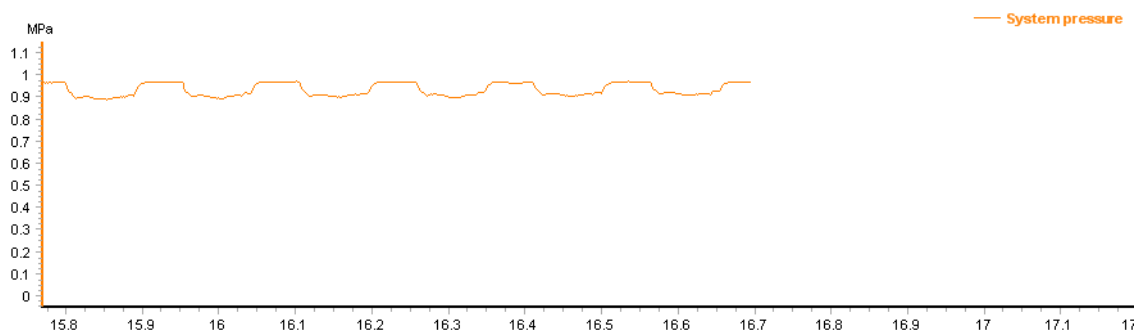


Incident: Leaking inlet check valve.

Action: Replace the check valve. See [Section 7.8.9 Replace the pump head check valves, on page 329](#).

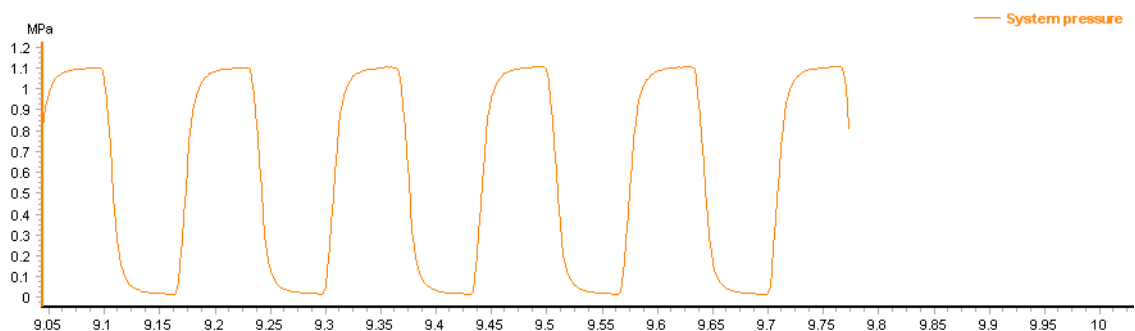


Incident: Leaking outlet check valve.

Actions: Replace the check valve. See [Section 7.8.9 Replace the pump head check valves, on page 329](#).

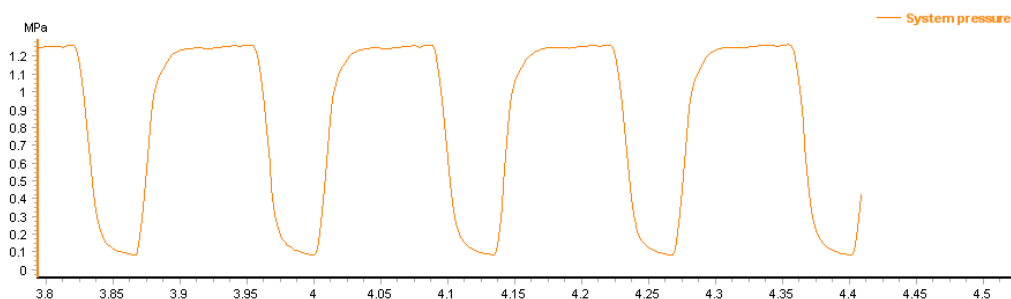

Incident: One inlet is blocked,

Action: Clean inlet tubing. For example, perform a System CIP.

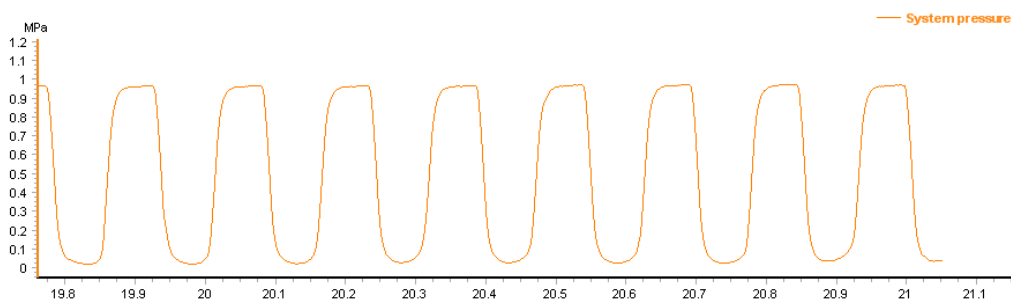

Remove persistent air bubbles

After purging the pump (see [Section 5.4 Prime inlets and purge pump heads, on page 158](#)), check that all air bubbles have been removed by analyzing the pre-column pressure curve (see examples above). If the pressure curve indicates that there are still air bubbles present, repeat the purging process. If the problem persists, follow the instructions below to purge the pump with methanol (see [Section 5.4 Prime inlets and purge pump heads, on page 158](#) for detailed instructions for the purge procedure).

- 1 Make sure that the pump contains water.
- 2 Use a syringe to draw 100% methanol into the pump (see [Section 5.4 Prime inlets and purge pump heads, on page 158](#) for details).
- 3 Set the pump flow to 2.5 ml/min for ÄKTA pure 25 or 10 ml/min for ÄKTA pure 150.
- 4 Let the flow run until the disturbances in the pressure curve disappear.
- 5 Remove the methanol:
 - Stop the pump and move the inlet tubing to water. Make sure that no air is introduced into the system.
 - Set the pump flow to 1 ml/min for ÄKTA pure 25 or 5 ml/min for ÄKTA pure 150.
 - Run for 5 minutes.

- 6 Purge the pump again using an appropriate buffer.
-

8.7 Troubleshooting: Other components

In this section

- General Hardware: All modules
- Mixer
- Superloop
- Cabinet
- Power and ICU
- External air sensors
- I/O-box E9
- Instrument control panel

General hardware: All modules

Problem	Possible cause and action
Modules cannot be found by the instrument	• The cable between a module and the ICU is not connected Remove the module and make sure that the cable is connected. • Two similar modules have been added to the instrument, for example two Inlet valve A Remove one of the modules with the same Node ID. • The Node ID for one or more of the modules is incorrect, for example an Inlet valve A2 has the same Node ID as Inlet valve A. The instrument then considers them to have the same identity. Remove Inlet valve A2 and change the Node ID according to Section 9.16 Node IDs, on page 501.
An unknown instrument module is connected to the system	• The Node ID for one or more of the modules is incorrect Check Node ID and change the Node ID according to Section 9.16 Node IDs, on page 501.

Mixer

Problem	Possible cause and action
Leakage	• Leaking tubing connections Check the tubing connections. Tighten or replace if necessary. Check the O-ring. Replace it if it is damaged. See Section 7.8.4 Replace the O-ring inside the Mixer, on page 320. Check the Mixer chamber. Replace it if the liquid has penetrated the Mixer chamber walls and sealings. See Section 7.8.3 Replace the Mixer, on page 319. See Chapter 10 Ordering information, on page 503.
Unstable gradients	• Bad mixing of eluents Check the function of the Mixer. Place a stirrer bar in the palm of your hand. Hold the hand above the Mixer. The stirrer should move when the Mixer is activated. Check the Mixer chamber size and change chamber if necessary. See Section 7.8.3 Replace the Mixer, on page 319.
Noisy UV signal	• Bad mixing of eluents Check the function of the Mixer. Place a stirrer bar in the palm of your hand. Hold the hand above the Mixer. The stirrer should move when the Mixer is activated. Check the Mixer chamber size and change chamber if necessary, see Select Mixer chamber, on page 149.
The Mixer chamber was not recognized	• The Mixer chamber is not correctly installed Verify that the Mixer chamber is correctly installed. See Section 7.8.3 Replace the Mixer, on page 319. If the error is recurrent, replace the Mixer chamber. See Chapter 10 Ordering information, on page 503.
The internal Mixer temperature is too high	• The air intake on the rear or on the left side of the instrument is covered Make sure that none of the air intakes on the instrument are covered. • Hot surroundings Decrease the room temperature. Maximum operating temperature is 35°C. • Hardware error Switch off the instrument and wait until the temperature has decreased. Restart the instrument. If this error is recurrent, generate a System error report and contact Service.

Superloop


Problem	Possible cause and action
Overpressure during filling	The Superloop is filled to the max. Pressure is not released anywhere. Manually turn Injection valve to Manual load position.

Cabinet

Problem	Possible cause and action
The temperature of the instrument or an instrument component is too high	The air intake on the back or on the left side of the instrument is covered Make sure that none of the air intakes on the instrument are covered. Broken fans Contact Service. Hot surroundings Decrease the room temperature. Maximum operating temperature is 35°C.
Liquid from the Buffer tray is flowing onto the table	The waste tubing from the Buffer tray is loose Contact Service.

Power and ICU

Problem	Possible cause and action
The instrument cannot be turned on	The power cord is not connected Connect the power cord to the wall outlet and to the electrical inlet on the instrument. Make sure that the cord is attached using the clip, thereby preventing the cord from coming loose. No electric current in the wall outlet Make sure that there is electric current in the wall outlet. A fuse in the instrument ICU is broken Contact Service. The instrument is overheated Switch off the instrument and wait until the temperature has decreased. Restart the instrument. If this error is recurrent, generate a System error report and contact Service.

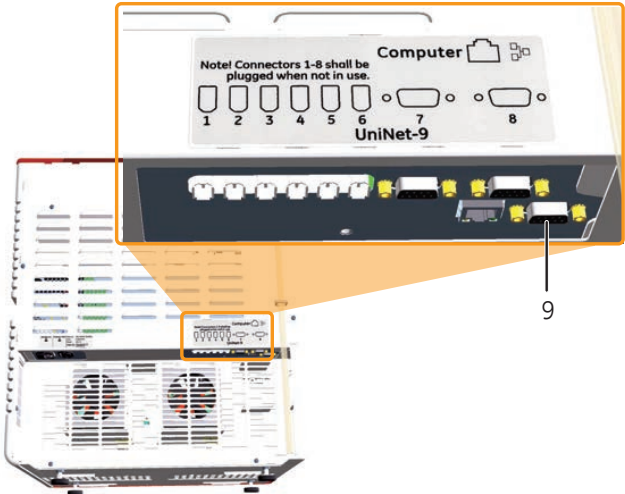Problem	Possible cause and action
One or more modules are automatically turned off	• One or some of the minor modules use too much current. Minor modules include all modules except the Fraction collector, the UV monitor and the pumps. The current is cut off by a temperature sensitive component. The instrument can be restarted when the temperature has decreased. If persistent, generate a System error report and contact Service.
The instrument cannot be seen in UNICORN	• The network cable is not connected Connect the cable, see UNICORN Administration and Technical Manual.
One or more module(s) is not found by the instrument	• The cable between a module and the ICU is not connected. Remove valves and check that cables are connected. • One or more jumpers are loose or missing. Check the connections on the back of the instrument. Empty positions for UniNet-9 connectors 1 to 8 must have connected jumpers. See the illustration below. The connector 9 should be protected with a plastic lid and must never have a jumper connected to it. 

Problem	Possible cause and action
The internal instrument temperature is too high	• The air intake at the rear or on the right side of the instrument is covered Make sure that none of the air intakes on the instrument are covered. • Hot surroundings Decrease the room temperature. Maximum operating temperature is 35°C. • Hardware error Switch off the instrument and wait until the temperature has decreased. Restart the instrument. If this error is recurrent, generate a System error report and contact Service.

External air sensors

Problem	Possible cause and action
The external air sensor is not found by the instrument	• The cable between the external air sensor and the ICU is not connected Check the back of the instrument and make sure that the cable is connected. • The external air sensor has not been selected in UNICORN Select the external air sensor in UNICORN. Refer to the installation instructions delivered together with the external air sensor.
Air is introduced into the flow path	• One of the connections is not tight enough Tighten the connectors.
Liquid is leaking from the external air sensor	• One of the connections is not tight enough Tighten the connectors.
The internal temperature of the air sensor is too high	• Hot surroundings Decrease the room temperature. Maximum operating temperature is 35°C. • Hardware error Switch off the instrument and wait until the temperature has decreased. Restart the instrument. If this error is recurrent, generate a System error report and contact Service.

I/O-box E9

Problem	Possible cause and action
The internal temperature of the I/O-box is too high	• Hot surroundings Decrease the room temperature. Maximum operating temperature is 35 C. • Hardware error
The I/O-box is not detected by the system	• Wrong Node ID Make sure that the Node ID is (00) for the primary box, and (01) for a potential secondary box.
The system does not detect Digital signals correctly	• Cables incorrectly connected Make sure that the cables are connected correctly, earth to earth etc.
Digital In always "0", regardless of input signals	• Digital Out connections switched Check that the digital Out cables are correctly connected, earth to earth etc.
External digital equipment does not respond to set changes in Digital Out	• Cables incorrectly connected Make sure that the cables are connected correctly, earth to earth etc. To isolate the problem: 1 Connect Digital Out (e.g. pin 6) to Digital In (pin 1,2,3, or 4). 2 Change the Digital Out 1 signal between "1" and "0". Verify that Digital out follows. 3 If not: contact Service. If it does: the problem probably lies within the connected equipment.
Analog In does not measure expected voltage	• Auto-zero on the wrong level Reset Auto-zero. • Digital Out connection error Make sure that Digital Out is connected correctly, earth to earth etc.
Noisy analog signal	• Too long cable between the external equipment and E9 Use as short cable as possible. Use shielded cable. Connect the cable shield to the D-sub connector's shield.
Analog In does not measure expected voltage	• Analog In is not calibrated Contact Service.

Problem	Possible cause and action
Analog Out does not generate expected voltage	• Analog Out is not calibrated Contact Service.

Instrument control panel

Problem	Possible cause and action
The internal temperature of the instrument control panel is too high	• The air intake on the rear or on the right side of the instrument is covered. Make sure that none of the air intakes of the instrument are covered. • Hot surroundings Decrease the room temperature. Maximum operating temperature is 35 C. • Hardware error Switch off the instrument and wait until the temperature has decreased. Restart the instrument. If this error is recurrent, generate a System error report and contact Service.

8.8 Troubleshooting: Instrument communication

Scenario	Possible cause and action
Multiple error messages in UNICORN: <i>Lost modules</i>	• A cable to a module (including Module Panels) is not connected Connect the cable: 1 Switch off the instrument. 2 Check all modules and connections. 3 Switch on the instrument. 4 In the displayed dialog in UNICORN, select the option Restart the system only and click OK. • A UniNet-9 connector is not plugged Check that all UniNet-9 connectors that are not in use are plugged.
UNICORN has lost communication with the instrument server	• The UNICORN client has lost connection to the instrument server during a temporary overload of the processor Restart the UNICORN client to regain control. The run continues and no data will be lost.
Warning message in UNICORN: <i>Instrument module is missing</i>	• The module is not functioning properly In the displayed dialog in UNICORN, select the option Restart the system only and click OK. If the problem still remains, replace the module or contact Service.
Warning messages in UNICORN: <i>(Warning) Two instrument modules have the same Node ID</i>	• Two or several modules have the same Node ID Change to correct Node IDs: 1 Switch off the instrument. 2 Check the Node ID for all modules, see Section 9.16 Node IDs, on page 501. 3 Switch on the instrument. 4 In the displayed dialog in UNICORN, select the option Restart the system only and click OK.

Scenario	Possible cause and action
Warning messages in UNICORN: <i>(Warning) Gate (12): Internal instrument error</i>	• One module has an incorrect Node ID Change the Node ID: 1 Switch off the instrument. 2 Check the Node ID for all modules, see Section 9.16 Node IDs, on page 501. 3 Switch on the instrument. 4 In the displayed dialog in UNICORN, select the option Restart the system only and click OK.

8.9 Troubleshooting: Method development

Scenario	Possible cause and action
Phase properties or text instructions are not available in the method editor as expected	• The module required for the instruction has not been enabled in the component selection in the administration module Review the component list. • The wrong system has been selected when creating the new method Make sure that the right system has been selected in the "new method" dialog.
A method has been created for a system that now has a different configuration	• Action: 1 Open the method in the method editor. 2 Select to either adapt the method to the new configuration OR Keep the text method unchanged and manually replace the text instructions that are not available for the new configuration. Refer to Open and save methods for different systems, on page 212 for more information.
An old method is to be transferred to a new system configuration.	• Action: 1 Open the method in the method editor. 2 Save as and select the new system. OR If the configuration is different on the new system, select to either adapt the method to the new configuration or to keep the text method unchanged and manually replace the text instructions that are not available. Refer to Open and save methods for different systems, on page 212 for more information.

8.10 Error codes

Introduction

This section describes the error codes that can appear for the different modules, together with corrective actions.

All modules

Error code	Description	Action
0 - 19	Internal instrument error	Restart the instrument. If recurrent please contact Service.

Instrument control unit

Error code	Description	Action
21 - 69	Internal instrument error	Restart the instrument. If recurrent please contact Service.

Valve

Error code	Description	Action
20, 24	Internal instrument error	Restart the instrument. If recurrent please contact Service.
22	Valve not finding position	Restart the instrument. If recurrent please contact Service.
23	Faulty air sensor	Restart the instrument. If recurrent please contact Service.
25	High temperature	See Section 8.4 Troubleshooting: Valves, on page 372

Pressure monitor

Error code	Description	Action
20, 21, 24-27	Internal instrument error	Restart the instrument. If recurrent please contact Service.
23	High temperature	See Pressure monitors, on page 369 .

Air sensor

Error code	Description	Action
20	High temperature	See External air sensors, on page 395 .

Mixer

Error code	Description	Action
25	Mixer motor error	Restart the instrument. If recurrent please contact Service.
26	Internal instrument error	Restart the instrument. If recurrent please contact Service.
27	High temperature	See Mixer, on page 392

pH monitor

Error code	Description	Action
20, 21	Internal instrument error	Restart the instrument. If recurrent please contact Service.
25	No factory calibration	Contact Service
26	High temperature	See pH monitor and pH valve, on page 367 .

Conductivity monitor

Error code	Description	Action
20-27	Internal instrument error	Restart the instrument. If recurrent please contact Service.
28	High temperature	See Conductivity monitor, on page 364
29	Temperature data error	Restart the instrument. If recurrent please contact Service.
32-34	No factory calibration	Contact Service

Pump

Error code	Description	Action
51-53	Internal pump error	Check that there is no blockage of the pump outlet. Restart the instrument. If recurrent please contact Service.
54	High temperature	See Section 8.6 Troubleshooting: Pumps, on page 384

UV monitor U9-M

Error code	Description	Action
21, 25, 26, 31	Grating error	Restart the instrument. If recurrent please contact Service.
22, 23, 32	Block filter error	Restart the instrument. If recurrent please contact Service.
24	Internal instrument error	Restart the instrument. If recurrent please contact Service.
27	Spectrum calibration error	Restart the instrument. If recurrent please contact Service.
28, 29	Lamp error	Restart the instrument. If recurrent please contact Service.
30	High temperature	See UV monitor U9-M and UV detector unit, on page 357 .

UV detector U9-D

Error code	Description	Action
24, 26, 28, 29, 31, 33	Internal instrument error	Restart the instrument. If recurrent please contact Service.
25	Too low light intensity	Check that the detector and flow cell are fitted correctly. If warning reappears, contact Service.
27	Too high light intensity	Check that the detector and flow cell are fitted correctly. If warning reappears, contact Service.
30	Too high light intensity, R channel	Check that the detector is fitted correctly. If warning reappears, contact Service.

Error code	Description	Action
32	Too high S light intensity, S channel	Check that the flow cell is fitted correctly. If warning reappears, contact Service.
34	No light detected	Check optical pathway and restart the instrument. If recurrent please contact Service.
35	Too low light intensity, R channel	Check that the detector is fitted correctly. If warning reappears, contact Service.
36	Too low light intensity, S channel	No light through flow cell. Check solution absorption and that the cell is fitted correctly.

UV monitor U9-L

Error code	Description	Action
51	High temperature	See UV monitor U9-L, on page 361 .
52, 55	Low lamp intensity	Contact Service.
54	Autozero out of range	Autozero requested when AU value is larger than 2.
58	Too low light intensity, S channel	No light through flow cell. Check solution absorption and that the cell is fitted correctly.
59, 60	Internal instrument error	Restart the instrument. If recurrent please contact Service.
61	Measurement error	Restart the instrument. If recurrent please contact Service.

Fraction collector F9-C

Error code	Description	Action
20 - 22	Internal instrument error.	Restart the fraction collector with the power switch on the ÄKTA pure instrument. If recurrent, generate a system error report and contact service.
32	The fraction collector failed to operate the accumulator.	Restart the fraction collector with the power switch on the ÄKTA pure instrument. If recurrent, generate a system error report and contact service.

Error code	Description	Action
33 - 35, 37 - 40, 55	Fraction collector configuration error.	The instrument restarts. If the error is recurrent, generate a system error report and contact service.
47 - 48	The fraction collector failed to detect the code on the cassette or the type of plate.	Clean the cassette code reader, the cassette type code on the cassette and the plate.
53	Calibration of the dropsync sensor failed.	Clean the Drop sync sensor, see user documentation for the location of the sensor. If this error is recurrent, please contact service.
54	Fraction collector movement is blocked. Either the door is open or there are communication problems.	Close the door of the fraction collector.
57 - 59	Internal fraction collector error.	The instrument restarts. If the error is recurrent, generate a system error report and contact service.
63	Tube change is too fast.	Lower the flow rate or increase the fractionation volume.
68, 72	Fraction collector arm movement is blocked.	The instrument restarts. If the error is recurrent, generate a system error report and contact service.

Fraction collector F9-R

Error code	Description	Action
20	High temperature	See Section 8.5 Troubleshooting: Fraction collector, on page 374
21	Drop sync warning	Clean the sensor and remove air bubbles in the flow path.
22	Tube sensor error	Check that the tube sensor is adjusted properly.
23	Delay queue full	Increase the fraction size. Fraction size must be greater than 1/10 of the delay volume.
24, 26	Internal instrument error	Restart the instrument. If recurrent please contact Service.
25, 28	Too fast tube change	Increase the fraction size or lower the flow rate.

Error code	Description	Action
27	Drop sync error	Clean the drop sensor Error code

Instrument control panel

Error code	Description	Action
51	High temperature	See <i>Instrument control panel, on page 397</i>

I/O-box

Error code	Description	Action
20	High temperature	See section "Troubleshooting"
21	Analog in signal below -2V	Check the external equipment connected to the I/O-box.
22	Analog in signal above 2V	Check the external equipment connected to the I/O-box.
23-28	Internal instrument error	Restart the instrument. If recurrent please contact Service.

9 Reference information

About this chapter

This chapter lists the allowed environmental and operational ranges for ÄKTA pure. Refer to *ÄKTA pure Product Documentation* for detailed technical specifications.

In this chapter

This chapter contains the following sections:

Section	See page
9.1 System specifications	408
9.2 Module specifications	411
9.3 Tubing and connectors	419
9.4 Recommended tubing kits for prepacked columns	427
9.5 Chemical resistance guide	430
9.6 Wetted materials	434
9.7 Predefined methods and phases	436
9.8 System settings	447
9.9 Manual instructions	464
9.10 Available Run data	486
9.11 Available Curves	489
9.12 Injection volumes and peak broadening	491
9.13 Delay volumes	492
9.14 Component volumes	497
9.15 Pressure control	499
9.16 Node IDs	501

9.1 System specifications

System specifications

Parameter	Data
System configuration	Benchtop system, external computer
Control system	UNICORN 6.3 or other compatible version
Connection between PC and instrument	Ethernet
Dimensions (W x D x H)	535 x 470 x 630 mm
Weight (excluding computer)	up to 53 kg
Power supply	100-240 V ~, 50-60 Hz
Power consumption	300 VA (typical) 25 VA (power-save)
Enclosure protective class	IP 21

Parameter	Data
Tubing and connectors	ÄKTA pure 25: • Inlet: FEP tubing, i.d. 1.6 mm, Tubing connector 5/16" + Ferrule (yellow), 1/8" • Pump to Injection valve: PEEK tubing, i.d. 0.75 mm, Fingertight connector, 1/16" • After Injection valve: PEEK tubing, i.d. 0.50 mm, Fingertight connector, 1/16" • Outlet and waste: ETFE tubing, i.d. 1.0 mm, Fingertight connector, 1/16" • Optional tubing kits: i.d. 0.25 mm, i.d. 0.75 mm, i.d. 1.0 mm
	ÄKTA pure 150: • Inlet: FEP tubing, i.d. 2.9 mm, Tubing connector 5/16" + Ferrule (blue), 3/16" • Pump to injection valve: PEEK tubing, i.d. 1.0 mm, 10-32 UNF connections • After Injection valve: PEEK tubing, i.d. 0.75 mm, 10-32 UNF connections • Outlet: FEP, i.d. 1.6 mm, 5/16-24 UNF connections • Waste: ETFE tubing, i.d. 1.0 mm, Fingertight connector, 1/16" • Optional tubing kits: i.d. 0.5 mm, i.d. 1.0 mm

Environmental ranges

Parameter	Data
Storage and transport temperature range	-25°C to +60°C
Chemical environment	Section 9.5 Chemical resistance guide, on page 430

Operating ranges

Parameter	Data
Operating temperature range	4°C to 35°C
Relative humidity	20% to 95%, non-condensing

Equipment noise level

Equipment	Acoustic noise level
ÄKTA pure instrument	< 60 dB A

9.2 Module specifications

Introduction

This section specifies the operating data of the components in ÄKTA pure. For general data for the system see [System specifications, on page 408](#).

System pumps

Parameter	Data
Pump type	Piston pump, metering type
Flow rate range	ÄKTA pure 25: 0.001 to 25 ml/min (up to 50 ml/min during column packing) ÄKTA pure 150: 0.01 to 150 ml/min (up to 300 ml/min during column packing)
Pressure range	ÄKTA pure 25: 0 to 20 MPa (2900 psi) ÄKTA pure 150: 0 to 5 MPa (725 psi)
Viscosity range	ÄKTA pure 25: 0.35 to 10 cP (5 cP above 12.5 ml/min) ÄKTA pure 150: 0.35 to 5 cP
Flow rate specifications	ÄKTA pure 25: - Accuracy: $\pm 1.2\%$ - Precision: RSD < 0.5% (Conditions: 0.25 to 25 ml/min, < 3 MPa, 0.8 to 2 cP) ÄKTA pure 150: - Accuracy: $\pm 1.5\%$ - Precision: RSD < 0.5% (Conditions: 1.0 to 150 ml/min, < 3 MPa, 0.8 to 2 cP)

Sample pump

Parameter	Data
Pump type	Piston pump, metering type
Dimensions (W x D x H)	215 x 370 x 210 mm
Weight	11 kg
Flow rate range	ÄKTA pure 25: 0.001 – 50 ml/min ÄKTA pure 150: 0.01 to 150 ml/min
Pressure range	ÄKTA pure 25: 0 to 10 MPa (1450 psi) ÄKTA pure 150: 0 to 5 MPa (725 psi)
Viscosity range	0.7 – 10 cP
Flow rate specifications	ÄKTA pure 25: - Accuracy: $\pm 2\%$ - Precision: RSD < 0.5% (Conditions: 0.25 – 50 ml/min, < 3 MPa, 0.8 – 3 cP) ÄKTA pure 150: - Accuracy: $\pm 2\%$ - Precision: RSD < 0.5% (Conditions: 1.0 – 150 ml/min, < 3 MPa, 0.8 – 3 cP)

Valves

Parameter	Data
Type	Rotary valves
Number of valves	Up to 12
Functions	Standard: Injection Options: Inlet A, Inlet B, Sample inlet, Extra inlet, Mixer bypass, Loop selection, Column selection, pH, Outlet, Versatile

Inlet options

Parameter	Data
Inlet A	1, 2 or 7 inlets
Inlet B	1, 2 or 7 inlets
Sample inlet	Up to 7 sample inlets and 1 buffer inlet

Outlet options

Parameter	Data
Number of outlets	1 or 10

Mixer

Parameter	Data
Mixing principle	Chamber with magnetic stirrer
Mixer volume	ÄKTA pure 25: 0.6, 1.4 or 5 ml ÄKTA pure 150: 1.4, 5 or 15 ml

Gradient formation

Parameter	Data
Gradient flow rate range	ÄKTA pure 25: 0.1 to 25 ml/min ÄKTA pure 150: 0.5 to 150 ml/min
Gradient composition accuracy	ÄKTA pure 25: ±0.6% (Conditions 5 to 95% B. 0.5 to 25 ml/min, 0.2 to 2 MPa, 0.8 to 2 cP) ÄKTA pure 150: ±0.8% (Conditions 5 to 95% B. 2 to 150 ml/min, 0.2 to 2 MPa, 0.8 to 2 cP)

Pressure monitors

Parameter	Data
Number of sensors	Up to 4
Placement of sensors	Standard: The System pressure monitor is located after the System pump Options: • The Pre-column pressure monitor and the Post-column pressure monitor are integrated in Column valve V9-C or V9H-C. • The Sample pressure monitor is located after the Sample pump.
Range	0 to 20 MPa (2900 psi)
Accuracy	± 0.02 MPa or ± 2% whichever is greater

External air sensor options

Parameter	Data
Number of sensors	Up to 7
Placement	• Integrated in inlet valve A, inlet valve B and sample inlet valve • After the injection valve • Before the system pumps • Before the sample pump
Sensing principle	Ultrasonic

UV monitor options

Parameter	Data
Number of monitors	Up to 2
Wavelength range	U9-L: 280 nm U9-M: 190 to 700 nm in steps of 1 nm, up to 3 wavelengths
Absorbance range	-6 to 6 AU
Resolution	0.001 mAU

Parameter	Data
Linearity	U9-L: within $\pm 5\%$ at 0 to 2 AU U9-M: within $\pm 2\%$ at 0 to 2 AU
Drift	U9-L (2 mm cell): $\leq 0.2 \text{ mAU} \text{ AU/h}$ U9-M (2 mm cell at 280 nm): $\leq 0.2 \text{ mAU} \text{ AU/h}$
Noise	U9-L: $< 0.1 \text{ mAU}$ U9-M: $< 0.08 \text{ mAU}$
Operating pressure	0 to 2 MPa
Flow cells: U9-L	Standard: Optical path length 2 mm Cell volume 2 μl Total volume: 30 μl Option: Optical path length 5 mm Cell volume 6 μl Total volume 20 μl
Flow cells: U9-M	Standard: Optical path length 2 mm Cell volume 2 μl Total volume: 11 μl Option: Optical path length 10 mm Cell volume 8 μl Total volume 12 μl Optical path length 0.5 mm Cell volume 1 μl Total volume 10 μl

Conductivity monitor options

Parameter	Data
Conductivity reading range	0.01 mS/cm to 999.99 mS/cm
Accuracy	$\pm 0.01 \text{ mS/cm}$ or $\pm 2\%$, whichever is greater, (within 0.3 to 300 mS/cm)
Operating pressure	0 to 5 MPa (725 psi)
Flow cell volume	22 μl
Temperature monitor range	0°C to 99°C

Parameter	Data
Temperature monitor accuracy	±1.5°C within 4°C to 45°C

pH monitor option

Parameter	Data
pH reading range	0 to 14
Accuracy	±0.1 pH unit within pH 2 to 12, temperature within ±3°C from calibration temperature
Operating pressure	0 to 0.5 MPa (72 psi)
Flow cell volume	ÄKTA pure 25: 76 µl ÄKTA pure 150: 129 µl

Outlet valve fractionation option

Parameter	Data
Number of outlets	10
Fraction volumes	0.01 to 20 000 ml
Delay volume (UV – outlet valve)	ÄKTA pure 25: 125 µl 66 µl with optional tubing kit (i.d. 0.25 mm) ÄKTA pure 150: 296 µl 245 µl with optional tubing kit (i.d. 0.5 mm)

Fraction collector options

Parameter	Data
Number of fraction collectors	Up to two. The second fraction collector must be an F9-R.
Number of fractions	F9-C: Up to 576 F9-R: Up to 175

Parameter	Data
Vessel types	F9-C: • Deep well plates, 96, 48 or 24 wells • Tubes 3, 5, 8, 15, 50 ml • Bottle, 250 ml F9-R: 3, 8, 15 or 50 ml tubes
Fraction volumes	F9-C: 0.1 to 250 ml F9-R: 0.1 to 50 ml
Spillage-free mode	F9-C: Automatic, Drop sync or Accumulator F9-R: Drop sync
Flammable liquids	F9-C: no F9-R: yes
Delay volume (UV – dispenser head)	ÄKTA pure 25: F9-R: 205 µl, 86 µl with optional tubing kit (i.d. 0.25 mm) F9-C: 435 µl, 214 µl with optional tubing kit (i.d. 0.25 mm) ÄKTA pure 150: F9-R: 473 µl, 278 µl with optional tubing kit (i.d. 0.5 mm) F9-C: 876 µl, 508 µl with optional tubing kit (i.d. 0.5 mm)
Dimensions (W x D x H)	• F9-C: 390 x 585 x 320 mm • F9-R: 320 x 400 x 250 mm
Weight	• F9-C: 21 kg • F9-R: 5 kg

I/O box

Parameter	Data
Number of ports	2 analog in, 2 analog out 4 digital in, 4 digital out
Analog range	In +/- 2 V Out +/- 1 V

9.3 Tubing and connectors

Tubing types

The table below shows the tubing types used in ÄKTA pure.

Description	Color	Scope of use	Volume/cm
PEEK, o.d. 1/16", i.d. 0.25 mm	Blue	High pressure tubing Reference capillary 1 Tubing Kit 0.25	0.5 µl
PEEK, o.d. 1/16", i.d. 0.50 mm	Orange	High pressure tubing Tubing kit 0.5 (standard)	2.0 µl
PEEK, o.d. 1/16", i.d. 0.75 mm	Green	High pressure tubing Tubing kit 0.75	4.4 µl
PEEK, o.d. 1/16", i.d. 1.0 mm	Beige	High pressure tubing Tubing kit 1.0	7.8 µl
FEP, o.d. 1/8", i.d. 1.6 mm	Transparent	Inlet tubing	20.0 µl
FEP, o.d. 3/16", i.d. 2.9 mm	Transparent	Inlet tubing for high flow rate and high viscosity	66.0 µl
ETFE, o.d. 1/16", i.d. 0.75 mm	Transparent	Narrow inlet tubing (op- tional)	4.4 µl
ETFE, o.d. 1/16", i.d. 1.0 mm	Transparent	Outlet and waste tubing	7.8 µl
Silicone, o.d. 12 mm, i.d. 8 mm	Transparent	Waste tubing from Buffer tray	0.3 ml

- Note:**
- Many different sizes/types of tubing can be connected to a chromatography system. Tubing with a smaller inner diameter (i.d.) holds less delay volume and will therefore generate less dilution of the protein peak. Narrow tubing, however, increases the system pressure, especially when running at high flow rates. The tubing used should match the application needs. See [Section 9.4 Recommended tubing kits for prepacked columns, on page 427](#) for more information.
 - When using the high pressure tubing kit with i.d. 1.0 mm to allow high flow rates in combination with high viscosities in the pumps, inlet tubing with a larger i.d. than standard might be needed to avoid outgassing.

Tubing connectors

The table below shows the tubing connectors used in ÄKTA pure.

Description	Use with tubing...
Fingertight connector, 1/16"	• PEEK, o.d. 1/16", i.d. 0.25 mm • PEEK, o.d. 1/16", i.d. 0.50 mm • PEEK, o.d. 1/16", i.d. 0.75 mm • PEEK, o.d. 1/16", i.d. 1.0 mm • ETFE, o.d. 1/16", i.d. 1.0 mm
Tubing connector 5/16" + Ferrule (blue), 1/16"	ETFE, o.d. 1/16", i.d. 0.75 mm
Tubing connector 5/16" + ferrule (blue) 3/16"	FEP o.d. 3/16" i.d. 2.9 mm
Tubing connector 5/16" + Ferrule (yellow), 1/8"	FEP, o.d. 1/8", i.d. 1.6 mm


Other connectors

The table below shows other connectors used in ÄKTA pure.

Description	Scope of use
Stop plug 1/16"	Stop plug for valve ports
Luer female	Syringe connector for pH valve and Injection valve

Tubing labels

The illustration below shows the tubing labels for for a typical system configuration.

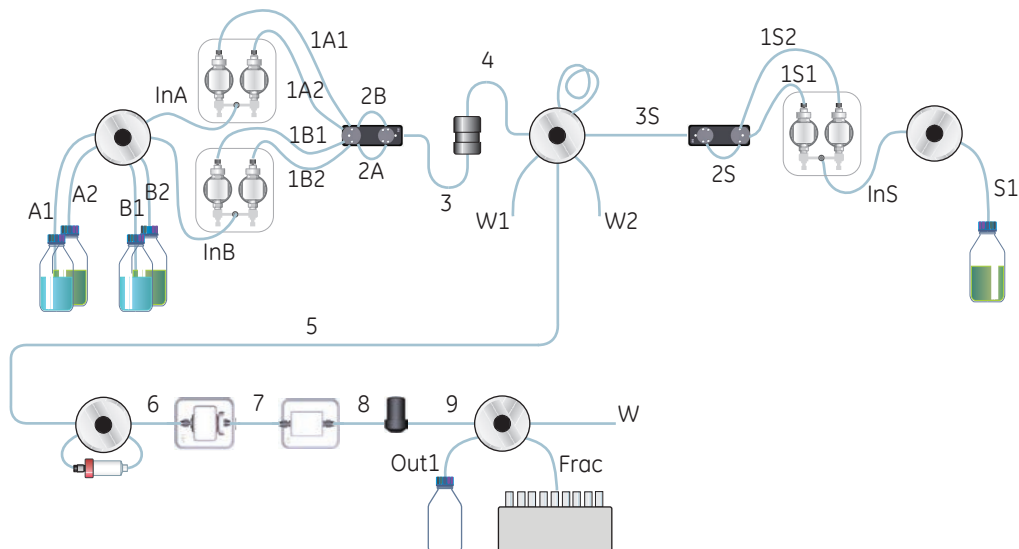

Inlet tubing

The table below shows the labels, standard diameters, and standard lengths of the inlet tubing.

Label	Description	Tubing		Length (mm)	Volume (ml)	
		ÄKTA pure 25	ÄKTA pure 150		ÄKTA pure 25	ÄKTA pure 150
A1-A2 and B1-B2	Inlets to Inlet valve AB	FEP, o.d. 1/8", i.d. 1.6 mm	FEP, o.d. 3/16", i.d. 2.9 mm	1500	3.0	9.9
A1-A7	Inlets to Inlet valve A	FEP, o.d. 1/8", i.d. 1.6 mm	FEP, o.d. 3/16", i.d. 2.9 mm	1500	3.0	9.9
B1-B7	Inlets to Inlet valve B	FEP, o.d. 1/8", i.d. 1.6 mm	FEP, o.d. 3/16", i.d. 2.9 mm	1500	3.0	9.9
InA	From Inlet valve A or Inlet valve AB to System pump A	FEP, o.d. 1/8", i.d. 1.6 mm	FEP, o.d. 3/16", i.d. 2.9 mm	300	0.6	2.0
InB	From Inlet valve B or Inlet valve AB to System pump B	FEP, o.d. 1/8", i.d. 1.6 mm	FEP, o.d. 3/16", i.d. 2.9 mm	300	0.6	2.0

Label	Description	Tubing		Length (mm)	Volume (ml)	
		ÄKTA pure 25	ÄKTA pure 150		ÄKTA pure 25	ÄKTA pure 150
S1-S7	Inlets to Sample inlet valve V9-IS or V9H-IS	FEP, o.d. 1/8", i.d. 1.6 mm	FEP, o.d. 3/16", i.d. 2.9 mm	1000	2.0	6.6
Buff	Inlet to Sample inlet valve V9-IS or V9H-IS	FEP, o.d. 1/8", i.d. 1.6 mm	FEP, o.d. 3/16", i.d. 2.9 mm	1000	2.0	6.6
InS	From Sample inlet valve V9-IS or V9H-IS to Sample pump S9 or S9H, respectively	FEP, o.d. 1/8", i.d. 1.6 mm	FEP, o.d. 3/16", i.d. 2.9 mm	580	1.2	3.8

Note: Narrow inlet tubing, ETFE, o.d. 1/16", i.d. 0.75 mm, is available for **S1-S7**.

High pressure tubing

The tables below shows the labels, standard diameters, and standard lengths of the standard high pressure tubing and the optional high pressure tubing.

Standard high pressure tubing

Label	Description	Tubing		Length (mm)	Volume (µl)	
		ÄKTA pure 25	ÄKTA pure 150		ÄKTA pure 25	ÄKTA pure 150
1A1	System pump A left to Restrictor A	PEEK, o.d. 1/16", i.d. 0.75 mm	PEEK, o.d. 1/16", i.d. 1.0 mm	340	150	270
1A2	System pump A right to Restrictor A	PEEK, o.d. 1/16", i.d. 0.75 mm	PEEK, o.d. 1/16", i.d. 1.0 mm	340	150	270
2A	Restrictor A to Pressure monitor	PEEK, o.d. 1/16", i.d. 0.75 mm	PEEK, o.d. 1/16", i.d. 1.0 mm	115	50	90
1B1	System pump B left to Restrictor B	PEEK, o.d. 1/16", i.d. 0.75 mm	PEEK, o.d. 1/16", i.d. 1.0 mm	340	150	270
1B2	System pump B right to Restrictor B	PEEK, o.d. 1/16", i.d. 0.75 mm	PEEK, o.d. 1/16", i.d. 1.0 mm	340	150	270

Label	Description	Tubing		Length (mm)	Volume (µl)	
		ÄKTA pure 25	ÄKTA pure 150		ÄKTA pure 25	ÄKTA pure 150
2B	Restrictor B to Pressure monitor	PEEK, o.d. 1/16", i.d. 0.75 mm	PEEK, o.d. 1/16", i.d. 1.0 mm	115	50	90
1S1	Sample pump left to Restrictor S	PEEK, o.d. 1/16", i.d. 0.75 mm	PEEK, o.d. 1/16", i.d. 1.0 mm	340	150	270
1S2	Sample pump right to Restrictor S	PEEK, o.d. 1/16", i.d. 0.75 mm	PEEK, o.d. 1/16", i.d. 1.0 mm	340	150	270
2S	Restrictor S to Sample pressure monitor	PEEK, o.d. 1/16", i.d. 0.75 mm	PEEK, o.d. 1/16", i.d. 1.0 mm	115	50	90
3S	Sample pressure monitor to injection valve.	PEEK, o.d. 1/16", i.d. 0.75 mm	PEEK, o.d. 1/16", i.d. 1.0 mm	530	230	420
3	Pressure monitor to Mixer	PEEK, o.d. 1/16", i.d. 0.75 mm	PEEK, o.d. 1/16", i.d. 1.0 mm	400	180	310
4	Mixer to Injection valve	PEEK, o.d. 1/16", i.d. 0.75 mm	PEEK, o.d. 1/16", i.d. 1.0 mm	200	90	160
5	Injection valve to Column valve	PEEK, o.d. 1/16", i.d. 0.50 mm	PEEK, o.d. 1/16", i.d. 0.75 mm	160	30	70
6	Column valve to UV monitor	PEEK, o.d. 1/16", i.d. 0.50 mm	PEEK, o.d. 1/16", i.d. 0.75 mm	160	30	70
7	UV monitor to Conductivity monitor	PEEK, o.d. 1/16", i.d. 0.50 mm	PEEK, o.d. 1/16", i.d. 0.75 mm	170	30	80
8	Conductivity monitor to Flow restrictor	PEEK, o.d. 1/16", i.d. 0.50 mm	PEEK, o.d. 1/16", i.d. 0.75 mm	95	20	40
9	Flow restrictor to Outlet valve	PEEK, o.d. 1/16", i.d. 0.50 mm	PEEK, o.d. 1/16", i.d. 0.75 mm	135	30	60

Label	Description	Tubing		Length (mm)	Volume (µl)	
		ÄKTA pure 25	ÄKTA pure 150		ÄKTA pure 25	ÄKTA pure 150
Frac	Outlet valve to Fraction collector F9-R	PEEK, o.d. 1/16", i.d. 0.50 mm	PEEK, o.d. 1/16", i.d. 0.75 mm	400	180	310
	Outlet valve to Fraction collector F9-C	PEEK, o.d. 1/16", i.d. 0.50 mm	PEEK, o.d. 1/16", i.d. 0.75 mm	350	70	160

Note: Tubing of different inner diameter can be used for tubing **Frac** and tubing **5** to **9**. An inner diameter (i.d.) of 0.5 mm is standard, but tubing kits of 0.25 mm i.d., 0.75 mm i.d. and 1.0 mm i.d. are also available. Tubing **3S** is not included in the kits, but should be changed to 1.0 mm i.d. if the Tubing kit 1.0 is used.

Optional high pressure tubing

Label	Description	Tubing		Length (mm)	Volume (µl)	
		ÄKTA pure 25	ÄKTA pure 150		ÄKTA pure 25	ÄKTA pure 150
3-1	Pressure monitor to Mixer valve	PEEK, o.d. 1/16", i.d. 0.75 mm	PEEK, o.d. 1/16", i.d. 1.0 mm	160	70	130
3-2	Mixer valve to Mixer	PEEK, o.d. 1/16", i.d. 0.75 mm	PEEK, o.d. 1/16", i.d. 1.0 mm	330	150	260
3-3	Mixer valve to Injection valve	PEEK, o.d. 1/16", i.d. 0.75 mm	PEEK, o.d. 1/16", i.d. 1.0 mm	260	120	200
8pH	Conductivity monitor to pH valve	PEEK, o.d. 1/16", i.d. 0.50 mm	PEEK, o.d. 1/16", i.d. 0.75 mm	180	40	80
9pH	pH valve to Outlet valve	PEEK, o.d. 1/16", i.d. 0.50 mm	PEEK, o.d. 1/16", i.d. 0.75 mm	160	30	70
L1	Injection valve port LoopF to Loop valve port F	PEEK, o.d. 1/16", i.d. 0.50 mm	PEEK, o.d. 1/16", i.d. 0.75 mm	160	30	70
L2	Injection valve port LoopE to Loop valve port E	PEEK, o.d. 1/16", i.d. 0.50 mm	PEEK, o.d. 1/16", i.d. 0.75 mm	160	30	70

Label	Description	Tubing		Length (mm)	Volume (µl)	
		ÄKTA pure 25	ÄKTA pure 150		ÄKTA pure 25	ÄKTA pure 150
1R	From pH flow cell to flow restrictor	PEEK, o.d. 1/16", i.d. 0.50 mm	PEEK, o.d. 1/16", i.d. 0.75 mm	80	20	40
2R	From flow restrictor to pH flow cell	PEEK, o.d. 1/16", i.d. 0.50 mm	PEEK, o.d. 1/16", i.d. 0.75 mm	80	20	40

Note: Tubing of different inner diameter can be used for tubing **8pH**, **9pH**, **1R** and **2R**. An inner diameter (i.d.) of 0.5 mm is standard, but tubing kits of 0.25 mm i.d., 0.75 mm i.d. and 1.0 mm i.d. are also available.

Reference capillary

The table below shows the label, diameter, and standard length of the reference capillary. The capillary is used during the System performance tests.

Label	Description	Tubing	Length (mm)	Volume (µl)
Ref 1	Reference capillary	PEEK, o.d. 1/16", i.d. 0.25 mm	400	20

Outlet tubing

The table below shows the labels, diameters, and standard lengths of the outlet tubing. The tubing is not mounted on delivery.

Label	Description	Tubing	Length (mm)	Volume (ml)
Out	Outlets from Outlet valve V9-Os or V9H-Os	ETFE, o.d. 1/16", i.d. 1.0 mm	1500	1.2
Out1 - Out10	Outlets from Outlet valve V9-O or V9H-O	V9-O: ETFE, o.d. 1/16", i.d. 1.0 mm V9H-O: FEP o.d. 1/8", i.d. 1.6 mm	1500	1.2 3.0

Waste tubing

The table below shows the labels, diameters, and standard lengths of the waste tubing. The waste tubing is mounted on delivery.

Label	Description	Tubing	Length (mm)	Volume (ml)
W1	System pump waste	ETFE, o.d. 1/16", i.d. 1.0 mm	1500	1.2

Label	Description	Tubing	Length (mm)	Volume (ml)
W2	Sample pump waste	ETFE, o.d. 1/16", i.d. 1.0 mm	1500	1.2
W3	pH valve waste	ETFE, o.d. 1/16", i.d. 1.0 mm	1500	1.2
W	System waste	ETFE, o.d. 1/16", i.d. 1.0 mm	1500	1.2
N/A	Top tray waste	Silicone, o.d. 12 mm, i.d. 8 mm	1500	80
N/A	Fraction collector F9-C waste	Silicone, o.d. 12 mm, i.d. 8 mm	1350	70

9.4 Recommended tubing kits for prepacked columns

This section specifies recommended tubing kits for prepacked columns used with ÄKTA pure.

Note: Where alternative tubing kits are listed for a given column, the **Pressure control** option may be used instead of changing the tubing kit to adapt to different run conditions. Refer to [Section 9.15 Pressure control, on page 499](#) for details.

Column name	Recommended Tubing Kits		Comments
	Standard system ¹	Advanced system ²	
All HiTrap™ 1 ml (including HisTrap™, GSTrap™, StrepTrap™)	0.5	0.5 with Pressure control or 0.75	
All HiTrap 5 ml (including HisTrap, GSTrap except 4B, StrepTrap)	0.5 or 0.75	0.75	0.75 with Pressure control for maximum flow rate combined with high viscosity.
GSTrap 4B, 5 ml	0.5 or 0.75	0.5 with Pressure control or 0.75	
All HiScreen™	0.5 or 0.75	0.5 with Pressure control or 0.75	
RESOURCE™ Q, S, ETH, ISO, PHE and RPC 1 ml	0.5	0.5	
RESOURCE RPC 3 ml	0.5	0.5	
RESOURCE Q, S 6 ml	0.5 or 0.75	0.75	0.75 with Pressure control for maximum flow rate combined with high viscosity.
SOURCE™ 15RPC ST 4.6/100	0.5	0.5	Avoid combination of column valve V9-C and pH position in valve V9-pH . Resolution may be improved with 0.25.
SOURCE 15Q, S, PHE 4.6/100 PE	0.5	0.5	Avoid combination of column valve V9-C and pH position in valve V9-pH . Resolution may be improved with 0.25.
Mini Q™, Mini S™ 4.6/50 PE	0.25 or 0.5	0.25 or 0.5	Use 0.25 for maximum resolution. Avoid column valve V9-C and pH position in V9-pH .

Column name	Recommended Tubing Kits		Comments
	Standard system ¹	Advanced system ²	
Mono Q™, Mono S™, Mono P™ HR 5/5	0.5	0.5	Avoid combination of column valve V9-C or V9H-C and pH position in valve V9-pH or V9H-pH . Resolution may be improved with 0.25.
Mono P HR 5/20	0.5	0.5	
Mono Q, S HR 10/10	0.5	0.5	
Mono Q, Mono S HR 16/10	0.5 or 0.75	0.5 or 0.75	
Superdex™ Peptide, 75, 200 Superose™ 6, 12 HR 10/30	0.5	0.5	
Mono Q, Mono S 4.6/100 PE	0.5	0.5	Avoid combination of column valve V9-C or V9H-C and pH position in valve V9-pH or V9H-pH . Resolution may be improved with 0.25.
Mono Q, Mono S, Mono P 5/50 GL	0.5	0.5	Avoid combination of column valve V9-C or V9H-C and pH position in valve V9-pH or V9H-pH . Resolution may be improved with 0.25.
Superdex 200 5/150 GL	0.25	0.25	Avoid column valve V9-C and pH position in V9-pH .
Mono P 5/200 GL	0.5	0.5	
Mono Q, Mono S 10/100 GL	0.5 or 0.75	0.5 or 0.75	
Superdex Peptide, 75, 200, Superose 6, 12 10/300 GL	0.5	0.5	
All HiPrep™ 16/10 (including GSTPrep FF, HisPrep FF)	0.5 or 0.75	0.75	
HiPrep 16/60 Sephacryl™ S 100-500 HR	0.5 or 0.75	0.5 with Pressure control or 0.75	
HiPrep 26/10 Desalting HiPrep 26/10 Sepharose™ 6 FF	0.5 with Pressure Control or 0.75	0.75 with Pressure control or 1.0	

Column name	Recommended Tubing Kits		Comments
	Standard system ¹	Advanced system ²	
HiPrep 26/60 Sephacryl S 100-500 HR	0.5 or 0.75	0.5 with Pressure control or 0.75	
HiLoad™ 16/10 Phenyl Sepharose HP, Q Sepharose HP, SP Sepharose HP	0.5 or 0.75	0.5 with Pressure control or 0.75	
HiLoad 16/60 Superdex 30 pg, 75 pg, 200 pg	0.5 or 0.75	0.5 with Pressure control or 0.75	
HiLoad 26/10 Phenyl Sepharose HP, Q Sepharose HP, SP Sepharose HP	0.5 or 0.75	0.75	
HiLoad 26/60 Superdex 30 pg, 75 pg, 200 pg	0.5 or 0.75	0.5 with Pressure control or 0.75	

¹ Standard system configuration.

Normal flow rates.

Moderate sample and buffer viscosities.

² Complex system configuration (for additional tubing, use the same tubing dimension as the Tubing Kit).

Maximum flow rates.

High viscosities (≥3 cP).

9.5 Chemical resistance guide

Introduction

This section specifies the chemical resistance of ÄKTA pure to some of the most commonly used chemicals in liquid chromatography.

Biocompatibility

ÄKTA pure is designed for maximum biocompatibility, with biochemically inert flow paths constructed mainly from titanium, PEEK and highly resistant fluoropolymers and fluoroelastomers. Titanium is used as far as possible to minimize contribution of potentially deactivating metal ions such as iron, nickel and chromium. There is no standard stainless steel in the flow path. Plastics and rubber materials are selected to avoid leakage of monomers, plasticizers or other additives.

Cleaning chemicals

Strong cleaning works well with 2 M sodium hydroxide, 70% acetic acid or the alcohols methanol, ethanol and isopropyl alcohol. Complete system cleaning using 1 M hydrochloric acid should be avoided in order to not damage the pressure sensors. If you are cleaning separation media using 1 M hydrochloric acid, use loop injections of the acid and make sure that the column is not mounted on the column valve **V9-C**. The column valve **V9-C** contains a pressure sensor which can be damaged by 1 M hydrochloric acid.

Long time use of 0.2 M HCl connected to the Quaternary valve as part of a **BufferPro** recipe is acceptable. The solution becomes diluted further down in the system.

If sodium hypochlorite is used as sanitizing agent instead of 2 M sodium hydroxide, use a concentration up to 10%.

Organic solvents

Reversed phase chromatography of proteins works well with 100% acetonitrile and additives trifluoroacetic acid (TFA) up to 0.2% or formic acid up to 5%.

Strong organic solvents like ethyl acetate, 100% acetone or chlorinated organic solvents should be avoided. These might cause swelling of plastic material and reduce the pressure tolerance of PEEK tubing. For this reason, flash chromatography and straight ("normal") phase chromatography is generally not recommended on the system

Assumptions made

The ratings are based on the following assumptions:

- Synergy effects of chemical mixtures have not been taken into account.
- Room temperature and limited overpressure is assumed.

Note: Chemical influences are time and pressure dependent. Unless otherwise stated, all concentrations are 100%.

List of chemicals

Note: A user can be exposed to large volumes of chemical substances over a long time period. Material Safety Data Sheets (MSDS) provide the user with information regarding characteristics, human and environmental risks and preventive measures. Make sure that you have the MSDS available from your chemical distributor and/or databases on the internet.

Aqueous buffers

Continuous use.

Chemical	Concentration	CAS no/EC no
Aqueous buffers pH 2-12	N/A	N/A

Strong chemicals and salts for CIP

Up to 2 h contact time at room temperature.

Chemical	Concentration	CAS no/EC no
Acetic acid	70%	75-05-8/ 200-835-2
Decon™ 90	10%	N/A
Ethanol	100%	75-08-1/ 200-837-3
Methanol	100%	67-56-1/ 200-659-6
Hydrochloric acid ¹	0.1 M	7647-01-0/ 231-595-7
Isopropanol	100%	67-63-0/ 200-661-7
Sodium hydroxide	2 M	1310-73-2/ 215-185-5
Sodium hydroxide/ethanol	1 M/40%	N/A
Sodium chloride	4 M	7647-14-5/ 231-598-3
Sodium hypochlorite	10%	7681-52-9/231-668-3

¹ If hydrochloric acid, HCl, is used as a cleaning agent when columns are connected to the system, the HCl concentration should not exceed 0.1 M in the pressure sensors. Remember that the ÄKTA pure system has pressure sensors in the column valve **V9-C**.

For other parts of the system up to 1 M HCl is acceptable for short periods of use. See [Cleaning chemicals, on page 430](#)

Solubilization and denaturing agents

Continuous use, as additives in separation and purification methods

Chemical	Concentration	CAS no/EC no
Guanidinium hydrochloride	6 M	50-01-1/ 200-002-3

Chemical	Concentration	CAS no/EC no
Sodium dodecyl sulfate (SDS)	1%	151-21-3/ 205-788-1
TRITON™ X-100	1%	9002-93-1
Tween™ 20	1%	9005-64-5/ 500-018-3
Urea	8 M	57-13-6/ 200-315-5

Chemicals used in reversed phase chromatography (RPC)

Continuous use.

Chemical	Concentration	CAS no/EC no
Acetonitrile ¹	100%	75-05-8/ 200-835-2
Acetonitrile/Tetrahydrofuran ¹	85%/15%	109-99-9/ 203-726-8
Acetonitrile/water/Trifluoroacetic acid (TFA) ²	Max 0.2% TFA	N/A
Ethanol	100%	75-08-1/ 200-837-3
Isopropanol	100%	67-63-0/ 200-661-7
Methanol	100%	74-93-1/ 200-659-6
Water/organic mobile phase/formic acid	Max 5% formic acid	N/A

- ¹ Organic solvents can penetrate weaknesses in PEEK tubing walls more easily than water based buffers. Special care should therefore be taken with prolonged use of organic solvents close to pressure limits.

Note: Quaternary valve is not resistant.

Depending on pressure, tubing between pump head and pressure monitor needs to be changed. See [Section 7.8.1 Replace tubing and connectors, on page 314](#) for more information.

- ² Mobile phase system

Note: It is recommended to replace the mixer sealing ring with the highly resistant O-ring (code no 29-0113-26) if the system is to be exposed to organic solvents or high concentrations of organic acids, such as acetic acid and formic acid, for a longer period of time.

Salts and additives for hydrophobic interaction chromatography (HIC)

Continuous use.

Chemical	Concentration	CAS no/EC no
Ammonium chloride	2 M	12125-02-9/ 235-186-4
Ammonium sulfate	3 M	7783-20-2/ 231-984-1
Ethylene glycol	50%	107-21-1/ 203-473-3
Glycerol	50%	56-81-5/ 200-289-5

Reducing agents and other additives

Continuous use.

Chemical	Concentration	CAS no/EC no
Arginine	2 M	74-79-3/ 200-811-1
Benzyl alcohol	2%	100-51-6/ 202-859-9
Dithioerythritol (DTE)	100 mM	3483-12-3 / 222-468-7
Dithiothreitol (DTT)	100 mM	3483-12-3 / 222-468-7
Ethylenediaminetetraacetic acid (EDTA)	100 mM	60-00-4/ 200-449-4
Mercaptoethanol	20 mM	37482-11-4/ 253-523-3
Potassium chloride	4 M	7447-40-7/ 231-211-8

Other substances

Chemical	Concentration	CAS no/EC no
Acetone	10%	67-64-1/ 200-662-2
Ammonia	30%	7664-41-7/ 231-635-3
Dimethyl sulfoxide (DMSO)	5%	67-68-5/ 200-664-3
Ethanol for long-term storage	20%	75-08-1/ 200-837-3
Phosphoric acid	0.1 M	7664-38-2/ 231-633-2

9.6 Wetted materials

Material definitions

The tables below list the materials that come into contact with process fluids in the ÄKTA pure system.

Primary flow path: Material

Material	Abbreviation
Ethylene ChloroTriFluoroEthylene	ECTFE
Ethylene TetraFluoroEthylene	ETFE
Fluorinated Ethylene Propylene	FEP
Fluorinated Propylene Monomer	FPM/FKM
Fully Fluorinated Propylene Monomer	FFPM/FFKM
PolyChloroTriFluoroEthylene	PCTFE
PolyEtherEtherKetone	PEEK
PolyPropylene	PP
PolyTetraFluoroEthylene	PTFE
PolyVinylidene DiFluoride	PVDF
UltraHighMolecularWeightPolyEthylene	UHMWPE
Aluminum oxide	
Elgiloy	
Hastelloy™ C-276	
Quartz glass	
Ruby	
Sapphire	
Titanium grade 2	
Titanium grade 5	

Pump rinse system: Material

Material	Abbreviation
EthylenePropyleneDiene M-class rubber	EPDM
PolyEtherEtherKetone	PEEK
PolyPropylene	PP
PolyPhenylene Sulfide	PPS
PolyVinylidene DiFluoride	PVDF
Silicone	

9.7 Predefined methods and phases

Introduction

A predefined method contains a set of phases, each phase reflecting a specific stage of a chromatography or maintenance run. You can select additional phases from the phase libraries and add these to an existing method, or remove phases that are not required.

The predefined purification methods have default values with suitable running conditions for the chosen column type such as flow and pressure limits. Other settings (e.g., sample application technique, sample volume, elution profile and fractionation) are set on the **Phase Properties** pane in the appropriate phases.

This section describes the predefined methods and phases.

A method is built up by a number of phases. Each phase represents a major process step in the method, for example, equilibration or elution. Predefined methods, that include all the phases necessary to run the system, are available for different chromatography techniques and also for system cleaning.

This sections contains the following subsections:

Section	See page
9.7.1 Predefined purification methods	437
9.7.2 Predefined maintenance methods	443
9.7.3 Predefined phases	445

9.7.1 Predefined purification methods



The **Method Editor** has predefined methods for different separation techniques. The methods include a number of relevant phases.

The table below describes the available predefined purification methods and which phases that are included.

Predefined purification method	Principle	Included phases
<i>Affinity Chromatography (AC)</i>	After equilibration and sample application, the protein of interest is adsorbed to the column ligand. After a wash to remove unbound sample, elution is performed either by using a buffer containing a competitor to displace the protein of interest, or by changing the pH or ionic strength. Finally, the column is re-equilibrated with start buffer.	 <pre> graph TD A[Method Settings] --> B[Equilibration] B --> C[Sample Application] C --> D[Column Wash] D --> E[Elution] E --> F[Equilibration] </pre>

Predefined purification method	Principle	Included phases
Affinity Chromatography (AC) with Tag Removal	After equilibration, the sample of tagged protein is applied. After washing to remove unbound sample the column is equilibrated with cleavage buffer, a protease is applied and the flow is stopped. The cleaved protein and the protease are eluted by starting the flow. The next step regenerates the column, eluting the tag, un-cleaved protein and protease (if tagged). Finally, the column is re-equilibrated. Required components The required components for this method are Inlet valve (2-ports or 7-ports) and Mixer valve, or the sample pump. Required solutions The method phases are pre-configured to use the following solutions in the following inlets and loop: Inlet A1: Equilibration buffer Inlet A2 or sample inlet: Sample Inlet B1: Cleavage buffer Inlet B2: Affinity Regeneration buffer Loop: Protease Note: • Select Inject sample directly onto the column in the sample application phase. • The protease application phase is preconfigured to empty the loop with the protease with a volume of 0.7 ml. The recommended protease volume is 0.7 CV (column volume). If a column volume different than 1 ml is used, this value needs to be changed to correspond to 0.7 CV.	<pre> graph TD A[Method Settings] --> B[Equilibration] B --> C[Sample Application] C --> D[Wash Out Unbound Sample] D --> E[Optional Wash] E --> F[Condition Column with Cleavage Buffer] F --> G[Protease Application] G --> H[Finalize Protease Application] H --> I[Incubation] I --> J[Elution Cleaved Protein] J --> K[Affinity Regeneration] K --> L[Equilibration] </pre>

Predefined purification method	Principle	Included phases
Anion Exchange Chromatography (AIEX)	After equilibration and sample application, negatively charged proteins are adsorbed to the column ligand. After a wash, to remove unbound sample, elution is performed using a gradient of increasing salt concentration (of e.g. NaCl). Finally, the column is washed and re-equilibrated with start buffer.	 <pre> graph TD A[Method Settings] --> B[Equilibration] B --> C[Sample Application] C --> D[Column Wash] D --> E[Elution] E --> F[Column Wash] F --> G[Equilibration] </pre>
Cation Exchange Chromatography (CIEC)	After equilibration and sample application, positively charged proteins are adsorbed to the column ligand. After a wash, to remove unbound sample, elution is performed using a gradient of increasing salt concentration (of e.g. NaCl). Finally, the column is washed and re-equilibrated with start buffer.	 <pre> graph TD A[Method Settings] --> B[Equilibration] B --> C[Sample Application] C --> D[Column Wash] D --> E[Elution] E --> F[Column Wash] F --> G[Equilibration] </pre>
Chromatofocusing (CF)	After equilibration and sample application, elution is performed using a pH gradient. The proteins separate and elute according to their isoelectric points. Finally, the column is re-equilibrated.	 <pre> graph TD A[Method Settings] --> B[Equilibration] B --> C[Sample Application] C --> D[Elution] D --> E[Equilibration] </pre>



Predefined purification method	Principle	Included phases
Desalting	After equilibration and sample application, the proteins are eluted isocratically. This technique is commonly used for buffer exchange.	
Gel filtration (GF)	After equilibration and sample application, proteins separate and elute according to their size (largest first).	
Hydrophobic Interaction Chromatography (HIC)	After equilibration and sample application (use a buffer containing a high salt concentration, for example 2 M ammonium sulfate) hydrophobic proteins are adsorbed to the column ligand. After a wash to remove unbound sample, elution is performed using a gradient of decreasing salt concentration. Finally, the column is washed and re-equilibrated with start buffer.	
Manual Loop Fill	The sample application loops of the loop valve are manually filled with samples. The method will guide the user through the process by pausing and displaying on-screen instructions. Up to five loops can be filled with different samples. The loops are filled in descending order. Partial or complete loop fill can be chosen. Automatic washing of loops and flow path are integrated in the method. The required components for this phase are a column valve and a loop valve.	

Predefined purification method	Principle	Included phases
NHS-coupling	A column packed with NHS-activated Sepharose is washed with 1 mM HCl, followed by immediate application of the protein for covalent coupling onto the column. After incubation the non-bound protein is washed out and the remaining active groups are deactivated with ethanolamine buffer, followed by further washes. Required components The required component for this method is an Inlet valve (2-ports or 7-ports). Required solutions The method phases are preconfigured to use the following solutions in the following inlets and sample loop: Inlet A1: Coupling buffer, for example 0.2 M NaHCO_3 + 0.5 M NaCl pH 8.3. Inlet A2: Activation solution, for example 1 mM HCl Inlet B1: High pH buffer, for example 0.5 M ethanolamine, 0.5 M NaCl pH 8.3 Inlet B2: Low pH buffer, for example 0.1 M Sodium acetate, 0.5 M NaCl pH 4.0 Sample loop: Ligand in coupling buffer Note: <i>The NHS coupling phase is preconfigured to empty the loop with the ligand with a volume of 1 ml. The recommended ligand volume is 1 CV (column volume). If a column volume different than 1 ml is used, this value needs to be changed to correspond to 1 CV.</i>	<pre> graph TD A[Method Settings] --> B[Activation] B --> C[NHS-coupling] C --> D[Finalize NHS-coupling] D --> E[Incubation] E --> F[Optional Wash] F --> G[Wash & Deactivation high pH] G --> H[Wash & Deactivation low pH] H --> I[Wash & Deactivation high pH] I --> J[Wash Incubation] J --> K[Wash & Deactivation low pH] K --> L[Wash & Deactivation high pH] L --> M[Wash & Deactivation low pH] M --> N[Storage Solution] </pre>

Predefined purification method	Principle	Included phases
Reversed Phase Chromatography (RPC)	After equilibration and sample application, hydrophobic proteins adsorb to the column ligand. After a wash to remove unbound sample, elution is performed by generating a gradient of a non-polar, organic solvent such as acetonitrile. Finally, the column is washed and re-equilibrated.	Method Settings Equilibration ▼ Sample Application ▼ Column Wash ▼ Elution ▼ Column Wash ▼ Equilibration

9.7.2 Predefined maintenance methods

A number of predefined methods for preparation and cleaning are available. These maintenance methods are used to prepare the system, clean the system, and to fill the system with storage solution. The table below describes the available predefined maintenance methods.

Predefined maintenance method	Principle	Included phases
Column CIP	The column is filled with a cleaning solution. Select inlet positions. Enter the solution identity, volume, flow rate and incubation time. By adding steps, several cleaning solutions can be used. Suggestions for cleaning steps are available for a number of column types.	
Column Performance Test	After equilibration of the column, sample is injected via a loop and eluted isocratically. A non-adsorbing sample like acetone or salt should be used. After the run, calculate column performance in the Evaluation module. The efficiency of the column is determined in terms of height equivalent to a theoretical plate (HETP), and the peak asymmetry factor (A_s). The result is logged in the column logbook.	
Column Preparation	The column is filled with buffer solution. Select inlet positions. Enter the solution identity, volume, flow rate and incubation time. By adding steps, several preparation solutions can be used.	
Intelligent Packing	Packs AxiChrom™ columns, with a predetermined column type, by motorized power or by a flow of hydraulic liquid that pushes the adaptor down. The user initiates the start of compression at the exact point when the adapter reaches the consolidated bed surface. The adapter compresses the bed according to the packing factor or target bed height as selected. Two Column Performance Test phases (upflow and/or downflow) can be performed after the AxiChrom column has been packed. Only available for some types of AxiChrom columns. Note: <i>Intelligent packing is also available for systems that use wizard generated methods.</i>	

Predefined maintenance method	Principle	Included phases
System CIP	The system is filled with cleaning solution. Select for example inlets, outlets and column positions to be cleaned. Three System CIP phases are included in the method to facilitate the use of three different cleaning solution. Additional System CIP phases can be added from the Phase Library if desired.	 <pre> graph TD MS[Method Settings] --> SC1[System CIP] SC1 --> SC2[System CIP] SC2 --> SC3[System CIP] </pre>
System Preparation	The system is filled with preparation solution. Select for example inlets, outlets and column positions to be prepared. Two System Preparation phases are included in the method. Additional System Preparation phases can be added from the Phase Library if desired.	 <pre> graph TD MS[Method Settings] --> SP1[System Preparation] SP1 --> SP2[System Preparation] </pre>

9.7.3 Predefined phases

The table below describes the predefined phases.


Phase Name	Description
Method Settings	The first, and mandatory, phase in any method. Defines common parameters used in the subsequent phases. The Method Settings phase defines: 1 Column type Note: <i>The Column type list can be filtered in two steps:</i> • Select the chromatography technique to be used in the list Show by technique • Select Show only suggested columns to show the columns that are suggested for the selected chromatography technique. 2 Pressure limit 3 Flow rate 4 Option to control the flow to avoid overpressure Note: <i>Default values for pressure limits and flow rate are given for the selected column type.</i> • Column position • Flow restrictor use • Unit selection for Method base and Flow rate • Monitor settings: - pH monitor - Air sensor alarm settings - UV monitor Note: <i>The first wavelength of U9-M and the fixed wavelength for U9-L or U9-L 2nd is always turned on. The second and third wavelengths for UV monitor U9-M can be set on or off.</i> • Settings for Column Logbook • Start Protocol • Result name and location Note: <i>Some of these options may not be required by certain methods.</i>

Phase Name	Description
<i>Equilibration</i>	Equilibrates the column before purification, or re-equilibrates the column after purification.
<i>Sample Application</i>	Applies sample to the column. Defines the sample application technique, the sample volume, and the handling of flowthrough.
<i>Column Wash</i>	Washes out unbound sample after sample application or removes strongly bound proteins after elution.
<i>Elution</i>	Elutes the sample from the column. Defines parameters for the elution and fractionation settings.
<i>Column Preparation</i>	Prepares the column before use by removing the storage solution and equilibrating the column. By adding steps, several preparation solutions can be used sequentially.
<i>Column CIP</i>	Cleans the column after purification runs by rinsing the column with a cleaning solution to remove nonspecifically bound proteins. By adding steps, several cleaning solutions can be used sequentially.
<i>System Preparation</i>	Prepares the system before a run by removing storage solution and filling the system and inlets with buffer solution. One preparation solution is used per phase.
<i>System CIP</i>	Cleans the system after purification runs by rinsing the system with a cleaning solution. One cleaning solution is used per phase.
<i>Column performance test</i>	Tests the efficiency of a packed column in terms of height equivalent to a theoretical plate (HETP), and the peak asymmetry factor (A_s).
<i>Manual Loop Fill</i>	Is used to manually fill the additional sample application loops mounted on the loop valve. The filling options are: • Partial loop fill • Complete loop fill
<i>Miscellaneous</i>	Can be added to any method at suitable places. The instructions can help the user to better organize the graphical output of the results or introduce a controlled delay in the method run.

9.8 System settings

Introduction

The **System Settings** function is used to set the parameters for the available instructions. The **Edit** dialog in which to edit the system settings are shown below.

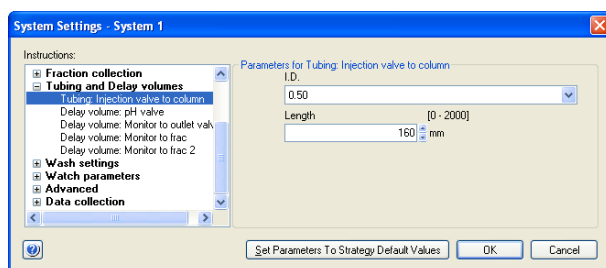

The following subsections list the system settings available for ÄKTA pure.

Section	See page
9.8.1 System settings - UV	448
9.8.2 System settings - Conductivity	449
9.8.3 System settings - pH	450
9.8.4 System settings - Pressure alarms	451
9.8.5 System settings - Air sensor	453
9.8.6 System settings - I/O-box	455
9.8.7 System settings - Fraction collection	456
9.8.8 System settings - Tubing and Delay volumes	458
9.8.9 System settings - Wash settings	460
9.8.10 System settings - Watch parameters	461
9.8.11 System settings - Advanced	462
9.8.12 System settings - Data collection	463

9.8.1 System settings - UV

The table below describes the UV related system settings available for ÄKTA pure.

Instruction name	Description
Alarm UV	Alarm UV enables or disables the alarm for the UV signal. When enabled, it sets the alarm limits for the UV signal from UV monitor U9-L. When the UV signal falls outside the set limits, an alarm will be triggered and the method will be paused.
Alarm UV1	Alarm UV 1 enables or disables the alarm for the UV 1 signal from UV monitor U9-M. When enabled, it sets the alarm limits for the UV 1 signal. When the signal falls outside the set limits, an alarm is issued and the method will be paused. Note: <i>It is not possible to set an alarm signal for the UV 2 or UV 3 signals from UV monitor U9-M.</i>
Alarm UV 2nd	Alarm UV 2nd enables or disables the alarm for the UV signal from U9-L, 2nd. When enabled, it sets the alarm limits for the UV signal from UV monitor U9-L, 2nd. When the signal falls outside the set limits, an alarm will be triggered and the method will be paused.
Wavelength	Wavelength sets the wavelengths for UV monitor U9-M. The corresponding curves in the chromatogram are marked with the set wavelengths. Note: - The instruction is available when UV monitor U9-M (variable) is selected in the component list. For best performance, do not use more wavelengths than necessary for the application. - At low wavelengths, the eluent can have significant absorbance of its own.
Noise reduction UV	Noise reduction UV filters the noise in the UV signal from U9-M or U9-L (depending on the configuration). A column-specific averaging time is set automatically when a column is defined in a method run and Averaging time is set as a variable.
Noise reduction UV 2nd	Noise reduction UV 2nd filters the noise in the UV signal from U9-L, 2nd. A column-specific averaging time is set automatically when a column is defined in a method run and Averaging time is set as a variable.

9.8.2 System settings - Conductivity

The table below describes the conductivity related system settings available for ÄKTA pure.

Instruction name	Description
Alarm conductivity	Alarm conductivity enables or disables the conductivity alarm. When enabled, it sets the alarm limits for the conductivity signal. When the conductivity falls outside the set limits, an alarm will be triggered and the method will be paused.
Relative scale cond	Relative scale cond facilitates monitoring of a gradient, for which the user sets the conductivity values for 0% and 100%. The Relative scale cond can be set in ascending manner (0% for low and 100% for high conductivity) or in descending manner (0% for high and 100% for low conductivity). Note: <i>The Relative scale cond in descending manner is especially useful for conductivity visualization in RPC and HIC, where the conductivity curve is reversed compared to the concentration curve (i.e., high conductivity at 0% B and low conductivity at 100% B).</i>
Cond temp condensation	Cond temp compensation is used to adjust the conductivity values to a reference temperature in order to compare conductivity values between runs that have been performed at different temperatures. Setting the compensation factor to 0% turns this function off.

9.8.3 System settings - pH

The table below describes the pH related system settings available for ÄKTA pure.

Instruction name	Description
Alarm pH	Alarm pH enables or disables the pH alarm. When enabled, it sets the alarm limits for the pH signal. When the pH falls outside the set limits, an alarm will be triggered and the method will be paused.

9.8.4 System settings - Pressure alarms

The table below describes the pressure alarm related system settings available for ÄKTA pure.

Instruction name	Description
Alarm system pressure	Alarm system pressure sets the alarm limits for the system pressure. When enabled and the system pressure falls outside the set pressure limits, an alarm will be triggered and the method will be paused. Default values for the alarm limits are set by the values in the column list when a column is selected in the method and Alarm system pressure is set as a variable. Low alarm is only triggered if the pressure first exceeds the Low alarm limit for ten seconds continuously and then falls below the Low alarm limit. Note: <i>Setting the Low alarm or the system flow rate to 0 deactivates the low pressure alarm.</i>
Alarm sample pressure	Alarm sample pressure sets the alarm limits for the sample pressure. When enabled and the sample pressure falls outside the set pressure limits, an alarm will be triggered and the method will be paused. Default values for the alarm limits are set by the values in the column list when a column is selected in the method and Alarm sample pressure is set as a variable. Low alarm is only triggered if the pressure first exceeds the Low alarm limit for ten seconds continuously and then falls below the Low alarm limit. Note: <i>Setting the Low alarm or the system flow rate to 0 deactivates the low pressure alarm.</i>
Alarm delta column pressure	Alarm delta column pressure sets the alarm limits for the delta column pressure (pre-column pressure minus post-column pressure). When enabled and the delta column pressure falls outside the set pressure limits, an alarm will be triggered and the method will be paused. Low alarm is only triggered if the pressure first exceeds the Low alarm limit for ten seconds continuously then falls below the Low alarm limit. Note: • <i>Setting the Low alarm to 0 deactivates the low pressure alarm.</i> • <i>Instruction Alarm delta column pressure is available only when Column valve V9-C or V9H-C (5-columns) is selected in the component list.</i>

Instruction name	Description
Alarm pre column pressure	Alarm pre column pressure sets the alarm limits for the pre column pressure. When enabled and the pre column pressure falls outside the set pressure limits, an alarm is issued and the method will be paused. Default values for the alarm limits are set by the values in the column list when a column is selected in the method and Alarm pre column pressure is set as a variable. Low alarm is only triggered if the pressure first exceeds the Low alarm limit for ten seconds continuously then falls below the Low alarm limit. Note: <i>Setting the Low alarm to 0 deactivates the low pressure alarm.</i>

9.8.5 System settings - Air sensor

The table below describes the air sensor related system settings available for ÄKTA pure.

Normal (30 µl) is used to detect when a buffer or sample vessel is empty. **High** (10 µl) is used to detect small air bubbles

Instruction name	Description
Alarm inlet A air sensor	Alarm inlet A air sensor enables or disables the air sensor alarm for the built-in air sensor at inlet A. If the alarm is enabled and air is detected, an alarm will be triggered and the method will be paused.
Alarm inlet B air sensor	Alarm inlet B air sensor enables or disables the air sensor alarm for the built-in air sensor at inlet B. If the alarm is enabled and air is detected, an alarm will be triggered and the method will be paused.
Alarm inlet S air sensor	Alarm inlet S air sensor enables or disables the air sensor alarm for the built-in air sensor at the sample inlet. If the alarm is enabled and air is detected, an alarm will be triggered and the method will be paused.
Alarm external air sensor X	Alarm external air sensor X enables or disables the alarm for the optional air sensor number X. If the alarm is enabled and air is detected, an alarm will be triggered and the method will be paused.
Sensitivity inlet A air sensor	Sensitivity inlet A air sensor is used together with the Alarm inlet A air sensor instruction and sets the sensitivity of the built-in air sensors at inlet A. Normal (30 µl) is used to detect when a buffer or sample vessel is empty. High (10 µl) is used to detect small air bubbles
Sensitivity inlet B air sensor	Sensitivity inlet B air sensor is used together with the Alarm inlet B air sensor instruction and sets the sensitivity of the built-in air sensors at inlet B. Normal (30 µl) is used to detect when a buffer or sample vessel is empty. High (10 µl) is used to detect small air bubbles
Sensitivity inlet S air sensor	Sensitivity inlet S air sensor is used together with the Alarm inlet S air sensor instruction and sets the sensitivity of the built-in air sensors at the sample inlet. Normal (30 µl) is used to detect when a buffer or sample vessel is empty. High (10 µl) is used to detect small air bubbles

Instruction name	Description
Sensitivity external air sensor X	Sensitivity external air sensor X is used together with the Alarm external air sensor X instruction and sets the sensitivity of the optional air sensor number X. The optional air sensor can be located either before any of the inlets A or B or after the injection valve. Normal (30 µl) is used to detect when a buffer or sample vessel is empty. High (10 µl) is used to detect small air bubbles - When located before an inlet, the default sensitivity is Normal. - When located after the injection valve, the default sensitivity is High and the pump currently pumping onto the column is used for calculating the air volume for the external air sensor. Note: <i>Using an air sensor after the injection valve is only useful when running at lower pressures. High pressure dissolves any small air bubbles present.</i>

9.8.6 System settings - I/O-box

The table below describes the I/O-box related system settings available for ÄKTA pure.

Instruction name	Description
Digital out X	Digital out X sets the value of the signal sent out by digital port number X to either 0 or 1. The default value is 1.
Noise reduction analog in X	Noise reduction analog in X filters the noise in the analog signal in port number X.
Alarm analog in X	Alarm analog in X enables or disables the alarm for the analog signal in port number X. When enabled, it sets the alarm limits for the analog signal. If the alarm is enabled and the analog signal falls outside the set limits, an alarm will be triggered and the method will be paused.
Alarm digital in X	Alarm digital in X enables or disables the alarm for the signal in digital port number X. The alarm can be triggered by either of the signal values, 0 or 1. If the alarm is enabled and the condition set in 'Value' occurs, an alarm will be triggered and the method will be paused.
Configure analog out X	Configure analog out X enables the user to send one of the pre-defined signals (UV signal, conductivity, temperature, pH or concentration of eluent B) to the analog out port number X, and also to set the range of that signal.

9.8.7 System settings - Fraction collection

The tables below describe the fraction collection related system settings available for ÄKTA pure.
Fraction collector F9-C

Instruction name	Description
Fractionation settings	Fractionation settings comprises fractionation mode and fractionation order. Fractionation mode (<i>Automatic</i> , <i>Accumulator</i> or <i>DropSync</i>). Fractionation order (<i>Row-by-row</i> , <i>Column-by-column</i> , <i>Serpentine-row</i> , <i>Serpentine-column</i>). For fractionation mode DropSync , only the Serpentine option is available.
Last tube filled	Last tube filled : Action when last tube is filled (pause, direct the flow to one of outlets or direct the flow to waste).
Cassette configuration	Cassette configuration : Automatic or Manual configuration. If Automatic is selected, a Quick scan or a Full scan will be performed when the door of the fraction collector is closed to determine which type of cassettes and plates are used. If Manual is selected, used plates and tubes in each tray position are entered.
Fraction collector lamp	Fraction collector lamp : Lamps in the fraction collector chamber on or off.
Peak fractionation parameters	The Peak fractionation parameters set the detection parameters for peak collection, that is they decide when a peak starts and ends. This information is used by the instructions Peak fractionation and Peak frac in outlet valve in order to start/end the peak collection.

Fraction collector F9-R

Instruction name	Description
Fractionation settings	Drop sync synchronises tube change to drop release. The available settings are on or off. It is recommended to use Drop sync for flow rates below 2 ml/min. Higher flow rates can however be used, depending on the properties (for example viscosity) of the liquid.
Fractionation numbering mode	Determines whether the fraction number is reset at the end of a method or not. Note: <i>The default setting is Reset.</i>
Fractionation settings frac 2	Drop sync on or off. It is recommended to use this setting for flow rates below 2 ml/min. Higher flow rates can be however be used, depending on the properties (e.g. viscosity) of the liquid.

Instruction name	Description
Fractionation numbering mode frac 2	Determines whether fraction number for the second fraction collector is reset at the end of a method or not. Note: <i>The default setting is Reset.</i>
Peak fractionation parameters	Peak fractionation parameters sets the detection parameters for peak collection, i.e. it determines when a peak starts and ends. This information is used by the instructions Peak fractionation, Peak fractionation frac 2 and Peak frac in outlet valve in order to start/end the peak collection.

9.8.8 System settings - Tubing and Delay volumes

The table below describes the system settings related to tubing and delay volumes, available for ÄKTA pure.

Instruction name	Description
Tubing: Injection valve to column	The instruction is used in calculations of pre-column pressure when Column valve V9-C or V9H-C (5-columns) is not mounted onto the system. In such cases, there is no pre-column pressure sensor present. The estimated pre-column pressure is either calculated by using the measured system pressure and the length of the tubing between the system pressure sensor and the column valve or by using the measured sample pressure and the length of the tubing between the sample pressure sensor and the column valve depending on the position of the injection valve. The instruction is available only when Column valve V9-C or V9H-C (5-columns) is not selected in the component list.
Tubing: Sample pump to injection valve	The instruction is used in calculations of pre-column pressure when Column valve V9-C or V9H-C (5-columns) is not mounted onto the system. In such cases, there is no pre-column pressure sensor present. The estimated pre-column pressure is either calculated by using the measured system pressure and the length of the tubing between the system pressure sensor and the column valve or by using the measured sample pressure and the length of the tubing between the sample pressure sensor and the column valve depending on the position of the injection valve. The instruction is available only when Column valve V9-C or V9H-C (5-columns) is not selected and a sample pump (S9 or S9H) is selected in the component list.
Delay volume: pH valve	Delay volume: pH valve is used to calculate the delay volume between the monitor and the Outlet valve. The instruction is used to make sure that the collected fractions correspond to the fractions indicated in the chromatogram. It is recommended not to alter the default values for restrictor and pH cell delay volumes when standard modules and standard tubing for flow restrictor are used.
Delay volume: Monitor to outlet valve	Delay volume: Monitor to outlet valve is used to define the delay volume between the monitor and the Outlet valve. The instruction is used to make sure that the collected fractions correspond to the fractions indicated in the chromatogram. The delay volume must be changed when changing tubing to another I.D. or length or when removing or adding components.

Instruction name	Description
Delay volume: Monitor to frac	Delay volume: Monitor to frac is used to define the delay volume between the monitor and the Fraction collector. The instruction is used to make sure that the collected fractions correspond to the fractions indicated in the chromatogram. The instruction is available only when the Fraction collector is selected in the component list.
Delay volume: Monitor to frac 2	Delay volume: Monitor to frac 2 is used to define the delay volume between the monitor and the second Fraction collector. The instruction is used to make sure that the collected fractions correspond to the fractions indicated in the chromatogram. The instruction is available only when the second Fraction collector is selected in the component list.

9.8.9 System settings - Wash settings

The table below describes the wash related system settings available for ÄKTA pure.

Instruction name	Description
System wash settings	System wash settings sets the flow rate used for System wash. Note: - The volume for system wash is set in the System wash instruction. - The flow rate should not exceed 10 ml/min if narrow inlet tubing (i.d. 0.75 mm) is used. - Adjust the flow rate during the system wash so that the system pressure does not exceed 2 MPa.
System pump wash settings	System pump wash settings sets the flow rate and the wash volume used during system pump washes. Note: The flow rate should not exceed 10 ml/min if narrow inlet tubing (i.d. 0.75 mm) is used.
Sample pump wash settings	Sample pump wash settings sets the flow rate and the wash volume used during sample pump washes. Note: The flow rate should not exceed 10 ml/min if narrow inlet tubing (i.d. 0.75 mm) is used.
Fraction collector wash settings	Fraction collector wash settings sets the flow rate during Fraction collector wash.
Mixer by-pass wash settings	Mixer by-pass wash settings sets the flow rate used during Mixer by-pass wash and defines wash volumes for mixer by-pass wash options. Note: The flow rate should not exceed 10 ml/min if narrow inlet tubing (i.d. 0.75 mm) is used.
Loop wash settings	Loop wash settings sets the flow rate used during Loop wash. Note: - The volume for system wash is set in the Loop wash instruction. - The flow rate should not exceed 10 ml/min if narrow inlet tubing (i.d. 0.75 mm) is used.

9.8.10 System settings - Watch parameters

The table below describes the watch parameter settings available for ÄKTA pure.

Instruction name	Description
Watch UV parameters	Watch UV parameters sets the accepted signal fluctuation and Delta peak limit of the UV signal for some of the tests in the Watch and Hold until instructions.
Watch UV 2nd parameters	Watch UV 2nd parameters sets the accepted signal fluctuation and Delta peak limit of the UV 2nd signal for some of the tests in the Watch and Hold until instructions.
Watch cond parameters	Watch cond parameters sets the accepted fluctuation and Delta peak limit of the conductivity signal for some of the tests in the Watch and Hold until instructions.
Watch pH parameters	Watch pH parameters sets the value for the accepted fluctuation of the pH signal used for the test Stable signal in the instructions Watch and Hold until .
Watch flow parameters	Watch flow parameters sets the value for the accepted fluctuation of the flow rate signal used for the test Stable signal in the instructions Watch and Hold until with signal System flow .
Watch pressure parameters	Watch pressure parameters sets the value for the accepted fluctuation of the pressure signals used for the test Stable signal in the instructions Watch and Hold until .
Watch analog in parameters	Watch analog in parameters sets the accepted signal fluctuation and Delta peak limit of the analog signal for some of the tests in the Watch and Hold until instructions.

9.8.11 System settings - Advanced

The table below describes the advanced system settings available for ÄKTA pure.

Instruction name	Description
Power-save	Power-save sets the instrument into power saving mode. When the function is enabled, the instrument enters power-saving mode after having been in state Ready for a certain time period. The instrument turns into state Ready when a method run, a method queue or a manual run ends. The time interval before the instrument enters power-saving mode is defined by the user.
Instrument control panel	Instrument control panel locks/unlocks the control panel located on the front side of the instrument. When unlocked, the buttons on the Instrument control panel are active and can be used to control a few basic functions of the instrument. When the Instrument control panel is locked, no functions are available.
Pressure control parameters	By using Pressure control the method can be run with the set flow rate without the risk of method stop due to pressure alarm. Pressure control is enabled in the instruction System flow or Sample flow . Pressure control parameters provides the P and I factors used in the regulator and can be adjusted for different columns.
Constant pressure flow parameters	Constant pressure flow parameters sets the values for the P and I factors needed to keep a constant pressure by varying the flow rate. The signal used for pressure control is set in the instruction Constant pressure flow .
Max flow during valve turn	Max flow during valve turn sets the maximum flow rate used during the turning of the injection and outlet valve in order to avoid high pressure alarms.
Method progressing flow	Method progressing flow sets which flow (automatic, system flow, sample flow) the progress of the method is calculated after. In automatic mode, the position of the injection valve determines if the system flow or the sample flow is used.
Sample pump setting	Sample pump setting enables sample pump flow while the injection valve is in manual load position.

9.8.12 System settings - Data collection

The table below describes the Data collection related system settings available for ÄKTA pure.

Instruction name	Description
Data collection	The Data collection settings determine the maximum number of data points collected for a given curve. Data reduction occurs if the maximum number of data points is exceeded. To avoid data reduction, set the maximum number of data points to be collected to 180000 or insert a New Chromatogram instruction in the method. Note: <i>The default setting is 54000 data points, which corresponds to 1.5 h for a signal of 10 Hz.</i>

9.9 Manual instructions

It is possible to manually interact with an ongoing method using **Manual instructions**.

Step	Action
1	In the System Control module: - select Manual:Execute Manual Instructions - or - use the shortcut Ctrl +M. <i>Result:</i> The Manual instructions dialog opens.
2	In the Manual instructions dialog: - Click the + symbol to show the instructions for the instruction group that you want to modify. - Select the instruction that you want to modify. - Enter the new values for the instruction.
3	To execute several instructions at the same breakpoint, select and edit an instruction and click Insert . Repeat for several instructions.
4	To update parameter fields during method run, check the Auto update... box.
5	To perform the instructions, click Execute .

All available manual instructions are described in the following subsections.

Section	See page
9.9.1 Manual instructions - Pumps	465
9.9.2 Manual instructions - Flow path	469
9.9.3 Manual instructions - Monitors	471
9.9.4 Manual instructions - Fraction collection	472
9.9.5 Manual instructions - I/O-box	476
9.9.6 Manual instructions - Alarms	477
9.9.7 Manual instructions - Wash settings	480
9.9.8 Manual instructions - Watch parameters	481
9.9.9 Manual instructions - Advanced	482
9.9.10 Manual instructions - Other	485

9.9.1 Manual instructions - Pumps

The table below describes the pump related manual instructions available for ÄKTA pure.

Instruction name	Description
System flow	System flow defines the system flow rate. Flow rate can be set either as volumetric or as linear flow. A column type must be selected before using linear flow.
Sample flow	Sample flow defines the system flow rate. Flow rate can be set either as volumetric or as linear flow. A column type must be selected before using linear flow.
Gradient	Gradient sets a gradient (linear or stepwise) using the system pumps A and B. Note: <i>Set gradient length value to 0 to perform a step gradient.</i>
Pump A wash	Pump A wash is used to change buffers in the inlet tubing, pump and mixer. Note: - Pressing End during Pump wash will terminate both the wash and the run immediately. - Pressing Continue during Pump wash will terminate the wash and the run will continue from the point at which the pump wash instruction was executed. - An instruction issued when a Pump wash is in progress will not be executed until the wash is completely finished and all valves have turned back to the previous positions. Pump wash cannot be executed when the system is in state HOLD.

Instruction name	Description
Pump B wash	Pump B wash is used to change buffers in the inlet tubing, pump and mixer. Note: - Pressing End during Pump wash will terminate both the wash and the run immediately. - Pressing Continue during Pump wash will terminate the wash and the run will continue from the point at which the Pump wash instruction was executed. - An instruction issued when a Pump wash is in progress will not be executed until the wash is completely finished and all valves have turned back to the previous positions. Pump wash cannot be executed when the system is in state HOLD.
Sample pump wash	Sample pump wash is used to change buffers in the sample inlet tubing and sample pump. Note: - Pressing End during Sample pump wash will terminate both the wash and the run immediately. - Pressing Continue during Sample pump wash will terminate the wash and the run will continue from the point at which the Sample pump wash instruction was executed. - An instruction issued when a Sample pump wash is in progress will not be executed until the wash is completely finished and all valves have turned back to the previous positions. Sample pump wash cannot be executed when the system is in state HOLD. - The flow rate should not exceed 10 ml/min if narrow inlet tubing (I.D. 0.75 mm) is used.

Instruction name	Description
Mixer by-pass wash	Mixer by-pass wash is used to wash or fill the flow path (mixer valve and tubing) that is used for sample application with system pump. It is possible to choose a more extensive or a less extensive wash option. Note: - Pressing End during Mixer by-pass wash will terminate both the wash and the run immediately. - Pressing Continue during Mixer by-pass wash will terminate the wash and the run will continue from the point at which the Mixer by-pass wash instruction was executed. - An instruction issued during a Mixer by-pass wash will not be executed until the wash is completely finished and the valves have turned back to the previous positions. Mixer by-pass wash cannot be executed when the system is in state HOLD.
Loop wash	Loop wash is used to wash the Loop valve. It is possible to wash a single sample application loop, all loops or only the by-pass position. Loop wash instruction is not available, if a Column valve is not mounted on the system. Note: - Pressing End during Loop wash will terminate both the wash and the run immediately. - Pressing Continue during Loop wash will terminate the wash and the run will continue from the point at which the Loop wash instruction was executed. - An instruction issued when a Loop wash is in progress will not be executed until the wash is completely finished and the valves have turned back to the previous positions. Loop wash cannot be executed when the system is in state HOLD.

Instruction name	Description
System wash	System wash is used to fill the system with the selected buffer composition. The flow can be directed to the waste position of either the injection valve or the outlet valve. The flow is directed to the end of the flow path if outlet valve is not present. Note: - Pressing End during System wash will terminate both the wash and the run immediately. - Pressing Continue during System wash will terminate the wash and the run will continue from the point at which the System wash instruction was executed. - If System wash is performed during a Gradient operation, the current component B concentration is maintained during the wash. - An instruction issued during a system wash operation cannot be executed until the wash is completely finished and all valves have turned back to the previous positions. System wash cannot be executed when the system is in state HOLD. - Adjust the flow rate during the system wash so that the system pressure does not exceed 2 MPa.

9.9.2 Manual instructions - Flow path

The table below describes the flow path related manual instructions available for ÄKTA pure.

Instruction name	Description
Inlet A	Inlet A turns Inlet valve A to the selected position. Note: <i>Positions A1 - A7 are available, if Inlet valve V9-IA or V9H-IA (7-ports) is used. Only positions A1 and A2 are available, if Inlet valve V9-IAB or V9H-IAB (2-ports) is used.</i>
Inlet B	Inlet B turns the Inlet valve B to the selected position. Note: <i>Positions B1 - B7 are available, if Inlet valve V9-IB or V9H-IB (7-ports) is used. Only positions B1 and B2 are available, if Inlet valve V9-IAB or V9H-IAB (2-ports) is used.</i>
Sample inlet	Sample inlet turns the Sample inlet valve to the selected position.
Injection valve	Injection valve sets the Injection valve to the selected position. The instruction gives an injection mark in the chromatogram when the inlet valve switches to Inject or Direct Inject. Note: <i>Sample flow refers to the flow that enters the injection valve via SaP port.</i>
Column position	Column position turns the Column valve to the position specified in the parameter Position.
pH valve	pH valve sets the pH cell and the 0.2 MPa restrictor in positions inline or offline. The pH valve also has a calibration position. This position is only available when performing calibration of the pH monitor (In System control select System:Calibrate).The calibration position can also be used to fill the pH cell with storage solution since the pH valve is in open position. Note: • <i>It is not possible to turn the pH valve during any type of fractionation as it affects the delay volume.</i> • <i>The pH valve instruction can be given during the delay volume of the different stop fractionation instructions, but it is executed only after the set delay volume has been collected.</i>
Outlet valve	Outlet valve turns the Outlet valve to the selected position. The instruction gives a mark in the chromatogram when the valve is switched to the selected position.

Instruction name	Description
Loop valve	Loop valve turns the Loop valve to the selected position.
Mixer valve	Mixer valve turns the Mixer valve to the selected position. Note: <i>Setting Mixer valve in by-pass position makes it possible to use System pump A for direct loading of the sample onto the column.</i>
Versatile valve X	Versatile valve X turns the Versatile valve number X to the selected position. Note: <i>Four sets of positions are available. In positions 1-3 and 2-4 only a single flow channel can be used. In positions 1-4 & 2-3 and 1-2 & 3-4 the flow can be directed through two channels simultaneously.</i>
Inlet valve (X1)	Instruction Inlet valve X1 turns the extra valve to the selected position. The extra valve is a basic 8 port valve, without air sensor, to be used for general applications.
Inlet valve (X2)	Instruction Inlet valve X2 turns the extra valve to the selected position. The extra valve is a basic 8 port valve, without air sensor, to be used for general applications.
Injection mark	Injection mark sets an injection mark in the chromatogram at the point where this instruction is executed. Note: <i>The instruction is useful when the sample is loaded onto the column by the system pump.</i>

9.9.3 Manual instructions - Monitors

The table below describes the monitor related manual instructions available for ÄKTA pure.

Instruction name	Description
Auto zero UV	Auto zero UV sets the UV signals from U9-M or U9-L to 0 mAU.
Auto zero UV 2nd	Auto zero UV 2nd sets the UV signal from UL-9, 2nd to 0 mAU.
Wavelength	Wavelength sets the wavelengths for UV monitor U9-M. The corresponding curves in the chromatogram are marked with the set wavelengths. Note: - The instruction is available when UV monitor U9-M (variable) is selected in the component list. For best performance, do not use more wavelengths than necessary for the application. - At low wavelengths, the eluent can have absorbance of its own.
Noise reduction UV	Noise reduction UV filters the noise in the UV signal from UV monitor U9-M or U9-L. A column-specific averaging time is set automatically when a column is defined in a method run and Averaging time is set as a variable.
Noise reduction UV 2nd	Noise reduction UV 2nd filters the noise in the UV monitor signal from U9-L, 2nd. A column-specific averaging time is set automatically when a column is defined in a method run and Averaging time is set as a variable.
Relative scale cond	Relative scale cond facilitates monitoring of a gradient, for which the user sets the conductivity values for 0% and 100%. The Relative scale cond can be set in ascending manner (0% for low and 100% for high conductivity) or in descending manner (0% for high and 100% for low conductivity). Note: The Relative scale cond in descending manner is especially useful for conductivity visualization in RPC and HIC, where the conductivity curve is reversed compared to the concentration curve (i.e., high conductivity at 0% B and low conductivity at 100% B).

9.9.4 Manual instructions - Fraction collection

The table below describes the fraction collection related manual instructions available for ÄKTA pure.

Instruction name	Description
Fractionation	Fractionation is used when collecting fractions with a fraction collector.
Stop fractionation	Stop fractionation ends the fractionation after the set delay volume (specified in System Settings:Tubing and Delay volumes) has been collected. The outlet valve is then turned to position Waste. Note: <i>If Stop fractionation is issued when both Fractionation and Peak fractionation are active, fractionation is stopped after the set delay volume has been collected. The outlet valve remains in position Frac and peak fractionation continues.</i>
Peak fractionation	Peak fractionation enables collection of only those peaks that fulfill the conditions set in the Peak fractionation parameters instruction.
Stop peak fractionation	Stop peak fractionation ends the peak fractionation after the set delay volume (specified in System Settings:Tubing and Delay volumes) has been collected. The outlet valve is then turned to position Waste .
Last tube filled	Only for Fraction collector F9-C. Last tube filled sets the action to perform after the fraction collector fills the last tube of the run: pause the fractionation, direct the flow to one of the outlet ports of the outlet valve or direct the flow to waste.
Reset frac number	Only for Fraction collector F9-R. Sets fraction numbers to restart from 1. The restart occurs when the instruction is issued. The instruction overrides the continuous numbering mode if Fractionation numbering mode is set to Continue in System Settings .
Feed tube	Fraction collector F9-C: Feed tube moves the fractionation arm to the position specified by the parameter Start position, after the set delay volume has been collected. A fraction mark is given in the chromatogram. Fraction collector F9-R: Feed tube moves the tube rack forward one tube after the set delay volume has been collected and a fraction mark is set. When fractionation or peak fractionation is not ongoing, Feed tube moves the rack instantly and no fraction mark is set.

Instruction name	Description
Fractionation numbering mode	Only for Fraction collector F9-R. Fractionation numbering mode determines whether the fraction number is reset at the end of a method or not. Note: <i>The default setting is Reset.</i>
Fraction collector wash	Only for Fraction collector F9-C. Fraction collector wash is used to wash the fraction collector with the current solution present in the system. The wash flow rate is set in the instruction Wash settings:Fraction collector wash settings and the current inlet positions are used. After the wash, the flow rate and the valve positions automatically go back to their previous settings. Note: <i>Fraction collector wash cannot be executed during any type of fractionation.</i>
Reset tube type	Only for Fraction collector F9-C. Reset tube type resets all the tube types in the fraction collector. Note: <i>It is not allowed to execute the Reset tube type instruction during fractionation.</i>
Frac cleaning position	Only for Fraction collector F9-C. Frac cleaning position enables manual cleaning of the dispenser head. The system is paused and the fractionation arm is moved to the middle front of the interior of the fraction collector. It is then possible to open the door of the fraction collector and manually clean the dispenser head. Note: <i>The Frac cleaning position instruction cannot be executed during fractionation.</i>
Fraction collector lamp	Only for Fraction collector F9-C. Fraction collector lamp turns the light in the fraction collector on or off.
Cassette configuration	Only for Fraction collector F9-C. Cassette configuration is set to either automatic or manual: - Automatic: the fraction collector automatically detects the cassette types present in the fraction collector. - Manual: The fraction collector content is manually set.
Fractionation frac 2	Fractionation frac 2 is used when collecting fractions with the second Fraction collector.

Instruction name	Description
Stop fractionation frac 2	Stop fractionation frac 2 ends the fractionation after the set delay volume for the second Fraction collector (specified in System Settings:Tubing and Delay volumes) has been collected. The outlet valve is then turned to position Waste. Note: <i>If Stop fractionation frac 2 is issued when both Fractionation frac 2 and Peak fractionation frac 2 are active, fractionation is stopped after the set delay volume has been collected. The Outlet valve V9-O or V9H-O remains in position Outlet 10 / Frac 2 (or Outlet 1 if Outlet valve V9-Os is mounted on the instrument) and peak fractionation in the second Fraction collector continues.</i>
Peak fractionation frac 2	Peak fractionation frac 2 enables collection of only those peaks that fulfill the conditions set in the Peak fractionation parameters instruction.
Stop peak fractionation frac 2	Stop peak fractionation frac 2 ends the peak fractionation in second Fraction collector after the set delay volume (specified in System Settings:Tubing and Delay volumes) has been collected. The outlet valve is then turned to position Waste.
Reset frac number frac 2	Sets fraction numbers to restart from 1 for the second Fraction collector. The restart occurs when the instruction is issued. The instruction overrides the continuous numbering mode if Fractionation numbering mode frac 2 is set to Continue in System Settings.
Feed tube frac 2	During fractionation or peak fractionation the instruction Feed tube frac 2 moves the second Fraction collector tube rack forward one tube after the set delay volume has been collected and a fraction mark is set. When fractionation or peak fractionation is not ongoing, Feed tube frac 2 moves the rack instantly and no fraction mark is set.
Fractionation in outlet valve	Applicable if no fraction collector is used. Fractionation in outlet valve enables fractionation via the outlet valve. When the set fraction size/outlet has been collected, the outlet valve turns to the next position. A fraction mark is set in the chromatogram for each new outlet position. If using Outlet valve V9-Os or V9H-Os (1-outlet), only one fraction can be collected via Outlet 1 position.
Stop frac in outlet valve	Applicable if no fraction collector is used. Stop frac in outlet valve ends the fractionation in outlet valve after the set delay volume (specified in System Settings:Tubing and Delay volumes) has been collected. The outlet valve is then turned to position Waste.

Instruction name	Description
Peak frac in outlet valve	Applicable if no fraction collector is used. Peak frac in outlet valve enables collection of only those peaks that fulfill the conditions set in Peak fractionation parameters . When the set fraction size/outlet has been collected, the outlet valve turns to the next position. A fraction mark is set in the chromatogram for each new outlet position. If Outlet valve V9-Os or V9H-Os (1-outlet) is used, only one peak can be collected via Outlet 1 position.
Stop peak frac in outlet valve	Applicable if no fraction collector is used. Stop peak frac in outlet valve ends the peak fractionation in outlet valve after the set delay volume (specified in System Settings:Tubing and Delay volumes) has been collected. The outlet valve is then turned to position Waste .
Peak fractionation parameters	Peak fractionation parameters sets the detection parameters for peak collection, i.e. it determines when a peak starts and ends. This information is used by the instructions Peak fractionation , Peak fractionation frac 2 and Peak frac in outlet valve in order to start/end the peak collection.

9.9.5 Manual instructions - I/O-box

The table below describes the I/O-box related manual instructions available for ÄKTA pure.

Instruction name	Description
Auto zero analog in X	Auto zero analog in X sets the value of the analog signal in the analog port number X to 0 mV.
Reset auto zero analog in X	Reset auto zero analog in X sets the signal in analog port number X to its current value, i.e. the actual voltage in the analog port number X.
Noise reduction analog in X	Noise reduction analog in X filters the noise in the analog signal in port number X.
Digital out X	Digital out X sets the value of the signal sent out by digital port number X to either 0 or 1. The default value is 1.
Pulse digital out X	Pulse digital out X generates a pulsed signal in digital port number X. The signal changes from the initial state (0 or 1) to the opposite state and returns to the initial state after the defined length of time.
Configure analog out X	Configure analog out X enables the user to send one of the pre-defined signals (UV signal, conductivity, temperature, pH or concentration of eluent B) to the analog out port number X, and also to set the range of that signal.

9.9.6 Manual instructions - Alarms

The table below describes the alarm related manual instructions available for ÄKTA pure.

Instruction name	Description
Alarm system pressure	Alarm system pressure sets the alarm limits for the system pressure. When enabled and the system pressure falls outside the set pressure limits, an alarm will be triggered and the method will be paused. Default values for the alarm limits are set by the values in the column list when a column is selected in the method and Alarm system pressure is set as a variable. Low alarm is only triggered if the pressure first exceeds the Low alarm limit for ten seconds continuously and then falls below the Low alarm limit. Note: <i>Setting the Low alarm or the system flow rate to 0 deactivates the low pressure alarm.</i>
Alarm sample pressure	Alarm sample pressure sets the alarm limits for the sample pressure. When enabled and the pressure falls outside the set pressure limits, an alarm will be triggered and the method will be paused. Low alarm is only triggered if the pressure first exceeds the Low alarm limit for ten seconds continuously then falls below the Low alarm limit. Note: <i>Setting the Low alarm to 0 deactivates the low pressure alarm.</i>
Alarm delta column pressure	Alarm delta column pressure sets the alarm limits for the delta column pressure (pre-column pressure minus post-column pressure). When enabled and the delta column pressure falls outside the set pressure limits, an alarm will be triggered and the method will be paused. Low alarm is only triggered if the pressure first exceeds the Low alarm limit for ten seconds continuously then falls below the Low alarm limit. Note: • <i>Setting the Low alarm to 0 deactivates the low pressure alarm.</i> • <i>Instruction Alarm delta column pressure is available only when Column valve V9-C or V9H-C (5-columns) is selected in the component list.</i>

Instruction name	Description
Alarm pre column pressure	Alarm pre column pressure sets the alarm limits for the pre column pressure. When enabled and the pre column pressure falls outside the set pressure limits, an alarm is issued and the method will be paused. Default values for the alarm limits are set by the values in the column list when a column is selected in the method and Alarm pre column pressure is set as a variable. Low alarm is only triggered if the pressure first exceeds the Low alarm limit for ten seconds continuously then falls below the Low alarm limit. Note: <i>Setting the Low alarm to 0 deactivates the low pressure alarm.</i>
Alarm UV	Alarm UV enables or disables the alarm for the UV signal. When enabled, it sets the alarm limits for the UV signal from UV monitor U9-L. When the UV signal falls outside the set limits, an alarm will be triggered and the method will be paused.
Alarm UV1	Alarm UV1 enables or disables the alarm for the UV 1 signal from UV monitor U9-M. When enabled, it sets the alarm limits for the UV 1 signal from UV monitor U9-M. When the UV signal falls outside the set limits, an alarm is issued and the method will be paused. Note: <i>It is not possible to set an alarm signal for the UV 2 or UV 3 signals from UV monitor U9-M.</i>
Alarm UV 2nd	Alarm UV 2nd enables or disables the alarm for the UV signal from UV monitor U9-L, 2nd. When enabled, it sets the alarm limits for the UV signal from U9-L, 2nd. When the UV signal falls outside the set limits, an alarm will be triggered and the method will be paused.
Alarm conductivity	Alarm conductivity enables or disables the conductivity alarm. When enabled, it sets the alarm limits for the conductivity signal. When the conductivity falls outside the set limits, an alarm will be triggered and the method will be paused.
Alarm pH	Alarm pH enables or disables the pH alarm. When enabled, it sets the alarm limits for the pH signal. When the pH falls outside the set limits, an alarm will be triggered and the method will be paused.
Alarm inlet A air sensor	Alarm inlet A air sensor enables or disables the air sensor alarm for the built-in air sensor at inlet A. If the alarm is enabled and air is detected, an alarm will be triggered and the method will be paused.

Instruction name	Description
Alarm inlet B air sensor	Alarm inlet B air sensor enables or disables the air sensor alarm for the built-in air sensor at inlet B. If the alarm is enabled and air is detected, an alarm will be triggered and the method will be paused.
Alarm sample inlet air sensor	Alarm sample inlet air sensor enables or disables the air sensor alarm for the built-in air sensor at the sample inlet. If the alarm is enabled and air is detected, an alarm will be triggered and the method will be paused.
Alarm external air sensor X	Alarm external air sensor X enables or disables the alarm for the optional air sensor number X. If the alarm is enabled and air is detected, an alarm will be triggered and the method will be paused.
Alarm analog in X	Alarm analog in X enables or disables the alarm for the analog signal in port number X. When enabled, it sets the alarm limits for the analog signal. If the alarm is enabled and the analog signal falls outside the set limits, an alarm will be triggered and the method will be paused.
Alarm digital in X	Alarm digital in X enables or disables the alarm for the signal in digital port number X. The alarm can be triggered by either of the signal values, 0 or 1. If the alarm is enabled and the condition set in 'Value' occurs, an alarm will be triggered and the method will be paused.

9.9.7 Manual instructions - Wash settings

The table below describes the wash related manual instructions available for ÄKTA pure.

Instruction name	Description
System wash settings	System wash settings sets the flow rate used for System wash. Note: - The volume for system wash is set in the System wash instruction. - The flow rate should not exceed 10 ml/min if narrow inlet tubing (I.D. 0.75 mm) is used. - Adjust the flow rate during the system wash so that the system pressure does not exceed 2 MPa.
System pump wash settings	System pump wash settings sets the flow rate and wash volume used during system pump washes. Note: The flow rate should not exceed 10 ml/min if narrow inlet tubing (I.D. 0.75 mm) is used.
Sample pump wash settings	Sample pump wash settings sets the flow rate and wash volume used during sample pump washes.
Fraction collector wash settings	Fraction collector wash settings sets the flow rate during Fraction collector wash.
Mixer by-pass wash settings	Mixer by-pass wash settings sets the flow rate used during Mixer by-pass wash and defines wash volumes for mixer by-pass wash options. Note: The flow rate should not exceed 10 ml/min if narrow inlet tubing (I.D. 0.75 mm) is used.
Loop wash settings	Loop wash settings sets the flow rate used during Loop wash. Note: - The volume for system wash is set in the Loop wash instruction. - The flow rate should not exceed 10 ml/min if narrow inlet tubing (I.D. 0.75 mm) is used.

9.9.8 Manual instructions - Watch parameters

The table below describes the watch parameter instructions available for ÄKTA pure.

Instruction name	Description
Watch UV parameters	Watch UV parameters sets the accepted signal fluctuation and Delta peak limit of the UV signal for some of the tests in the Watch and Hold until instructions.
Watch UV 2nd parameters	Watch UV 2nd parameters sets the accepted signal fluctuation and Delta peak limit of the UV 2nd signal for some of the tests in the Watch and Hold until instructions.
Watch cond parameters	Watch cond parameters sets the accepted fluctuation and Delta peak limit of the conductivity signal for some of the tests in the Watch and Hold until instructions.
Watch pH parameters	Watch pH parameters sets the value for the accepted fluctuation of the pH signal used for the test Stable signal in the instructions Watch and Hold until .
Watch flow parameters	Watch flow parameters sets the value for the accepted fluctuation of the flow rate signal used for the test Stable signal in the instructions Watch and Hold until with signal System flow .
Watch pressure parameters	Watch pressure parameters sets the value for the accepted fluctuation of the pressure signals used for the test Stable signal in the instructions Watch and Hold until .
Watch analog in parameters	Watch analog in parameters sets the accepted signal fluctuation and Delta peak limit of the analog signal for some of the tests in the Watch and Hold until instructions.

9.9.9 Manual instructions - Advanced

The table below describes the advanced manual instructions available for ÄKTA pure.

Instruction name	Description
Pressure control parameters	By using Pressure control the method can be run with the set flow rate without the risk of method stop due to pressure alarm. Pressure control is enabled in the instruction System flow or Sample flow. Pressure control parameters provides the P and I factors used in the regulator and can be adjusted for different columns. Pressure control min flow rate can be set either as volumetric or as linear flow. A column type must be selected before using linear flow.
Constant pressure flow	Constant pressure flow enables column packing at constant pressure. The system pump automatically adjusts the flow rate within the specified Minimum allowed flow rate – Maximum allowed flow rate range. The goal is to reach and keep the set Pressure at the selected Pressure sensor using the P and I factors set in the Constant pressure flow parameters instruction. The total volume is continuously updated using the actual flow rate. Both pressure control flow rates can be set either as volumetric or as linear flow. A column type must be selected before using linear flow. Note: - When Constant pressure flow is used, the P and I factors set in the Constant pressure flow parameters instruction are used to control the pressure, instead of the P and I values set in the Pressure control parameters instruction. - Pressure sensor Delta column pressure is available only when column valve V9-C or V9H-C (5-columns) is selected in the component list.
Constant pressure flow parameters	Constant pressure flow parameters sets the values for the P and I factors needed to keep a constant pressure by varying the flow rate. The signal used for pressure control is set in the instruction Constant pressure flow.

Instruction name	Description
Column packing flow	Column packing flow is used to set flow rates over 25 ml/min and 150 ml/min for ÄKTA pure 25 and ÄKTA pure 150, respectively. Both A and B pumps are used to generate the flow, making it possible to set flow rates up to 50 ml/min and 300 ml/min for ÄKTA pure 25 and ÄKTA pure 150, respectively. Flow rate can be set either as volumetric or as linear flow. A column type must be selected before using linear flow. Before executing the Column packing flow instruction it is important to: - Immerse inlet tubing A1 and B1 in the same buffer - Disconnect the column outlet tubing from the Column valve and place the tubing in a waste vessel Note: <i>When running Column packing flow only isocratic runs can be performed, gradients cannot be generated.</i>
Delay volume: Monitor to outlet valve	Delay volume: Monitor to outlet valve is used to define the delay volume between the monitor and the Outlet valve. The instruction is used to make sure that the collected fractions correspond to the fractions indicated in the chromatogram. The delay volume must be changed when changing tubing to another i.d. or length or when removing or adding components.
Delay volume: Monitor to frac	Delay volume: Monitor to frac is used to define the delay volume between the monitor and the Fraction collector. The instruction is used to make sure that the collected fractions correspond to the fractions indicated in the chromatogram. The instruction is available only when the Fraction collector is selected in the component list.
Delay volume: Monitor to frac 2	Delay volume: Monitor to frac 2 is used to define the delay volume between the monitor and the second Fraction collector. The instruction is used to make sure that the collected fractions correspond to the fractions indicated in the chromatogram. The instruction is available only when the second Fraction collector is selected in the component list.
Start volume count	Start volume count starts the volume counter function. The counted volume is saved into a memory. This instruction is best used in combination with Watch instructions.

Instruction name	Description
Stop volume count	Stop volume count stops the volume counter function. The counted volume is stored in the memory and can be recalled with the instruction Hold counted volume. The counted volume can also be recalled in following runs and is stored until a new Stop volume count instruction is issued. This instruction is best used in combination with Watch instructions.
Hold counted volume	Hold counted volume sets the system to Hold. The system will remain in the state Hold until the accumulated volume reaches the volume stored by the instructions Start volume count / Stop volume count.
Method progressing flow	Method progressing flow defines the flow from which the volume base is calculated. When set to Automatic, the position of the injection valve determines if the system flow or the sample flow is used.

9.9.10 Manual instructions - Other

The table below describes the other manual instructions available for ÄKTA pure.

Instruction name	Description
Set mark	Set mark inserts a mark into the current chromatogram with the text entered for the parameter Mark text .
Timer	Timer sets the system to pause or end after a set volume or time has passed. Select base sets the base to either accumulated time or accumulated volume. Timeout sets the volume or time. Action sets the action to perform (pause or end)

9.10 Available Run data

The table below lists all available **Run data** for ÄKTA pure.

Run Data	Range/Unit	Description
System state	N/A	Status of connection and run.
Acc. Volume	ml	Total accumulated volume in the current method or manual run.
Block volume	ml	Accumulated volume in the current block (method run only).
Acc. Time	min	Total accumulated time in the current method or manual run.
Block time	min	Accumulated time in the current block (method run only).
Scouting no	N/A	The current scouting number in the scouting scheme.
System flow	0.001 – 50.000 ml/min (ÄKTA pure 25) 0.01 – 300.00 ml/min (ÄKTA pure 150)	The set flow rate of the system pumps.
System linear flow	cm/h	The set flow velocity of the system pumps. Only available if a column is selected.
Sample flow	0.001 – 50.000 ml/min (ÄKTA pure 25) 0.01 – 300.00 ml/min (ÄKTA pure 150)	The set flow rate of the sample pump.
Sample linear flow	cm/h	The set flow velocity of the sample pump. Only available if a column is selected.
Inlet A	A1 - A7	The set position of the inlet valve A.
Inlet B	B1 - B7	The set position of the inlet valve B.
Inlet S	S1 - S7, buff	The set position of the sample inlet valve.
Conc B	0.0 – 100.0 %B	The set concentration B or the current value during a gradient.
Mixer valve	N/A	The set position of the Mixer valve.
Injection	N/A	The set position of the Injection valve.
Loop position	N/A	The set position of the Loop valve.

Run Data	Range/Unit	Description
Column position	N/A	The set position of the Column valve.
Column flow direction	N/A	The set flow direction position of the Column valve V9-C , Column valve V9H-C , Column valve V9-Cs and V9H-Cs .
System pressure	-1.00 – 20.00 MPa (ÄKTA pure 25) -1.00 – 5.00 MPa (ÄKTA pure 150)	The system pressure signal (at the system pumps).
Sample pressure	-1.00 – 10.00 MPa (ÄKTA pure 25) -1.00 – 5.00 MPa (ÄKTA pure 150)	The sample pressure signal (at the sample pump).
PreC pressure	-1.00 – 20.00 MPa (ÄKTA pure 25) -1.00 – 5.00 MPa (ÄKTA pure 150)	The pre-column pressure signal.
DeltaC pressure	-1.00 – 20.00 MPa (ÄKTA pure 25) -1.00 – 5.00 MPa (ÄKTA pure 150)	The delta-column pressure signal.
PostC pressure	-1.00 – 20.00 MPa (ÄKTA pure 25) -1.00 – 5.00 MPa (ÄKTA pure 150)	The post-column pressure signal.
UV	-6000.000 – 6000.000 mAu	The UV absorbance signal of the U9-L monitor.
UV 1	-6000.000 – 6000.000 mAU	The first UV/Vis absorbance signal of the U9-M monitor.
UV 2	-6000.000 – 6000.000 mAU	The 2nd UV/Vis absorbance signal of the U9-M monitor.
UV 3	-6000.000 – 6000.000 mAU	The 3rd UV/Vis absorbance signal of the U9-M monitor.
UV 2nd	-6000.000 – 6000.000 mAU	The UV absorbance signal of the second U9-L monitor.
Cond	0.00 – 999.99 mS/cm	The conductivity signal.
% Cond	0.0 – 100.0 %	The conductivity signal as a percentage of a set range.

Run Data	Range/Unit	Description
Cond temp	0.0 – 99.0 °C	The temperature signal (in the conductivity flow cell).
pH	0.00 – 14.00	The pH signal.
pH valve	N/A	The set position of the pH valve.
Outlet	N/A	The set position of the outlet valve.
Frac position	N/A	The current tube position of the fraction collector.
Frac 2 position	N/A	The current tube position of the fraction collector 2.
Inlet valve X1	N/A	The set position of the X1 valve.
Inlet valve X2	N/A	The set position of the X2 valve.
Versatile valve	N/A	The set position of the versatile valve.
Versatile valve 2	N/A	The set position of the versatile valve 2.
Versatile valve 3	N/A	The set position of the versatile valve 3.
Versatile valve 4	N/A	The set position of the versatile valve 4.
Air inlet A	No air, Air	The current state of the air alarm for the integrated air sensor in inlet valve A.
Air inlet B	No air, Air	The current state of the air alarm for the integrated air sensor in inlet valve B.
Air inlet S	No air, Air	The current state of the air alarm for the integrated air sensor in inlet valve IS.
Ext. air sensor, to Ext. air sensor 4	No air, Air	The current state of the air alarm for the external air sensors.
Analog in 1, to Analog in 4	-2000.0 – 2000.0 mV	The I/O-box analog input signals.
Digital in 1, to Digital in 8	0, 1	The I/O-box digital input signals.
Digital out 1, to Digital out 8	0, 1	The set value of the I/O-box digital output signals.

9.11 Available Curves

The table below lists all available **Curves** for ÄKTA pure.

Curve	Range	Sampling frequency	Description
UV 1	-6000.000 – 6000.000 mAU	10 Hz	The first UV/Vis absorbance signal of the U9-M monitor.
UV 2	-6000.000 – 6000.000 mAU	2 Hz	The 2nd UV/Vis absorbance signal of the U9-M monitor.
UV 3	-6000.000 – 6000.000 mAU	2 Hz	The 3rd UV/Vis absorbance signal of the U9-M monitor.
Cond	0.00 – 999.99 mS/cm	5 Hz	The conductivity signal.
% Cond	0.0 – 100.0 %	1 Hz	The conductivity signal as a percentage of a set range.
Conc B	0.0 – 100.0 %	1 Hz	The set concentration B or the current value during a gradient.
System flow	0.001 – 50.000 ml/min (ÄKTA pure 25) 0.01 – 300.00 ml/min (ÄKTA pure 150)	1 Hz	The set flow rate of the system pumps.
System linear flow	cm/h	1 Hz	The set flow velocity of the system pumps. Only available if a column is selected.
Sample flow	0.001 – 50.000 ml/min (ÄKTA pure 25) 0.01 – 300.00 ml/min (ÄKTA pure 150)	1 Hz	The set flow rate of the sample pump.
Sample linear flow	cm/h	1 Hz	The set flow velocity of the sample pump. Only available if a column is selected.
PreC pressure	-1.00 – 20.00 MPa (ÄKTA pure 25) -1.00 – 5.00 MPa (ÄKTA pure 150)	1 Hz	The pre-column pressure signal.
DeltaC pressure	-1.00 – 20.00 MPa (ÄKTA pure 25) -1.00 – 5.00 MPa (ÄKTA pure 150)	1 Hz	The delta-column pressure signal.

Curve	Range	Sampling frequency	Description
pH	0.00 – 14.00	1 Hz	The pH signal.
UV	-6000.000 – 6000.000 mAU	10 Hz	The UV absorbance signal of the U9-L monitor.
UV 2nd	-6000.000 – 6000.000 mAU	10 Hz	The UV absorbance signal of the second U9-L monitor.
System pressure	-1.00 – 20.00 MPa (ÄKTA pure 25) -1.00 – 5.00 MPa (ÄKTA pure 150)	10 Hz	The system pressure signal (at the system pumps).
Sample pressure	-1.00 – 10.00 MPa (ÄKTA pure 25) -1.00 – 5.00 MPa (ÄKTA pure 150)	10 Hz	The sample pressure signal (at the sample pump).
PostC pressure	-1.00 – 20.00 MPa (ÄKTA pure 25) -1.00 – 5.00 MPa (ÄKTA pure 150)	1 Hz	The post-column pressure signal.
Cond temp	0.0 – 99.0 °C	0.5 Hz	The temperature signal (in the conductivity flow cell).
Analog in 1, to Analog in 4	-2000.0 – 2000.0 mV	10 Hz	The I/O-box analog input signals.
UV cell path length	0.2, 0.5 cm	1 Hz	The nominal cell path length of the U9-L monitor.
UV cell path length	0.05, 0.2, 1.0 cm	1 Hz	The nominal cell path length of the U9-M monitor.
UV cell path length 2nd	0.2, 0.5 cm	1 Hz	The nominal cell path length of the 2nd U9-L monitor.
Digital in 1, to Digital in 8	0, 1	10 Hz	The I/O-box digital input signals.
Digital out 1, to Digital out 8	0, 1	10 Hz	The I/O-box digital output signals.

9.12 Injection volumes and peak broadening

The width of peaks at the fraction collector is influenced by the following:

- the properties of the column,
- the dimensions of the tubing,
- the dimensions of the modules in the flow path, and
- fluid dynamics.

Initial sample volume affects the peak width in gel filtration (GF) chromatography and other isocratic techniques. A sample zone is broadened during passage through a GF column so that the sample is diluted and the resolution decreases with increasing sample volume. Sample volume does not however affect the resolution in adsorption chromatography techniques such as affinity chromatography (AC), ion exchange chromatography (IEX), and hydrophobic interaction chromatography (HIC) if the retention factor k is high.

The effect of peak broadening in the system from sample injection to peak detection (including dilution on the column) is apparent in the chromatogram from the UV monitor, but broadening from the UV monitor to fraction collection is not visible in the chromatogram. This "hidden" effect is more pronounced for smaller peak volumes.

Narrow and short tubing reduces peak broadening. However, narrow tubing also increases the back pressure. See for recommendations on tubing dimensions for prepacked columns.


9.13 Delay volumes

Introduction

A number of methods, both theoretical and experimental, exist for determining the delay volume of a system. The easiest and recommended method is to perform a theoretical determination. Delay volumes for standard configurations are listed in [Standard delay volumes, on page 494](#).

Explanation of delay volume

The delay volume is the volume between the detector and the fraction collector or outlet that is used. The illustration below shows an example of the delay volume between the UV/Vis monitor and the fraction collector.

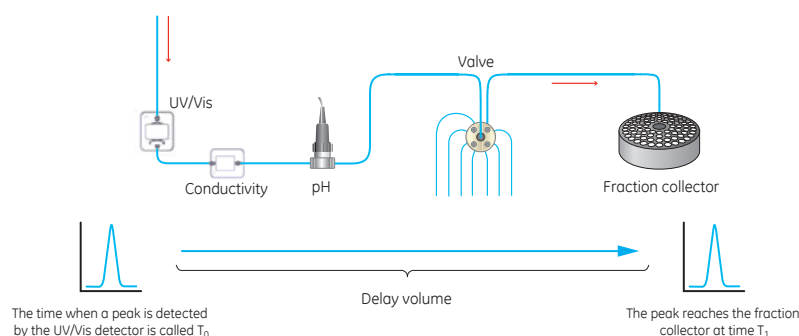

Theoretical determination of delay volumes

A theoretical determination is performed as described in the steps below:

Step	Action
1	Identify all components in the system flow path that contribute to the delay volume of interest.
2	Determine the internal volumes of all hardware modules and tubing, see Section 9.14 Component volumes, on page 497 for information about theoretical module volumes and Section 9.3 Tubing and connectors, on page 419 for information about tubing lengths and dimensions.
3	To obtain the total delay volume, sum up half of the flow cell volume of the monitor used (that is, the UV or UV/Vis monitor) with all volumes of tubing and modules that are located after the monitor in the flow path.

Note:


For pH-valve **V9-pH** and **V9H-pH** always use the volume for the valve in bypass position. The system automatically adds the volumes for the flow restrictor and the pH flow cell when if they are part of the system.

Set the delay volume in UNICORN

Follow the instructions below to set the delay volume between the UV monitor and the Outlet valve and between the UV monitor and the Fraction collector.

Step	Action
------	--------

- | | |
|---|---|
| 1 | Select System:Settings in the System Control module.
<i>Result:</i> The System Settings dialog opens. |
| 2 | <ul style="list-style-type: none"> Select Tubing and Delay Volumes and select Delay volume: Monitor to outlet valve. Type in the volume in the Volume field and click OK. |

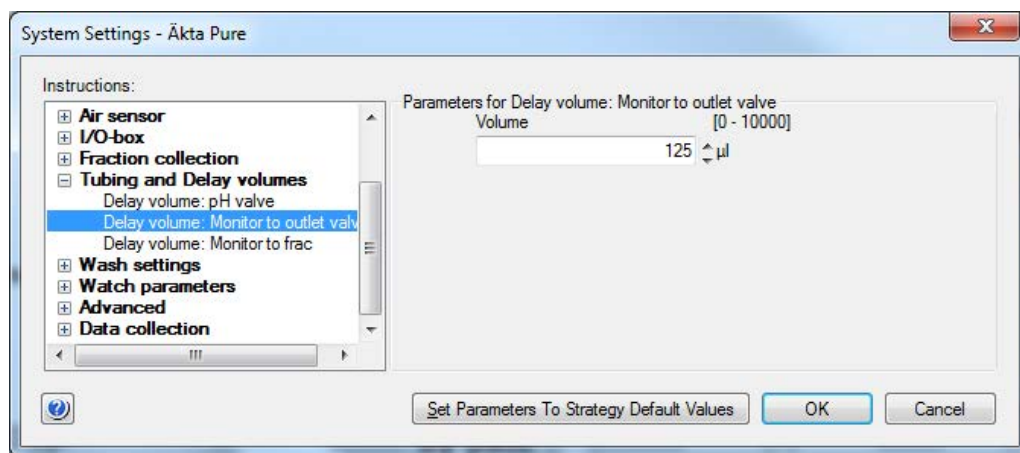

- | | |
|---|--|
| 3 | <p>In the System Settings dialog:</p> <ul style="list-style-type: none"> Select Delay volume: Monitor to outlet valve or Monitor to frac according to the configuration you are using. Type in the volume in the Volume field and click OK. |
|---|--|

Note:

*The system will use the delay volume appropriate to the configuration used and ignore other settings (e.g. the value for **Monitor to outlet valve** will be ignored if you are using a fraction collector). It is however recommended to set all delay volumes so that the volumes remain correct if you change fractionation method.*

Standard delay volumes

The table below lists the delay volumes for standard configurations using the available tubing kits with and without a pH valve and using tubing of standard length from the outlet valve to the fraction collector. The values are based on the flow cells for UV monitor **U9-M**. When using **U9-L**, add 9 µl for the 2 mm flow cell and 4 µl for the 5 mm flow cell. The values for delay volume Monitor to frac F9-C assume that the internal tubing of Fraction collector F9-C has the same inner diameter as the tubing kit.

Delay volumes ÄKTA pure 25

Tubing kit	pH valve V9-pH	Delay volume pH valve restrictor	Delay volume UV monitor to point of collection of eluent		
			Delay volume Monitor to outlet valve	Delay volume Monitor to frac F9-R	Delay volume Monitor to frac F9-C
0.25	No	N/A	66 µl	86 µl	214 µl
0.25	Yes	25 µl	77 µl	96 µl	225 µl
0.5 (standard)	No	N/A	125 µl	205 µl	435 µl
0.5 (standard)	Yes	48 µl	152 µl	231 µl	462 µl
0.75	No	N/A	223 µl	400 µl	803 µl
0.75	Yes	88 µl	277 µl	454 µl	857 µl
1.0	No	N/A	361 µl	675 µl	1319 µl
1.0	Yes	143 µl	452 µl	766 µl	1410 µl

Delay volumes ÄKTA pure 150

Tubing kit	pH valve V9H-pH	Delay volume pH valve restrictor	Delay volume UV monitor to point of collection of eluent		
			Delay volume Monitor to outlet valve	Delay volume Monitor to frac F9-R	Delay volume Monitor to frac F9-C
0.5	No	N/A	198 µl	278 µl	508 µl
0.5	Yes	60 µl	245 µl	324 µl	555 µl
0.75 (standard)	No	N/A	296 µl	473 µl	876 µl
0.75 (standard)	Yes	100 µl	370 µl	547 µl	950 µl
1.0	No	N/A	434 µl	748 µl	1392 µl
1.0	Yes	155 µl	545 µl	859 µl	1503 µl

- Note:**
- Always set the delay volume from the UV monitor to the point of collection of eluent. Depending on the system configuration, this will be **Delay volume: Monitor to outlet valve** or **Delay volume: Monitor to frac** in the system settings.
 - If the pH valve is mounted, make sure to set the value for the delay volume of the pH valve restrictor. The system automatically adds the volumes for the flow restrictor and the pH flow cell if they are part of the flow path.

Experimental method for determination of delay volumes

Delay volumes can be determined experimentally for Fraction collector F9-R, but not for Fraction collector F9-C. Instructions for measuring the delay volume using the UV monitor U9-M or UV monitor U9-L are provided below.

Two volumes are used to perform experimental delay volume measurements:

- V1: the volume between the Injection valve and the UV monitor used
- V2: the volume between the Injection valve and the fractionation collector tubing tip

The delay volume is then measured using the following procedure.

Step	Action
1	Check that a flow rate of 1 ml/min is delivered by the pump. Note: <i>If the flow rate is not correct, check if air bubbles may have entered the pump. Make sure to correct any problems before continuing.</i>
2	Fill a small sample loop, for example 20 µl, with a 1% to 5% acetone solution.
3	Set all components between the monitor and the fraction collector to by-pass mode.
4	Fill the system with water. Run the pump at a flow rate of 1 ml/min and inject the acetone solution as a sample.
5	Note the volume from the point of injection to the maximum of the peak in the chromatogram. This volume is volume measurement V1.
6	Reconfigure the system as follows to include the fraction collector in the flow path before the monitor: • Disconnect the two tubing segments from the UV monitor flow cell and connect these with a low-dead-volume connector, a 1/16" female to a 1/16" female union connector. • Mount the fractionation collector tubing tip on the top of the UV monitor flow cell. Connect tubing to the bottom of the UV monitor flow cell and lead this tubing to waste. It is preferable if the waste tubing gives some back pressure as the flow restrictor now is placed before the UV flow cell.
7	Set the Frac size to a large volume, for example 100 ml, so that the Outlet valve is in the Frac position during the entire run.

Step	Action
8	Start the pump at a flow rate of 1 ml/min and inject the acetone solution.
9	Note the volume from the point of injection to the appearance of the peak in the chromatogram. This volume is volume measurement V2.
10	To obtain the delay volume: • Subtract V1 from V2 and • add half of the volume of the UV flow cell.

Use of different monitors for peak fractionation in the same method

If different monitors or detectors are used for peak fractionation in different parts of the same method, the delay volumes have to be set as method instructions for each of the method parts. For example, both an external fluorescence detector and the UV monitor module can be used for peak fractionation.

9.14 Component volumes

The table below shows the component volumes of ÄKTA pure.

Component	Volume (µl)
Inlet valve V9-IA, V9-IB	88
Inlet valve V9H-IA, V9H-IB	212
Inlet valve V9-IAB	95
Inlet valve V9H-IAB	116
Sample inlet valve V9-IS	88
Sample inlet valve V9H-IS	212
Inlet valve V9-IX	88
Inlet valve V9H-IX	212
Air sensor L9-1.2	20
Air sensor L9-1.5	35
Pump P9 (P9-A , and P9-B) (total volume for two heads including T-connector and check valves)	549
Pump P9H (P9H A , P9H B , P9H S) (total volume for two heads including T-connector and check valves)	2163
System pump pressure monitor R9	45
Sample pump pressure monitor R9	45
Sample pump S9	1392
Mixer, 0.6 ml	600
Mixer, 1.4 ml	1400
Mixer, 5 ml	5000
Mixer, 15 ml	15000
Mixer valve V9-M	14
Mixer valve V9H-M	31
Loop valve V9-L	17
Loop valve V9H-L	76
Versatile valve V9-V	14
Versatile valve V9H-V	31
Injection valve V9-Inj	10

Component	Volume (µl)
Injection valve V9H-Inj	23
Column valve V9-C	110
Column valve V9H-C	190
Column valve V9-Cs	14
Column valve V9H-Cs	31
UV monitor U9-M : Flow cell 0.5 mm	10
UV monitor U9-M : Flow cell 2 mm	11
UV monitor U9-M : Flow cell 10 mm	12
UV monitor U9-L : Flow cell 2 mm	30
UV monitor U9-L : Flow cell 5 mm	15
Conductivity cell	22
Flow restrictor FR-902	10
pH valve V9-pH , in <i>By-pass</i> position	15
pH valve V9H-pH , in <i>By-pass</i> position	35
pH flow cell	76
Flow restrictor FR-902 and tubing when mounted on pH valve V9-pH	48
Outlet valve V9-O	9
Outlet valve V9H-O	82
Outlet valve V9-Os	9
Outlet valve V9H-Os	28
Fraction collector F9-C internal tubing (0.5 mm i.d.)	147
Fraction collector F9-C Dispenser head	94

Note: The given values for the component volumes of the valves are average values. Depending on the chosen flow path the actual component volume may differ somewhat.

9.15 Pressure control

Introduction

By using the function **Pressure control** to regulate the run, the method can be run with the set flow rate without the risk of method stop due to pressure alarm. If the pressure approaches the pressure limit, for example if the sample has higher viscosity than the buffer, the flow rate is automatically lowered. Pressure control is enabled in the manual instructions **Pumps:System flow** or **Pumps:Sample flow**. The default setting for Pressure Control is **Off**. To enable the function, set what pressure signal to use. It is recommended to use the pre-column pressure. The instruction **Advanced:Pressure control parameters** provides the P and I factors used in the regulator and can be adjusted for different columns, see information further down.

In the Method editor, pressure control is enabled by selecting **Control the flow to avoid overpressure** in the predefined phase **Method settings**.

Pressure control parameters

The table below describes the factors used for pressure regulation.

Parameter	Description
P factor	Proportional component in PI pressure regulation. Reduces the error between actual and requested target pressure, but may leave a permanent error.
I factor	Integrating component in PI pressure regulation. Eliminates the stationary error from the P factor, but introduces a slight instability that may lead to oscillation in the pressure and the actual flow rate. Set I = 0 to disable the I factor. As a general guide use a small I factor for high pressure columns and a large I factor for low pressure columns, see p. 500 for more recommendations.
Target value for pressure control	Sets the target value for the PI pressure regulation as a percentage of the pressure limit. If the target pressure is too close to the pressure limit there is a risk that a short pressure spike will trigger the pressure alarm. The pressure limit is set in the Alarm pressure instruction. The Alarm pressure used for pressure control depends on the settings in the System flow instruction.
Pressure control min flow rate	If the flow rate is reduced below the value set in Pressure control min flow rate , the method is paused and the system is set to state ALARMS AND ERRORS . Pressure control min flow rate can be set either as volumetric or as linear flow. A column type must be selected before using linear flow.

Recommended pressure control parameters

The table below contains the recommended values for P and I parameters for different media types.

Column/Media	Recommend- ed P factor	Recommended I factor	Additional information
Default	8	40	N/A
Small soft media columns	8	40	N/A
Large soft ¹ media columns	8	300 - 600	A higher I value than the default value is needed to speed up pressure ramp-up times.
Small rigid ² media columns	8	15	A lower I value than the default value is needed to avoid large fluctuations in pressure or flow rate. As an alternative, try increasing P.
	20	40	

¹ Soft media is defined as all GE separation media, except silica and MonoBeads.

² Rigid media is defined as GE separation media that is based on silica and MonoBeads.

Back pressure

Using narrow tubing between components will improve resolution but will lead to increased back pressure in the system. Narrow tubing after the column will increase the pressure in the column at a given flow rate. Make sure that the pressure sensor limits in the system are set so that the maximum pressure for the column used is not exceeded.

Additional instructions for avoiding pressure alarms

The instruction **Max flow during valve turn** sets the maximum flow rate used during the turning of the Injection valve and Outlet valve in order to avoid high pressure alarms. If the flow rate passing through the Injection valve or the Outlet valve is higher than the set max flow rate, the valves will only turn after decreasing the flow to the specified flow rate. After the valves have turned, the previous flow rate will be restored. The instruction is found in **System Control: System settings: Advanced**.

9.16 Node IDs

Node ID for core modules

The table below lists the Node ID for the core modules.

Core module	Label	Node ID
System pump A	P9 A / P9H A	0
System pump B	P9 B / P9H B	1
Pressure monitor	R9	0
Mixer	M9	0
Injection valve	V9-Inj / V9H-Inj	4

Node ID for optional modules

The table below lists the Node ID for the optional modules.

Note: The Node IDs of Sample pump S9 and Fraction collector F9-C cannot be changed by the user.

Note: The Node IDs for UV monitor U9-M and UV monitor U9-D should only be changed by service personnel.

Module	Label	Node ID
Inlet valve A	V9-IA / V9H-IA	0
Inlet valve B	V9-IB / V9H-IB	1
Inlet valve AB	V9-IAB / V9H-IAB	3
Inlet valve X1	V9-IX / V9H-IX	15
Inlet valve X2	V9-IX / V9H-IX	16
Mixer valve	V9-M / V9H-M	22
Sample inlet valve	V9-IS / V9H-IS	2
Loop valve	V9-L / V9H-L	17
Column valve (5-columns)	V9-C / V9H-C	5
Pre-column pressure monitor	N/A	2
Post-column pressure monitor	N/A	3
Column valve (1-column)	V9-Cs / V9H-Cs	7
pH valve	V9-pH / V9H-pH	11
Outlet valve (10-outlets)	V9-O / V9H-O	8

Module	Label	Node ID
Outlet valve (1-outlet)	V9-Os / V9H-Os	19
Versatile valve	V9-V / V9H-V	20
Versatile valve 2	V9-V / V9H-V	21
Versatile valve 3	V9-V / V9H-V	23
Versatile valve 4	V9-V / V9H-V	24
UV monitor (fixed)	U9-L	0
UV monitor 2nd	U9-L	1
UV monitor (variable)	U9-M	0
UV detector	U9-D	0
Conductivity monitor	C9	0
External air sensor	L9	0
External air sensor 2	L9	1
External air sensor 3	L9	2
External air sensor 4	L9	3
Fraction collector (cassettes)	F9-C	0
Fraction collector (round)	F9-R	0
Fraction collector (round), 2nd	F9-R	1
Sample pump	P9-S / P9H S	2
I/O-box	E9	0
I/O-box, 2nd	E9	1

10 Ordering information

Introduction

This chapter lists accessories and user replaceable spare parts available for ÄKTA pure.

Mixer

Item	Code no.
Mixer chamber 0.6 ml	28-9561-86
Mixer chamber 1.4 ml (mounted at delivery)	28-9562-25
Mixer chamber 5 ml (included with ÄKTA pure 150)	28-9562-46
Mixer chamber 15 ml	28-9803-09
O-ring 13.1 × 1.6 mm Note: <i>For Mixer chamber 0.6, 1.4, and 5 ml.</i>	28-9535-45
O-ring 13.1 × 1.6 mm (highly resistant) (can be used as an alternative to 28-9535-45)	29-0113-26
O-ring 22.1 × 1.6 mm Note: <i>For Mixer chamber 15 ml.</i>	28-9818-57
Online filter kit	18-1027-11

Tubing

Item	Code no.
Reference capillary 1	28-9507-49
Reference capillary 2	28-9507-50
Tubing Kit 0.5 mm standard, ÄKTA pure 25	29-0113-27
Tubing Kit 0.5 mm, ÄKTA pure 150	29-0516-69
Tubing Kit 0.25 mm, ÄKTA pure 25	29-0113-28
Tubing Kit 0.75 mm, ÄKTA pure 25	29-0113-29
Tubing Kit 0.75 mm standard, ÄKTA pure 150	29-0482-42

Item	Code no.
Tubing Kit 1.0 mm	29-0345-51
Tubing kit 10×1.0 m, ETFE ID 1.0 mm OD 1/16	28-9809-95
Tubing kit for sample inlet valve V9-IS (7-ports)	29-0353-31
Tubing kit for sample inlet valve V9H-IS (7-ports)	29-0511-66
Sample tubing kit for 7 inlets, i.d. 0.75 mm	28-9572-17
Inlet tubing kit 2+2	29-0113-30
V9-pH tubing kit	29-0113-31
V9H-pH tubing kit standard	29-0516-74
Tubing kit for inlet valve V9-IA (7 ports)	29-0113-32
Tubing kit for inlet valve V9H-IA (7 ports)	29-0511-97
Tubing kit for inlet valve V9-IB (7 ports)	29-0113-33
Tubing kit for inlet valve V9H-IB (7 ports)	29-0511-89
Outlet tubing kit, ÄKTA pure 25	29-0113-34
Outlet tubing kit, ÄKTA pure 150	29-0486-11
Rinse system tubing	29-0113-48
Union 1/16 male/male, i.d. 0.5 mm (5-pack)	28-9543-26
Tubing cutter	18-1112-46
Inlet filter holder kit	11-0004-07
Inlet filter set	11-0004-14

Holders

Item	Code no.
Adapter for air sensor	28-9563-42
Bottle holder	28-9563-27
Column clamp o.d. 10–21 mm	28-9563-19
Column holder	28-9562-82
Column holder rod	28-9562-70
Flexible column holder	28-9562-95
Loop holder	29-0113-50

Item	Code no.
Multi-purpose holder	29-0113-49
Rail extension	29-0113-52
Tube holder (5-pack)	28-9543-29
Tubing holder comb	28-9562-86
Tubing holder spool	28-9562-74
Inlet filter holder kit	11-0004-07
Screw lid GL45 kit	11-0004-10

UV monitor

Item	Code no.
UV monitor U9-L (Fixed wavelength)	29-0113-60
UV flow cell U9-0.5 0.5 mm for U9-M	28-9793-86
UV flow cell U9-2 2 mm for U9-M	28-9793-80
UV flow cell U9-10 10 mm for U9-M	28-9563-78
UV flow cell 2 mm for U9-L	29-0113-25
UV flow cell 5 mm for U9-L	18-1128-24

I/O box

Item	Code no.
I/O box E9	29-0113-61

Fraction collector F9-C

Item	Code no.
Fraction collector F9-C	29-0277-43
Tubing kit for F9-C	29-0336-32
Cassette tray	28-9542-09
Cassette, for deep-well plate (2-pack)	28-9542-12
Deep well plate, 96 x 2 ml	7701-5200

Item	Code no.
Deep well plate, 48 x 5 ml	7701-5500
Deep well plate, 24 x 10 ml	7701-5102
Cassette, for 50 ml tubes (2-pack)	28-9564-02
Cassette, for 3 ml tubes (2-pack)	28-9564-27
Cassette, for 8 ml tubes (2-pack)	28-9564-25
Cassette, for 15 ml tubes (2-pack)	28-9564-04
Rack, for 50 ml tubes	28-9803-19
Rack, for 250 ml bottles	28-9818-73
Cable 2.5 m, UniNet-9 D-type	29-0324-25

Fraction collector F9-R

Item	Code no.
Fraction collector F9-R	29-0113-62
Tube Rack Complete, 175 x 12 mm	19-8684-03
Tube Rack Complete, 95 x 10-18 mm	18-3050-03
Tube Rack Complete, 40 x 30 mm	18-1124-67
Bowl	18-3051-03
Tube support	18-3054-02
Tube holder	18-6464-01
Tube rack upgrade kit, 175 x 12 mm	19-7242-02
Tube rack upgrade kit, 95 x 18 mm	19-8689-02
Tube rack upgrade kit, 40 x 30 mm	18-1124-68
Drive sleeve	19-6067-02

Valves

Item	Code no.
Column valve kit V9-C	29-0113-67
Column valve kit V9H-C	29-0509-51
Column valve V9-Cs	29-0113-55
Column valve V9H-Cs	29-0906-93
Inlet valve V9-X1	28-9572-27
Inlet valve V9H-X1	28-9793-26
Inlet valve V9-X2	28-9572-34
Inlet valve V9H-X2	28-9793-28
Inlet valve kit V9-IA	29-0122-63
Inlet valve kit V9H-IA	29-0509-45
Inlet valve kit V9-IB	29-0123-70
Inlet valve kit V9H-IB	29-0509-46
Inlet valve kit V9-IAB	29-0113-57

Item	Code no.
Inlet valve kit V9H-IAB	29-0896-52
Sample inlet valve kit V9-IS	29-0277-46
Sample inlet valve kit V9H-IS	29-0509-43
Loop valve kit V9-L	29-0113-58
Loop valve kit V9H-L	29-0906-89
Mixer valve kit V9-M	29-0113-54
Mixer valve kit V9H-M	29-0906-92
Outlet valve kit V9-O	29-0122-61
Outlet valve kit V9H-O	29-0509-49
Outlet valve kit V9-Os (1 outlet)	29-0113-56
Outlet valve kit V9H-Os (1 outlet)	29-0906-94
pH valve kit V9-pH	29-0113-59
pH valve kit V9H-pH	29-0516-84
Versatile valve V9-V	29-0113-53
Versatile valve V9H-V	29-0906-91

Note: All valve kits include the necessary tubing.

Injection valve accessories

Item	Code no.
Sample loop 10 µl	18-1120-39
Sample loop 100 µl	18-1113-98
Sample loop 500 µl (mounted at delivery)	18-1113-99
Sample loop 1 ml	18-1114-01
Sample loop 2 ml	18-1114-02
Sample loop 10 ml	18-1161-24
Superloop 10 ml	19-7585-01
Superloop 50 ml	18-1113-82
Superloop 150 ml	18-1023-85
Fill port	18-1127-66

Item	Code no.
Injection kit	18-1110-89
Connector 1/16" male and Luer female	28-9858-12

External air sensors

Item	Code no.
Air sensor L9-1.2 mm	28-9565-02
Air sensor L9-1.5 mm	28-9565-00

pH monitor

Item	Code no.
pH electrode	28-9542-15
O-ring 5.3 × 2.4 mm	28-9564-97

Conductivity monitor

Item	Code no.
Conductivity monitor C9	29-0113-63

Flow restrictor

Item	Code no.
Flow restrictor FR-902	18-1121-35

Module components

Item	Code no.
Module Panel	29-0113-64
Multi-module front	29-0113-51
Extension box	29-1108-06

Cables

Item	Code no.
Jumper 1 IEC 1394 (F-type)	28-9564-89
Jumper D-SUB (D-type)	29-0113-65
External module cable, short (F-type)	29-0124-74
External module cable, long (F-type)	29-0113-66
Cable 2.5 m UniNet-9 D-type	29-0324-25

System Pumps and Sample pump S9H

Item	Code no.
P9 Seal kit 25 ml	28-9526-42
P9 Piston kit 25 ml	28-9526-40
P9H Seal kit 150 ml	28-9793-73
P9H Piston kit 150 ml	28-9793-68
Check valve kit	28-9793-64
Sample pump S9H	29-0505-93

Sample Pump S9

Item	Code no.
Sample pump S9	29-0277-45
P9-S Seal kit	28-9602-50
P9-S Piston kit	18-1112-13
Check valve kit	28-9793-64
Cable 2.5 m UniNet-9 D-type	29-0324-25

UNICORN

There are different UNICORN products and licenses available for different purposes, for example licenses for use with a workstation or for working remotely. Contact your local GE salesperson for more information on UNICORN products and licenses and how to order.

Index

A

Affinity chromatography
predefined method, 437–438

Air sensors

air sensor adapter, 83

A test, 225

B test, 227, 229

error codes, 402

external air sensors, 87

inlet valves, 40

troubleshooting, 395

ÄKTA pure

Cassettes and trays, 96

description, 13, 86

illustrations, 14

main features, 9

maintenance, 248

overview, 9

preparation, 191

troubleshooting, 353

Anion exchange

predefined method, 439

C

Cabinet

troubleshooting, 393

Cassettes, 96

quickrelease function, 98

Cation exchange

predefined method, 439

Chromatofocusing

predefined method, 439

CIP

column CIP, 281

column maintenance method, 443

column predefined phase, 446

system CIP, 275

system maintenance method, 444

system predefined phase, 213, 446

Cleaning

column, 219

system, 218

Column

attach column holder, 170

cleaning, 219

column CIP, 281

column holder, 80

column valve, 55

connect column, 170

pressure alarm, 174

storage, 219

Column CIP

maintenance method, 443

predefined phase, 446

Column performance test

maintenance method, 443

predefined phase, 213, 446

Column preparation

maintenance method, 443

predefined phase, 446

Column valve

description, 55

flow paths V9-C, 56

flow paths V9-Cs, 57

V9-C test, 231

Column wash

predefined phase, 446

Component volumes, 497

Conductivity monitor

calibration, 305

clean the conductivity flow cell, 297

description, 72

error codes, 402

troubleshooting, 364

Connectors

for ÄKTA pure, 420

replace connectors, 314

D

Delay volume

reference information, 492

settings, 205

Delta column pressure

description, 68

Desalting

predefined method, 440

Documentation, 11–12

E

Elution

predefined phase, 446

Equilibration

predefined phase, 446

Extension box, 85

F

Flow cells

- conductivity, 72
- pH, 60
- UV, U9-L, 70
- UV, U9-M, 69

Flow path

- component volumes, 497
- illustration, 25, 148, 421
- prepare, 148
- specifications, 25

Flow restrictor

- check function, 266
- FR-902 description, 74
- replace flow restrictor, 327

Fractionation

- assemble tube rack, 105, 197
- delay volume, 205
- fractionation types, 204
- prepare, 197

Fraction collector

- cleaning, 264, 285, 287
- description, 90
- error codes F9-R, 405
- F9-R test, 233, 236, 238
- function, 90
- preparation, 197
- quickrelease function, 98
- replace internal tubing, 316
- specifications, 417
- troubleshooting, 374, 382

Fraction collector F9-C

- Cassettes and racks, 96
- connect tubing, 102
- requirements on deep well plates, 100
- requirements on tubes, 99
- Tubes, 105

G

Gel filtration

- predefined method, 440

H

Hardware installation

- of a module, 76

Holders

- air sensor adapter, 83
- bottle holder, 83
- column clamp, 81
- column holder, 80
- column holder rod, 81

Extension box, 85

- flexible column holder, 82
- loop holder, 80
- multi-purpose holder, 79
- ordering information, 505
- rail extension, 79
- tubing holder comb, 83
- tubing holder spool, 82

Hydrophobic interaction chromatography (HIC)

- predefined method, 440

I

I/O-box E9

- connectors, 113
- description, 112
- error codes, 406
- Fraction collector F9-C installation, 112
- specifications, 418
- troubleshooting, 396

Injection valve

- description, 49
- flow paths, 49

Inlet tubing

- prepare, 150
- prime inlet tubing B, 159

inlet valves

- V9-IA test, 225
- V9-IB test, 227, 229

Inlet valves

- air sensors, 40
- description, 39
- inlet valve A, 39
- inlet valve AB, 39
- inlet valve B, 39
- inlet valve X1, 39
- inlet valve X2, 39
- troubleshooting, 373

Installation

- prepare waste tubing, 152

Instrument control panel

- error codes, 406
- function, 27
- location, 27
- status indications, 29
- troubleshooting, 397

Instrument control unit

- error codes, 401

Instrument overview

- Fraction collector F9-R, 103

- Instrument configurations, 14
- main parts, 14
- modules, 16
- wet side, 15
- Intelligent Packing
 - Predefined method, 443
- Ion exchange
 - predefined method, 439

L

- Log on
 - UNICORN, 155
- Loop valve
 - description, 52
 - flow paths, 52

M

- Maintenance
 - calibration procedures, 299
 - clean the instrument, 274
 - Maintenance Manager, 249
 - maintenance program, 255
 - maintenance when required, 273
 - replacement procedures, 313
 - semiannual maintenance, 269
 - weekly maintenance, 258
- Maintenance manager
 - handling maintenance notifications, 251
- Maintenance methods
 - column CIP, 443
 - column performance test, 443
 - column preparation, 443
 - system CIP, 444
 - system preparation, 444
- Manual instructions, 464
- Manual loop fill
 - predefined phase, 446
- Manual Loop Fill
 - predefined method, 440
- Methods
 - affinity chromatography, 437–438
 - anion exchange, 439
 - cation exchange, 439
 - chromatofocusing, 439
 - create method, 209
 - desalting, 440
 - gel filtration, 440
 - hydrophobic interaction chromatography (HIC), 440
 - Intelligent Packing, 443
 - maintenance methods, 209

- manual loop fill, 440
- NHS-coupling, 441
- predefined maintenance methods, 443
- predefined methods, 209, 437
- purification methods, 209
- reverse phase chromatography (RPC), 442
- Method settings
 - predefined phase, 445
- Miscellaneous
 - predefined phase, 446
- Mixer
 - choose mixer chamber, 149
 - description, 37
 - error codes, 402
 - mixer valve, 46
 - replace mixer, 319
 - replace the inline filter, 263
 - replace the o-ring, 320
 - specifications, 413
 - troubleshooting, 392
- Mixer valve
 - description, 46
 - flow paths, 46, 48
- Module panel
 - description, 84
 - troubleshooting, 373
- Module Panel Assembly, 122
- Modules
 - column valve, 55
 - conductivity monitor, 72
 - flow restrictor, 74
 - injection valve, 49
 - inlet valves, 39
 - loop valve, 52
 - mixer, 37
 - mixer valve, 46
 - outlet valve, 64
 - pH valve, 60
 - pressure monitor, 67
 - pumps, 33, 107
 - recommended positions, 122
 - UV monitor, 69
 - versatile valve, 59
- Monitors
 - conductivity, 72
 - external air sensors, 87
 - pH, 62
 - pressure monitor, 67
 - specifications, 415

- troubleshooting, 357
- UV, 69
- N**
- NHS-coupling
 - predefined method, 441
- Node ID
 - description, 76
 - list, 501
- O**
- Optional configurations
 - install optional modules, 76
- Ordering information
 - cables, 510
 - conductivity monitor, 509
 - dummy module, 509
 - external air sensors, 509
 - flow restrictor, 509
 - fraction collector, 507
 - holders, 505
 - I/O-box E9, 505
 - mixer, 503
 - pH monitor, 509
 - pump, 510
 - tubing, 504
 - UV monitor, 505–506, 509
 - valves, 508
- Outlet tubing
 - prepare, 151
- Outlet valve
 - description, 64
 - V9-O ports, 64
 - V9-Os ports, 65
- P**
- Performance tests
 - air sensor A and inlet valve V9-IA, 225
 - air sensor B and inlet valve V9-IB, 227, 229
 - column valve V9-C, 231
 - fraction collector F9-R, 233, 236, 238
 - overview, 222
 - UV U9-L system, 240
 - UV U9-M system, 244
- Phases
 - column CIP, 446
 - column performance test, 213, 446
 - column preparation, 446
 - column wash, 446
 - elution, 446
 - equilibration, 446
 - manual loop fill, 446
 - method settings, 445
 - miscellaneous, 446
 - predefined phases, 445
 - sample application, 446
 - system CIP, 213, 446
 - system preparation, 446
- pH monitor
 - calibration, 300
 - clean the pH electrode, 290
 - description, 62
 - error codes, 402
 - replace the pH electrode, 272
 - storage of the pH electrode, 219, 288
 - troubleshooting, 367
- pH valve
 - description, 60
 - flow paths, 61
 - troubleshooting, 367, 373
- Power and ICU
 - troubleshooting, 393
- Power save, 144
- Prepare the system
 - ÅKTA pure, 191
 - connect column, 170
 - flow path, 148
 - fraction collector, 197
 - inlet tubing, 150
 - mixer, 149
 - outlet tubing, 151
 - sample application, 177
 - Start UNICORN, 155
 - UV monitor U9-L, 150
 - UV monitor U9-M, 150
 - waste tubing, 152
- Pressure alarm
 - set, 174
- Pressure control
 - system configuration, 217
- Pressure monitor
 - error codes, 401
- Pressure monitors
 - calibration, 302
 - check the pressure monitors, 302
 - description, 67
 - troubleshooting, 369
- Prime inlet tubing B, 159
- Process picture
 - actions in the process picture, 217
- Pump piston rinsing system
 - flow path, 35

illustration, 35, 109, 259, 261, 349–350
prime, 260, 262

Pumps

change pump rinsing solution, 259
clean check valves, 293
description, 33
description, sample pump, 107
error codes, 403
purge sample pump, 165
purge system pumps, 159
replace check valves, 329
replace pump pistons, 348
replace pump piston seals of pump P9, 332
replace pump piston seals of Pump P9-S, 341
replace pump rinsing system tubing, 349
specifications, 411
troubleshooting, 384

Q

QuickRelease function, 98

R

reference information

injection volumes and peak broadening, 491

Reference information, 407

back pressure, 500
chemical resistance guide, 430
delay volumes, 492
module specifications, 411
pressure regulation, 499
system specifications, 408

Reverse phase chromatography (RPC)

predefined method, 442

Run

after run procedures, 218
available curves, 489
available run data, 486
choose method, 214
monitor run, 216
perform manual run, 215
perform run, 214
prepare run, 214

S

Sample application

flow paths, 49
injection valve, 49
predefined phase, 446

sample loading, 177

sample loop, 187

superloop, 180

Sample loop

sample loading, 187

Sample pump

description, 107

Software overview

software modules, 10

Storage

column, 219

pH electrode, 219

system, 219

Superloop

sample loading, 180

troubleshooting, 393

System CIP

maintenance method, 444

predefined phase, 213, 446

System cleaning, 218

System configuration

control pressure, 217

installation of modules, 76

modules and positions, 122

overview, 122

system properties, 125

system settings, 127

System Control module

manual instructions, 464

System preparation

before preparation, 147

maintenance method, 444

predefined phase, 446

System pumps

operating ranges, 33

System storage, 219

System test

UV U9-L, 240

UV U9-M, 244

T

Technical specifications

module specifications, 411

Trays, 96

Troubleshooting

error codes, 401

fraction collector, 374

Fraction collector, 382

instrument communication, 398

monitors, 357

other components, 391

- pumps, 384
- Tube rack
 - assembly, 105, 197
- Tubing
 - for ÄKTA pure, 419
 - replace tubing, 314, 316

U

- UNICORN
 - connect to system, 156
 - Log on, 155
 - Start, 155
- User information, 7
- UV detector U9-D
 - error codes, 403
- UV monitor
 - calibration, 150, 309
 - clean UV flow cell, 270
 - description, 69
 - installing two monitors, 137
 - replace UV flow cell, 322, 325
- UV monitor U9-L
 - description, 70, 150
 - error codes, 404
 - replace the flow cell, 325
 - system test, 240
 - troubleshooting, 361

- UV monitor U9-M
 - description, 69, 150
 - error codes, 403
 - system test, 244
 - troubleshooting, 357

V

- Valves
 - column valve, 55
 - error codes, 401
 - extra inlet valves, 39
 - injection valve, 49
 - inlet valves, 39
 - loop valve, 52
 - mixer valve, 46
 - outlet valve, 64
 - overview, 38
 - pH valve, 60
 - specifications, 412
 - versatile valve, 59
- Versatile valve
 - description, 59
 - flow paths, 59

W

- Waste tubing, 152
 - prepare, 152

For local office contact information, visit
www.gelifesciences.com/contact

GE Healthcare Bio-Sciences AB
Björkgatan 30
751 84 Uppsala
Sweden
www.gelifesciences.com/AKTA

GE and GE monogram are trademarks of General Electric Company.

ÄKTA, UNICORN, HiLoad, HiPrep, HiScreen, HiTrap, HisTrap, GSTrap, StrepTrap, Mini Q, Mini S, Mono Q, Mono S, Mono P, RESOURCE, Sephacryl, Sepharose, SOURCE, Superdex, Superloop, Superose, and Whatman are trademarks of General Electric Company or one of its subsidiaries.

Decon is a trademark of Decon Laboratories, Limited.

Elgiloy is a trademark of Elgiloy Limited Partnership.

Eppendorf is a trademark of Eppendorf AG.

Hostelloy is a trademark of Haynes International Inc.

Kautex is a trademark of Kautex Textron GmbH & Co. KG.

Nalgene is a trademark of Thermo Fisher Scientific Inc.

Seahorse Bioscience is a trademark of Seahorse Bioscience Corporation.

Triton is a trademark of Union Carbide Chemicals and Plastic Company Inc.

Tween is a trademark of Uniqema Americas LLC.

Microsoft and Windows are registered trademarks of Microsoft Corporation.

All other third party trademarks are the property of their respective owner.

Any use of UNICORN is subject to GE Healthcare Standard Software End-User License Agreement for Life Sciences Software Products. A copy of this Standard Software End-User License Agreement is available on request.

© 2012-2014 General Electric Company – All rights reserved.

First published Sep. 2012

All goods and services are sold subject to the terms and conditions of sale of the company within GE Healthcare which supplies them. A copy of these terms and conditions is available on request. Contact your local GE Healthcare representative for the most current information.

GE Healthcare Europe GmbH
Munzinger Strasse 5, D-79111 Freiburg, Germany

GE Healthcare UK Limited
Amersham Place, Little Chalfont, Buckinghamshire, HP7 9NA, UK

GE Healthcare Bio-Sciences Corp.
800 Centennial Avenue, P.O. Box 1327, Piscataway, NJ 08855-1327, USA

GE Healthcare Japan Corporation
Sanken Bldg. 3-25-1, Hyakunincho Shinjuku-ku, Tokyo 169-0073, Japan

